

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061317\
 Data File : BF095916.D
 Acq On : 14 Jun 2017 3:16
 Operator : SJ/MA
 Sample : I3635-13 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CL-02-061217-E

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.281	624	628	647	rBV	47273	160266	32.07%	3.742%
2	6.957	910	913	922	rBV	51479	136380	27.29%	3.184%
3	7.028	922	925	945	rVB	125517	295023	59.04%	6.888%
4	7.351	976	980	1000	rVB	291900	390191	78.09%	9.109%
5	7.586	1016	1020	1035	rBV	125563	191467	38.32%	4.470%
6	8.286	1135	1139	1163	rBV	38297	111894	22.39%	2.612%
7	9.380	1321	1325	1344	rBV	353680	499670	100.00%	11.665%
8	11.163	1623	1628	1638	rBV	191105	255124	51.06%	5.956%
9	11.869	1744	1748	1758	rBV	9863	15385	3.08%	0.359%
10	12.204	1800	1805	1820	rBV2	363624	472892	94.64%	11.040%
11	13.515	2024	2028	2038	rBV	49279	81736	16.36%	1.908%
12	14.598	2208	2212	2218	rBV	305294	405216	81.10%	9.460%
13	15.615	2381	2385	2390	rVB5	4094	7056	1.41%	0.165%
14	16.345	2504	2509	2515	rBV3	5839	11936	2.39%	0.279%
15	16.427	2515	2523	2529	rVV	40336	55727	11.15%	1.301%
16	16.727	2570	2574	2579	rBV	45900	53207	10.65%	1.242%
17	16.974	2612	2616	2621	rBV	193101	217728	43.57%	5.083%
18	17.286	2662	2669	2674	rBV6	4610	6853	1.37%	0.160%
19	17.339	2674	2678	2683	rBV6	4996	9081	1.82%	0.212%
20	17.445	2693	2696	2699	rBV3	4990	6022	1.21%	0.141%
21	18.027	2793	2795	2799	rBV5	4162	5620	1.12%	0.131%
22	18.174	2818	2820	2824	rVB4	5720	7155	1.43%	0.167%
23	18.239	2824	2831	2836	rBV7	12337	27381	5.48%	0.639%
24	18.321	2840	2845	2849	rBV	360819	435189	87.10%	10.160%
25	18.450	2863	2867	2870	rBV5	8956	14413	2.88%	0.336%
26	19.597	3058	3062	3070	rBV2	33388	66681	13.35%	1.557%
27	19.944	3118	3121	3124	rBV	28801	31967	6.40%	0.746%
28	19.992	3126	3129	3139	rVB	245100	312127	62.47%	7.287%


Sum of corrected areas: 4283387

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061317\
Data File : BF095916.D
Acq On : 14 Jun 2017 3:16
Operator : SJ/MA
Sample : I3635-13 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-02-061217-E

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

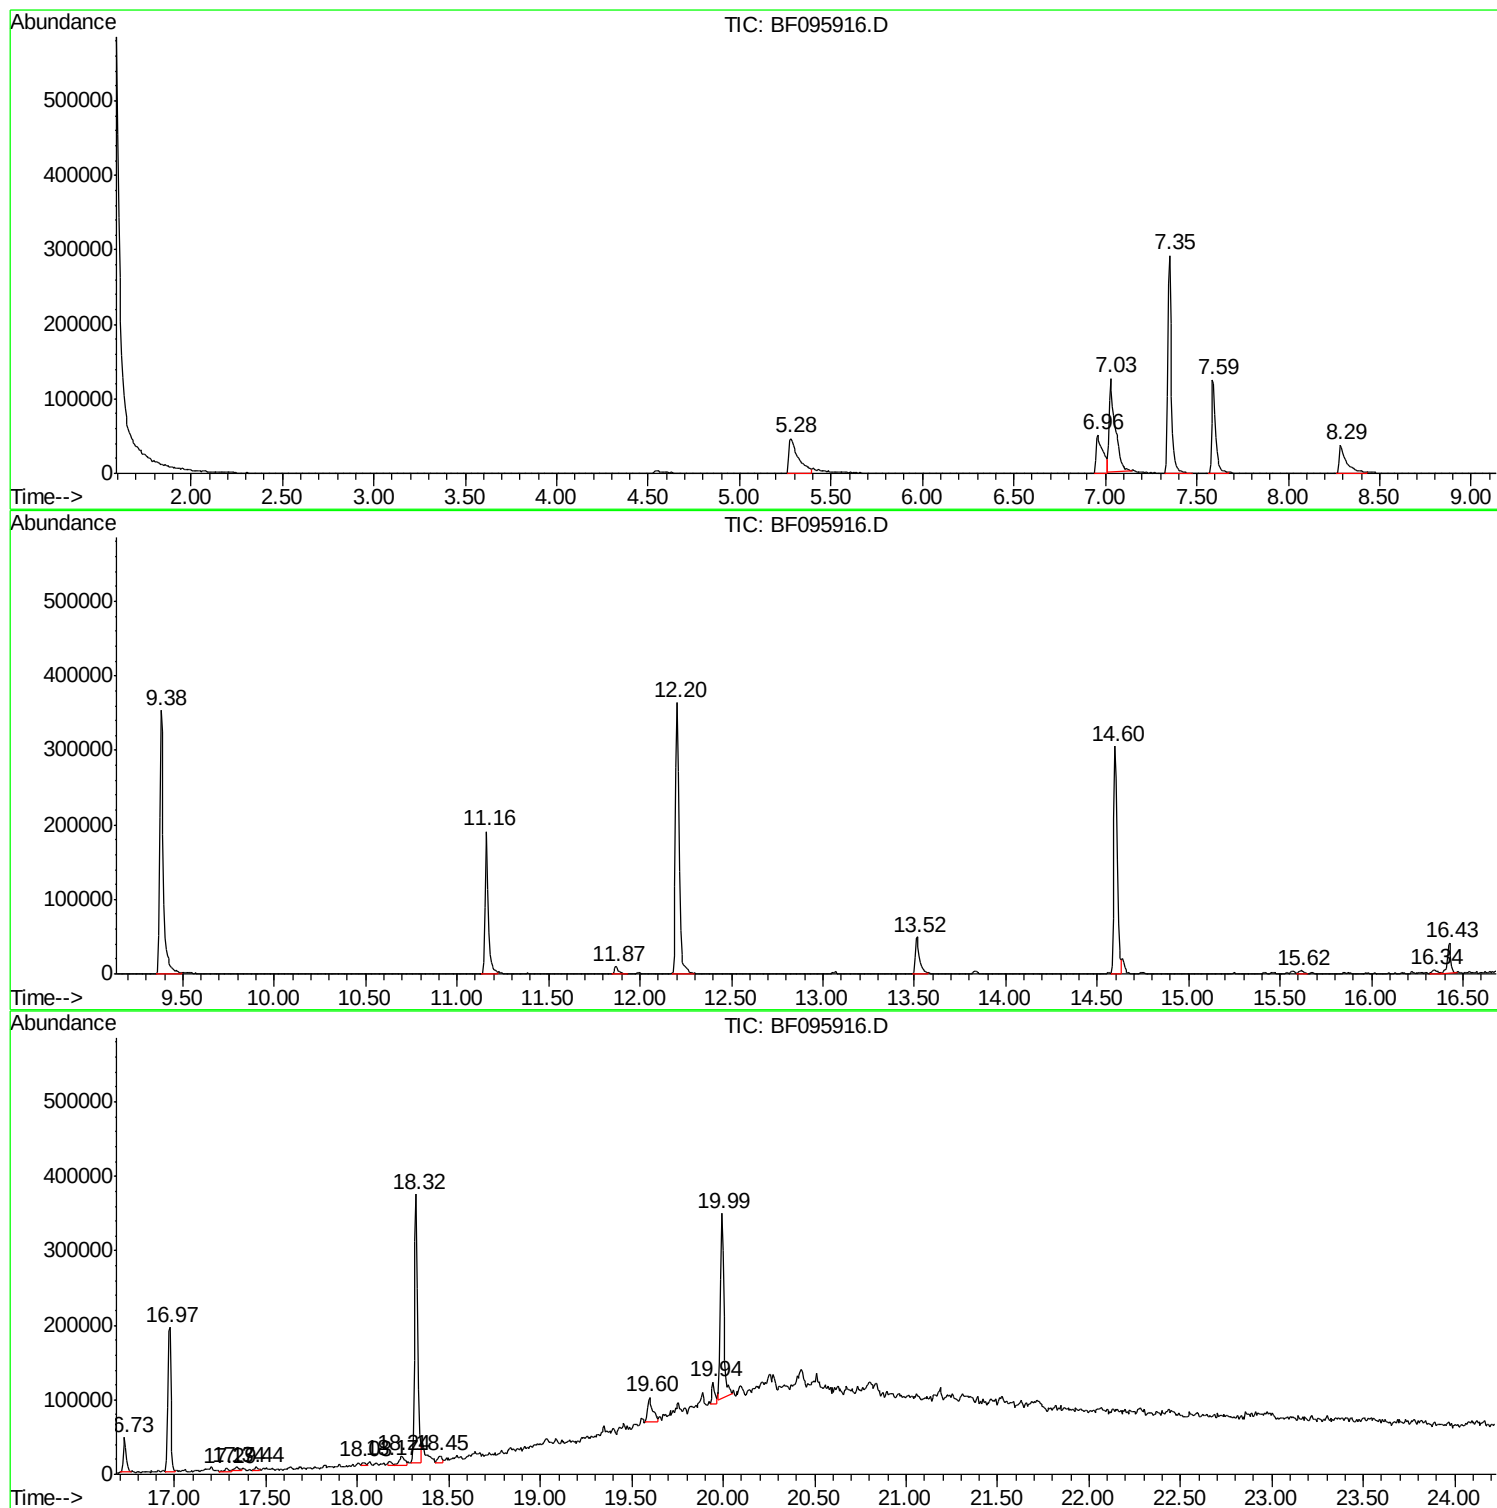

Data Path : Z:\HPCHEM1\BNA F\DATA\BF061317\
Data File : BF095916.D
Acq On : 14 Jun 2017 3:16
Operator : SJ/MA
Sample : I3635-13 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-02-061217-E










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.03 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.03	15.12 ng	295023	1,4-Dichlorobenzene-d4	7.35

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	25
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	10
5		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9

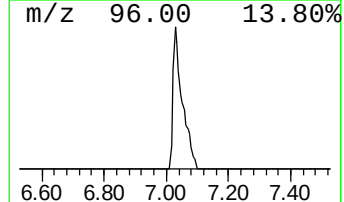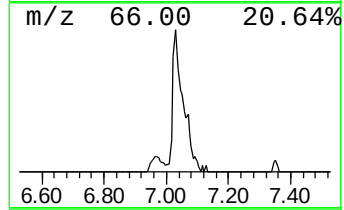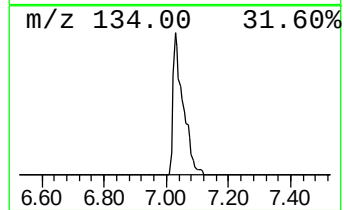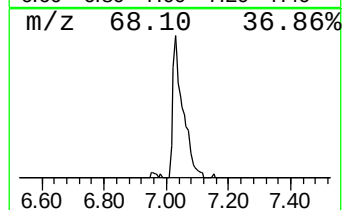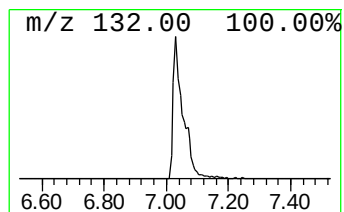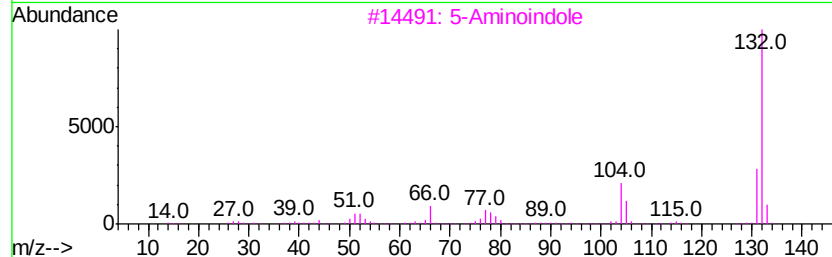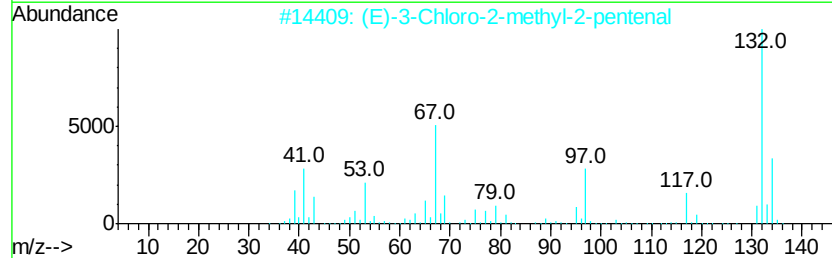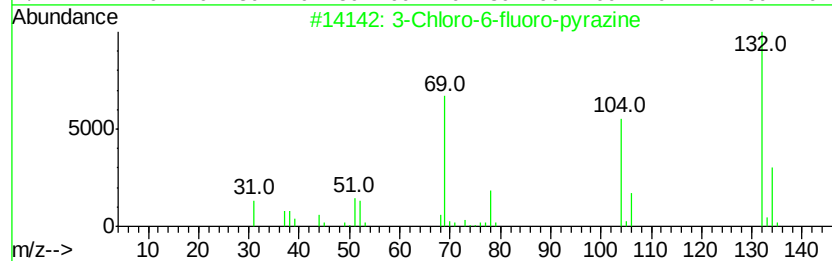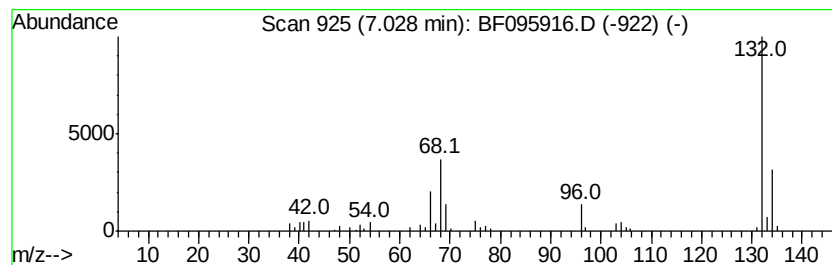

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061317\
Data File : BF095916.D
Acq On : 14 Jun 2017 3:16
Operator : SJ/MA
Sample : I3635-13 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-02-061217-E

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.03	7.03	15.1	ng	295023	1	7.35	390191	20.0