


Data Path : Z:\HPCHEM1\BNA_F\Data\BF061317\
 Data File : BF095894.D
 Acq On : 13 Jun 2017 15:11
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 05 16:15:31 2017

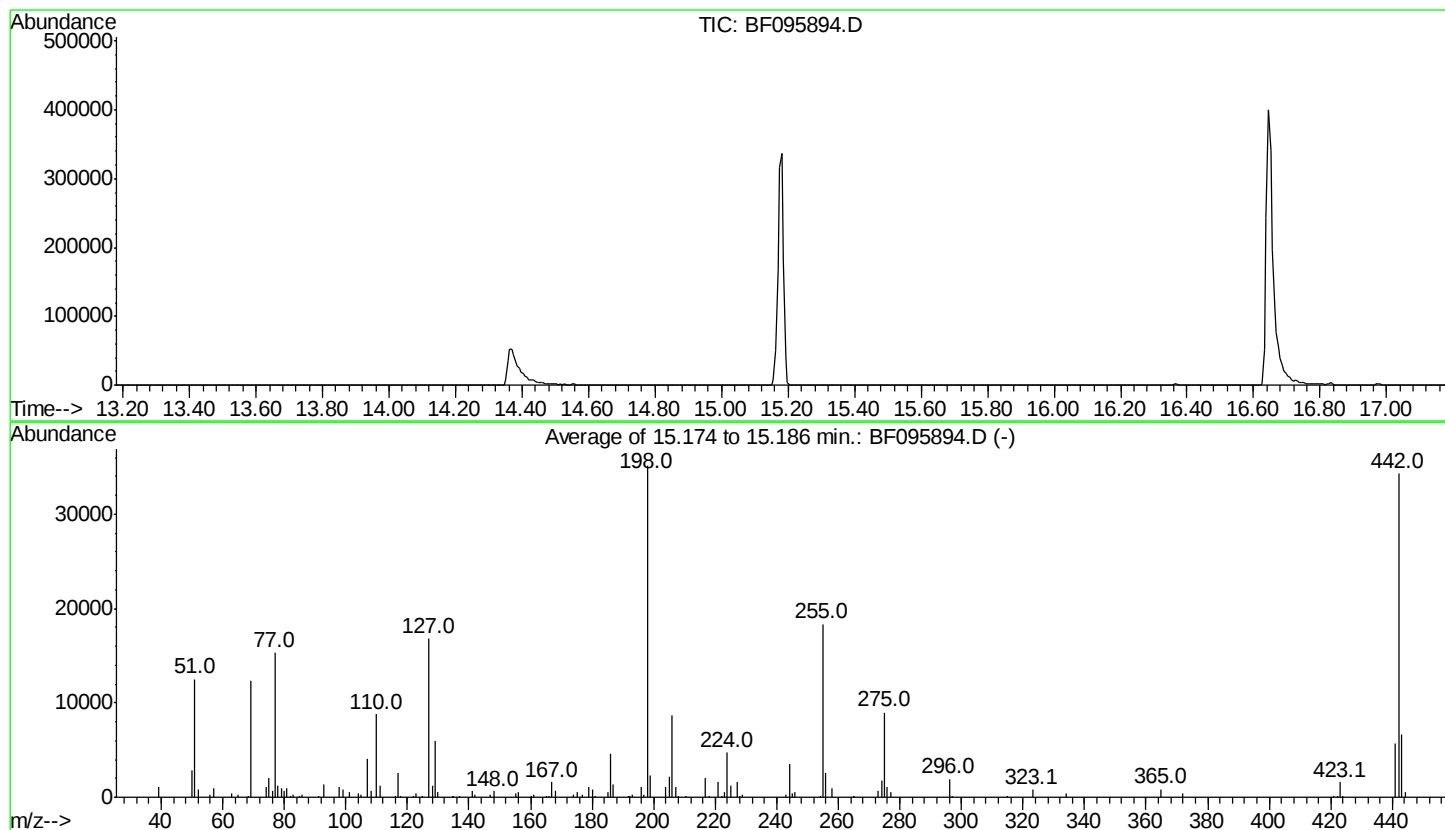

AutoFind: Scans 2310, 2311, 2312; Background Corrected with Scan 2304

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.5	12484	PASS
68	69	0.00	2	0.9	112	PASS
69	198	0.00	100	35.0	12296	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.7	16766	PASS
197	198	0.00	2	0.8	277	PASS
198	198	100	100	100.0	35128	PASS
199	198	5	9	6.4	2254	PASS
275	198	10	60	25.5	8958	PASS
365	198	1	100	2.4	841	PASS
441	442	0.01	24	16.7	5713	PASS
442	198	50	100	97.6	34272	PASS
443	442	15	24	19.5	6687	PASS