
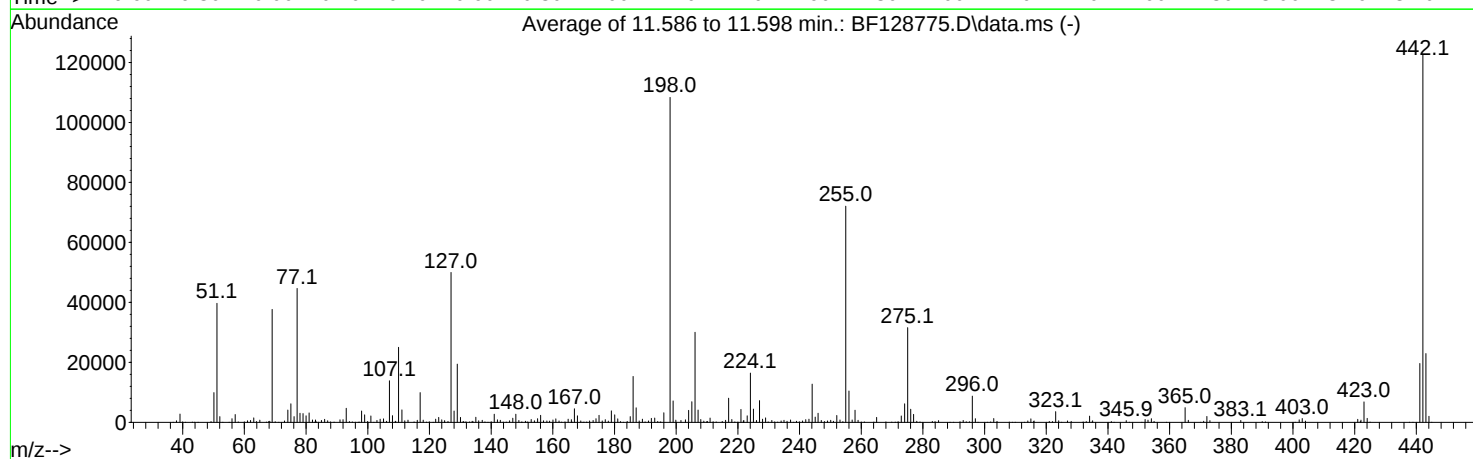


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061322\
 Data File : BF128775.D
 Acq On : 13 Jun 2022 09:36
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 14 14:53:53 2022

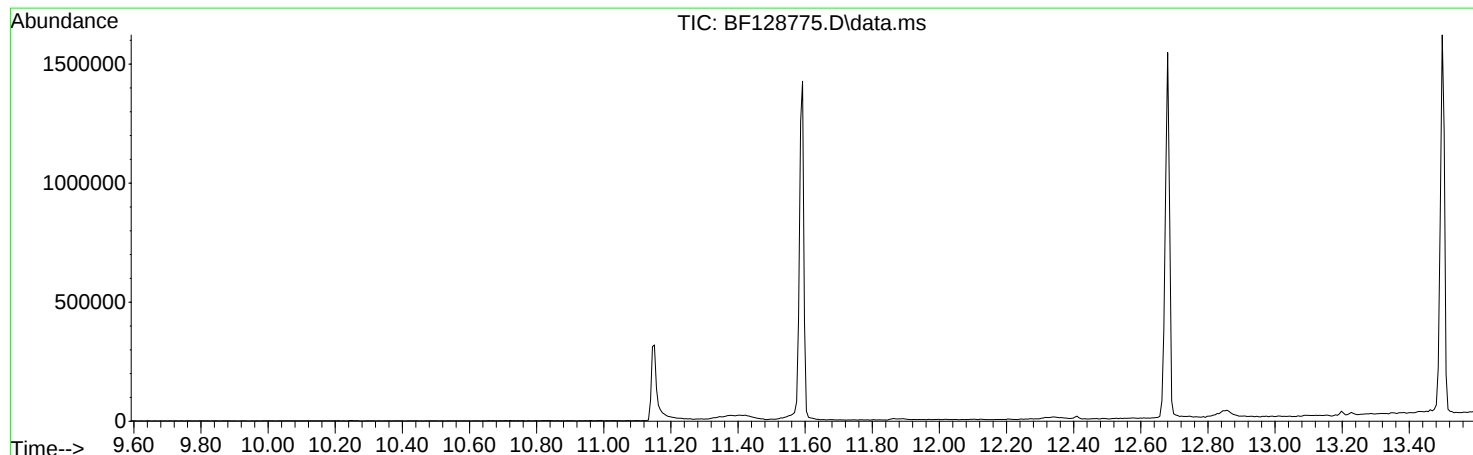




AutoFind: Scans 1581, 1582, 1583; Background Corrected with Scan 1574

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.7	39713	PASS
68	69	0.00	2	1.0	389	PASS
69	198	0.00	100	34.8	37692	PASS
70	69	0.00	2	0.6	210	PASS
127	198	10	80	46.1	49966	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	108357	PASS
199	198	5	9	6.6	7170	PASS
275	198	10	60	29.1	31574	PASS
365	198	1	100	4.6	4931	PASS
441	198	0.01	100	18.1	19613	PASS
442	442	50	100	100.0	122651	PASS
443	442	15	24	18.7	22971	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061322\
Data File : BF128775.D
Acq On : 13 Jun 2022 09:36
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 13 14:04:32 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 08 14:28:39 2022
Response via : Initial Calibration

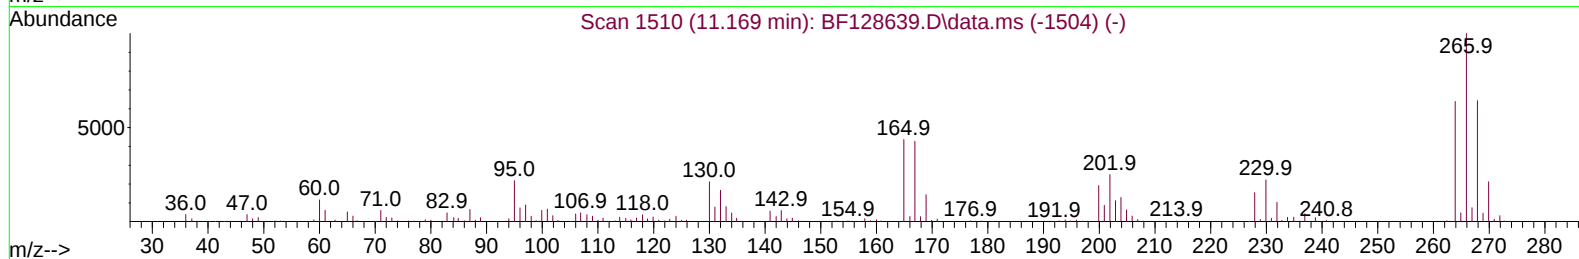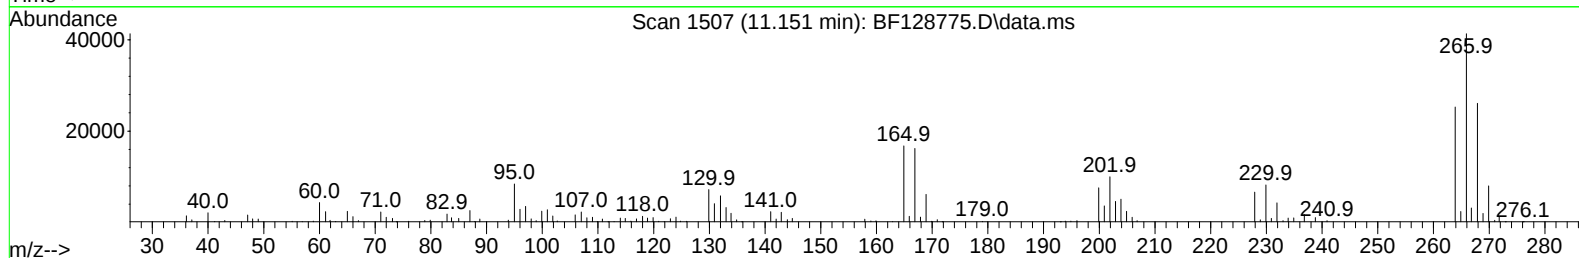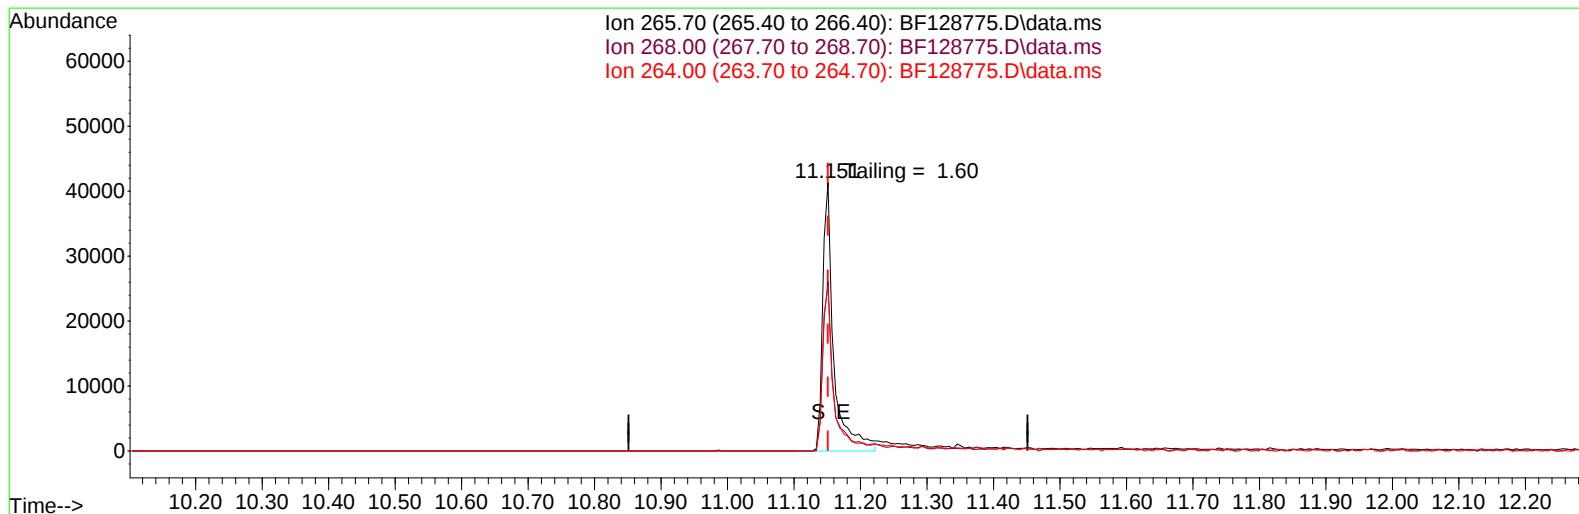

TIC: BF128775.D\data.ms

(70) Pentachlorophenol (C)

11.151min (-0.000) 14952.68 ng


response 52414

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.08
264.00	61.80	61.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061322\
Data File : BF128775.D
Acq On : 13 Jun 2022 09:36
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 13 14:04:32 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 08 14:28:39 2022
Response via : Initial Calibration

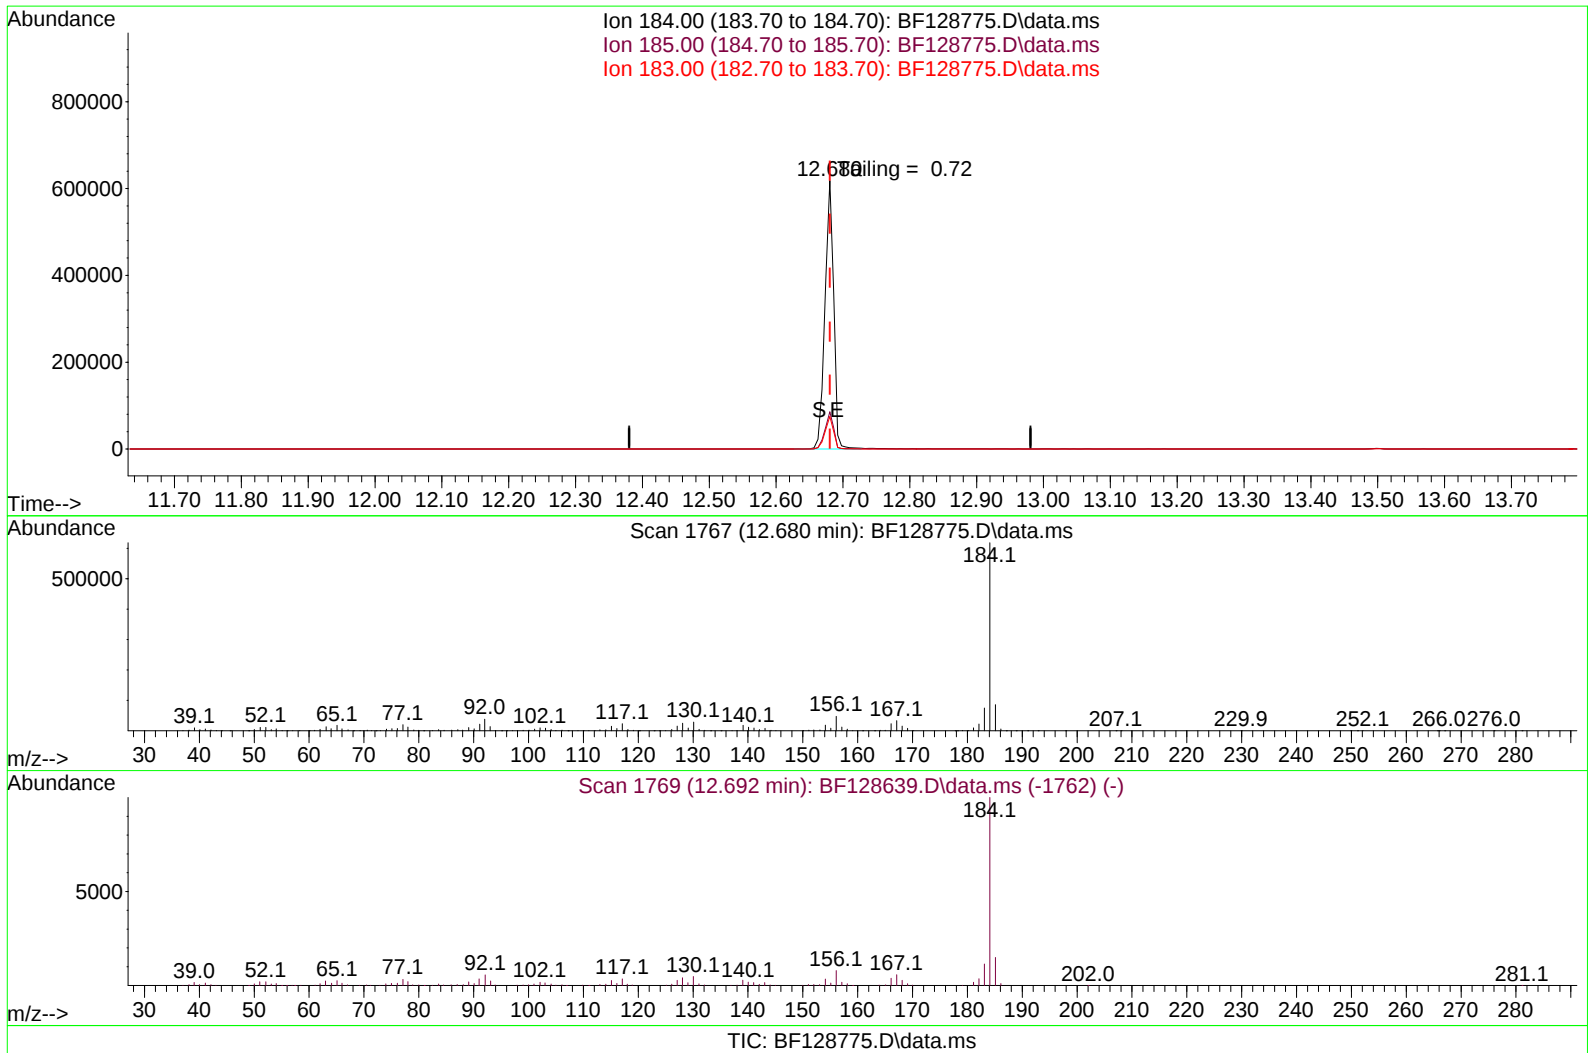**(77) Benzidine**

12.680min (-0.000) 484614.60 ng

response 560311

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	13.91
183.00	11.60	12.10
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/13/2022	BNA_F	<u>BF128775.D</u>
Compound Name	Response	Retention Time
DDT	267743	13.49
DDD	3275	13.19
DDE	1155	12.86
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4430	272173	1.63

Instrument :
BNA_F
ClientSampleId :
DFTPP