
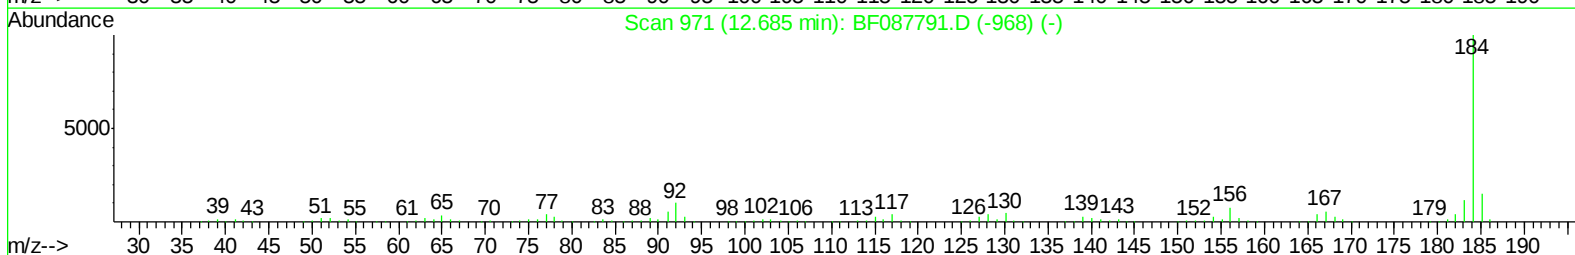
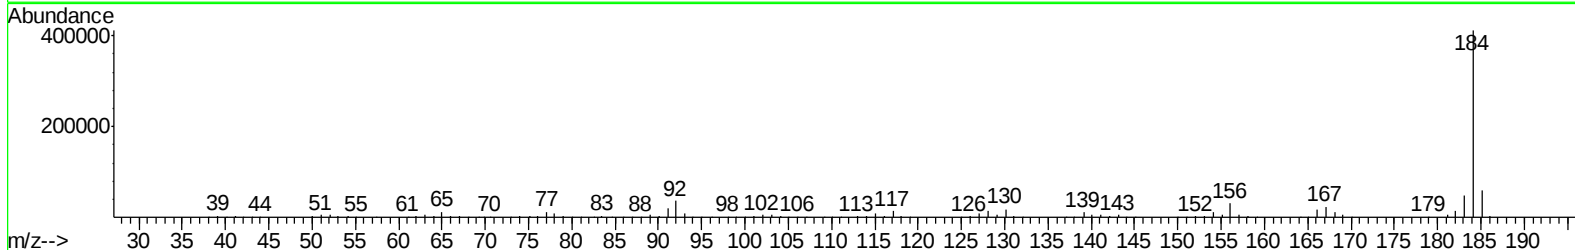


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061416\
Data File : BF088004.D
Acq On : 14 Jun 2016 14:42
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 15 07:26:35 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 15 04:08:24 2016
Response via : Initial Calibration

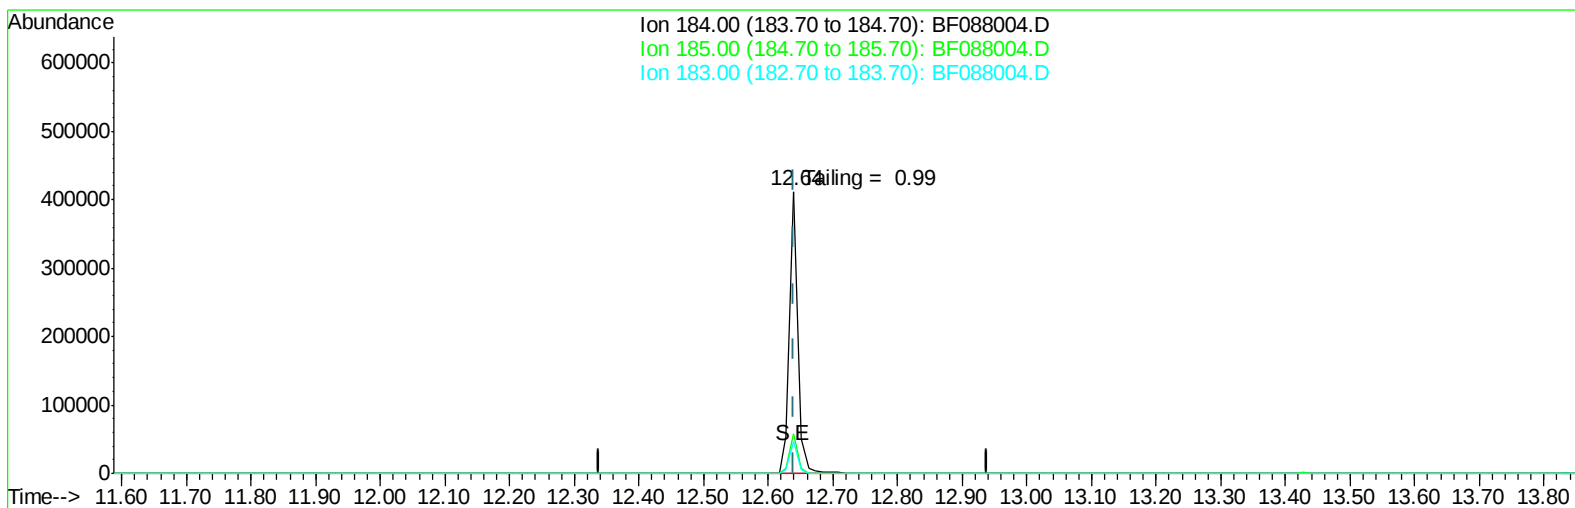

TIC: BF088004.D

(76) Benzidine




12.639min (-0.000) 0.00ng

response 368420

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	14.22
183.00	11.60	11.53
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061416\
Data File : BF088004.D
Acq On : 14 Jun 2016 14:42
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 15 07:26:35 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 15 04:08:24 2016
Response via : Initial Calibration

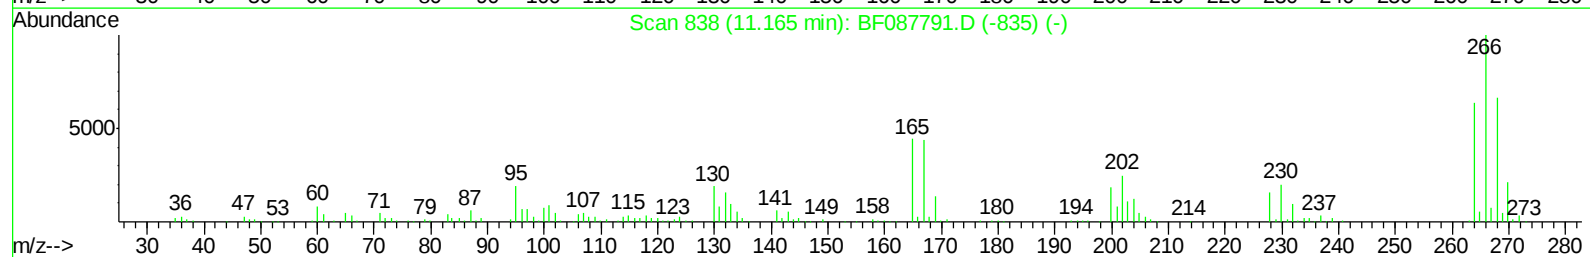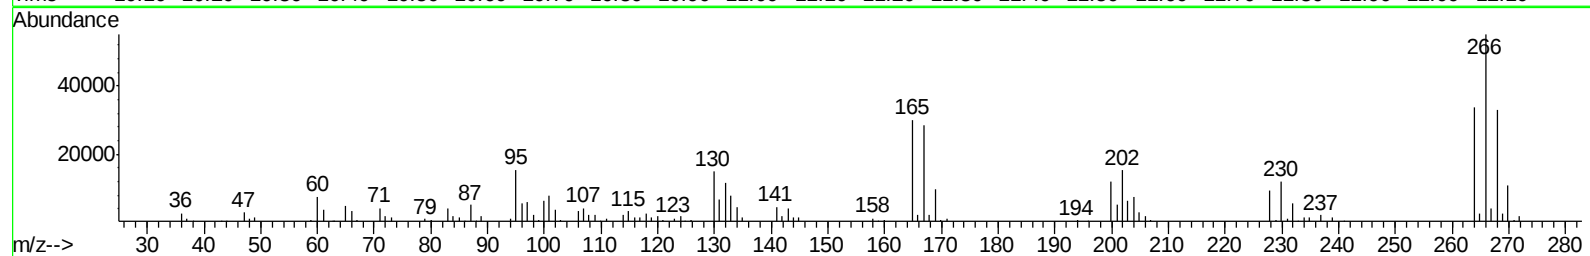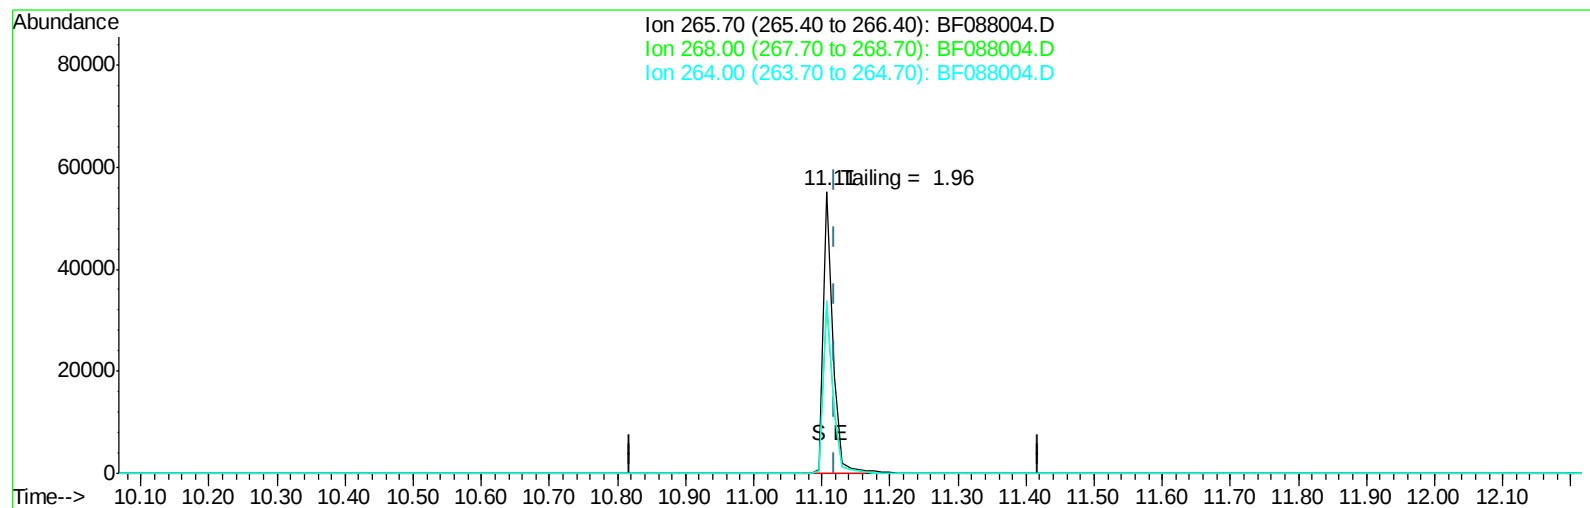

TIC: BF088004.D

(69) Pentachlorophenol (C)

11.108min (-0.012) 0.00ng

response 55112

Ion	Exp%	Act%
265.70	100	100
268.00	66.00	59.75
264.00	62.00	61.42
0.00	0.00	0.00