


Data Path : Z:\HPCHEM1\BNA F\DATA\BF061416\
 Data File : BF088022.D
 Acq On : 15 Jun 2016 2:48
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 13 14:10:49 2016

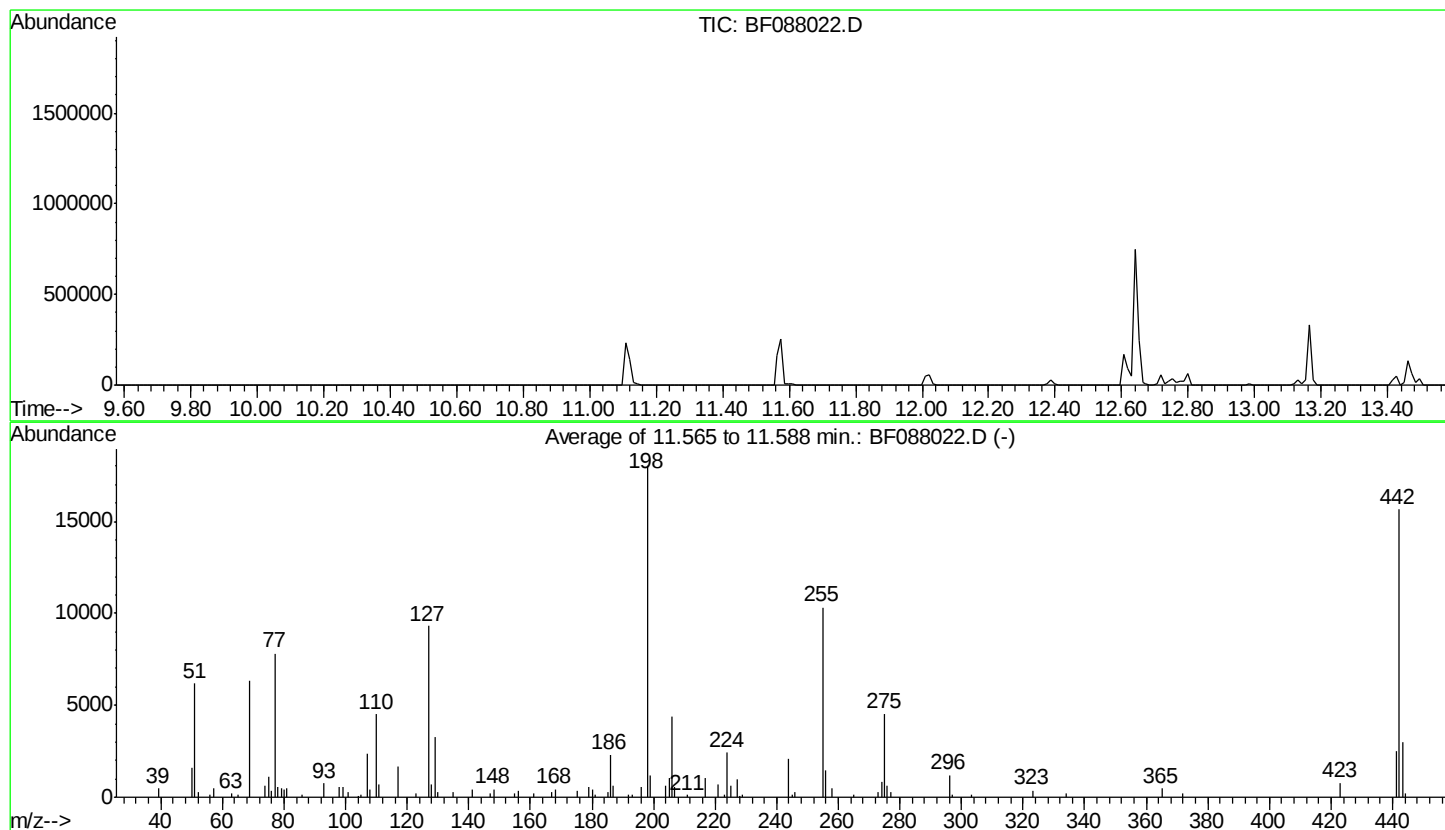

AutoFind: Scans 873, 874, 875; Background Corrected with Scan 870

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.2	6162	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.1	6322	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.7	9319	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	18029	PASS
199	198	5	9	6.4	1159	PASS
275	198	10	60	25.3	4555	PASS
365	198	1	100	2.6	464	PASS
441	442	0.01	24	16.1	2520	PASS
442	198	50	100	86.8	15647	PASS
443	442	15	24	19.0	2971	PASS