
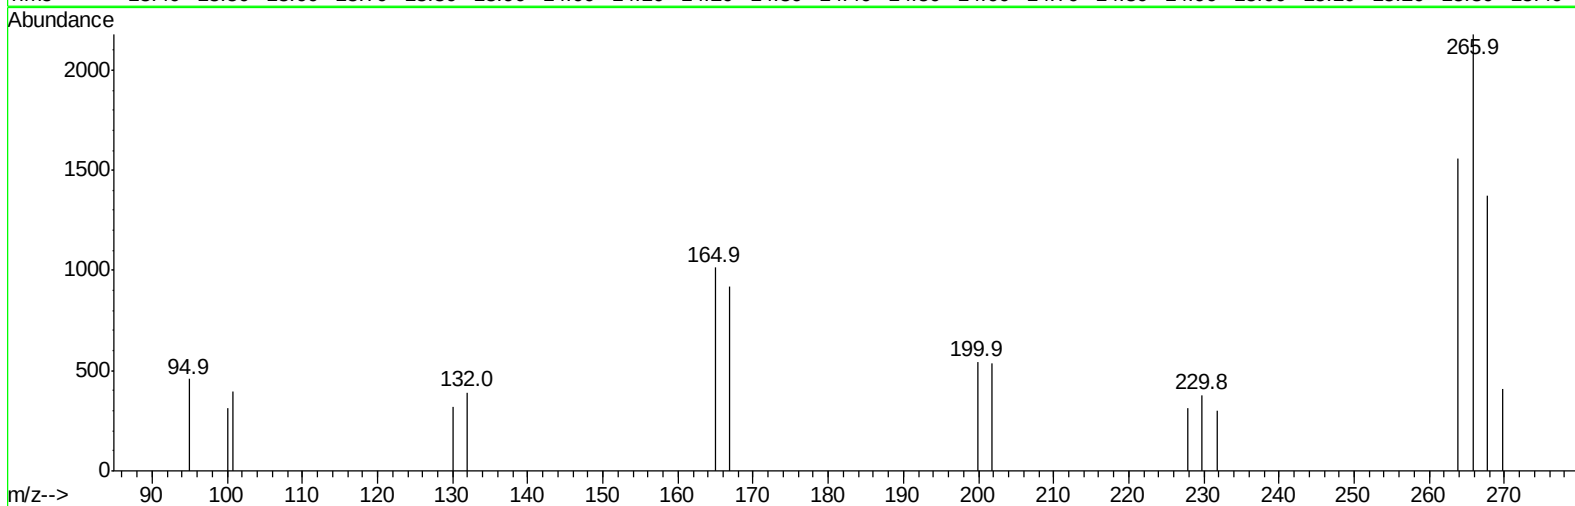


Data Path : Z:\HPCHEM1\BNA F\DATA\BF061417\
Data File : BF095946.D
Acq On : 15 Jun 2017 4:36
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 15 07:22:45 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 16:15:31 2017
Response via : Initial Calibration

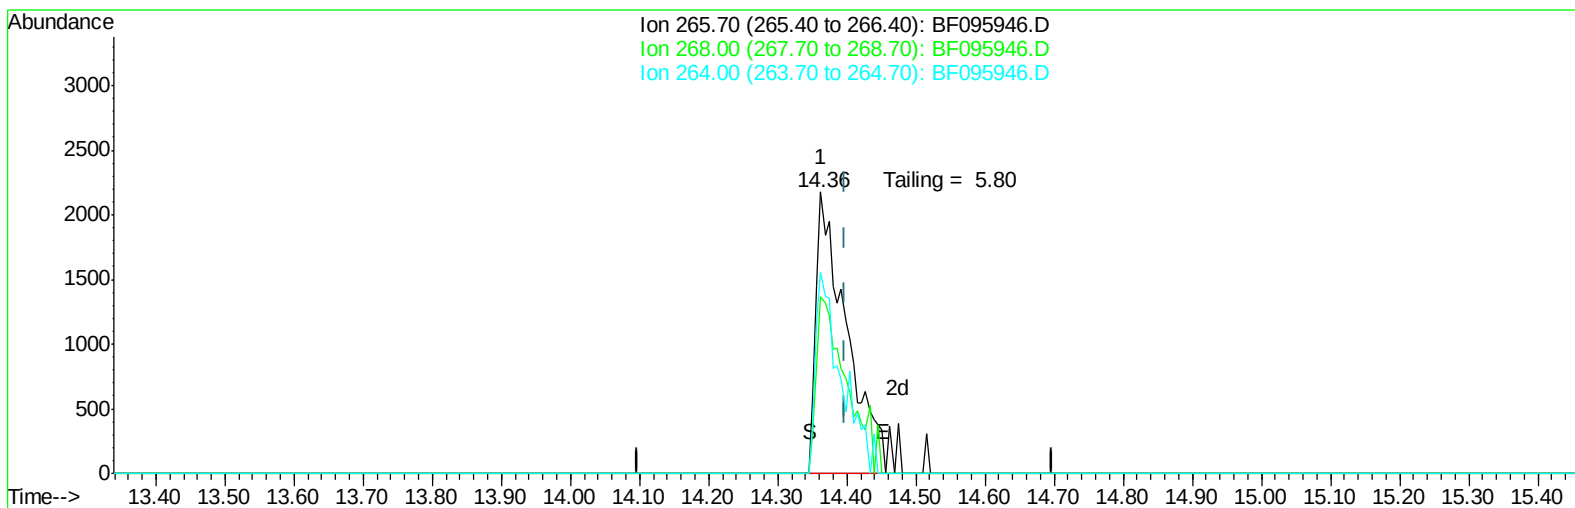

TIC: BF095946.D

(69) Pentachlorophenol (C)



14.362min (-0.035) 0.00ng

response 6577

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.95
264.00	64.60	71.44
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF061417\
Data File : BF095946.D
Acq On : 15 Jun 2017 4:36
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 15 07:22:45 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 16:15:31 2017
Response via : Initial Calibration

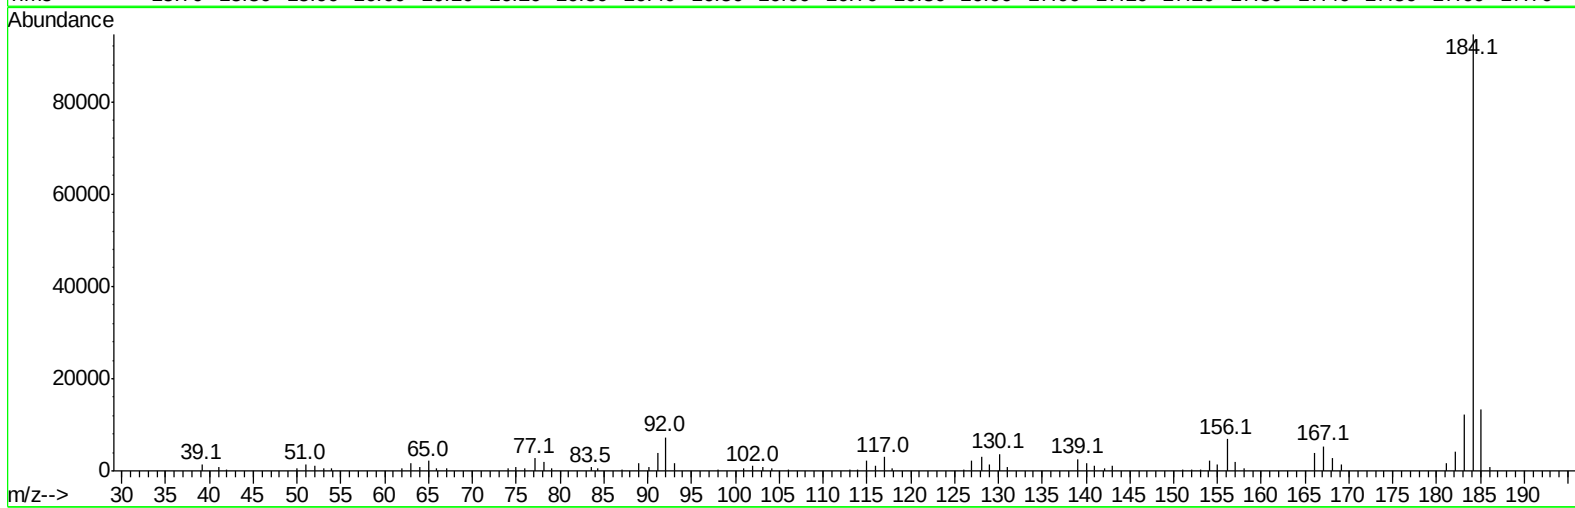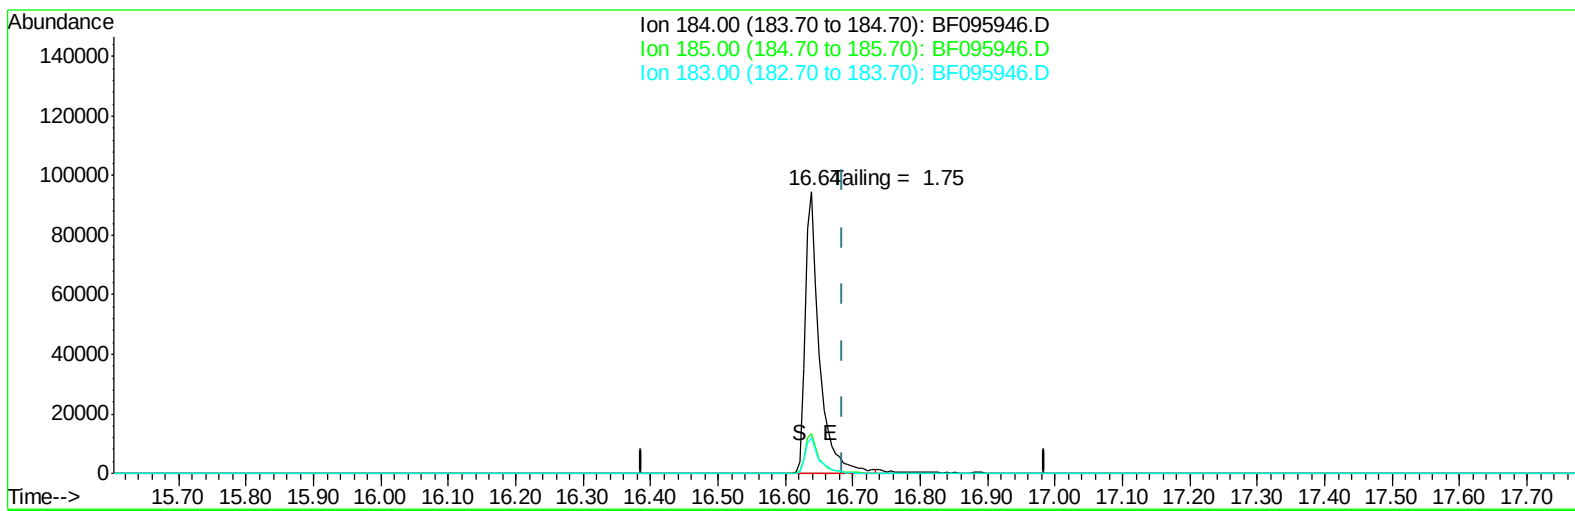

TIC: BF095946.D

(76) Benzidine

16.639min (-0.047) 6958.76ng

response 140844

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.07#
183.00	12.20	12.90
0.00	0.00	0.00