


Data Path : Z:\HPCHEM1\BNA F\Data\BF061417\
 Data File : BF095923.D
 Acq On : 14 Jun 2017 15:23
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 05 16:15:31 2017

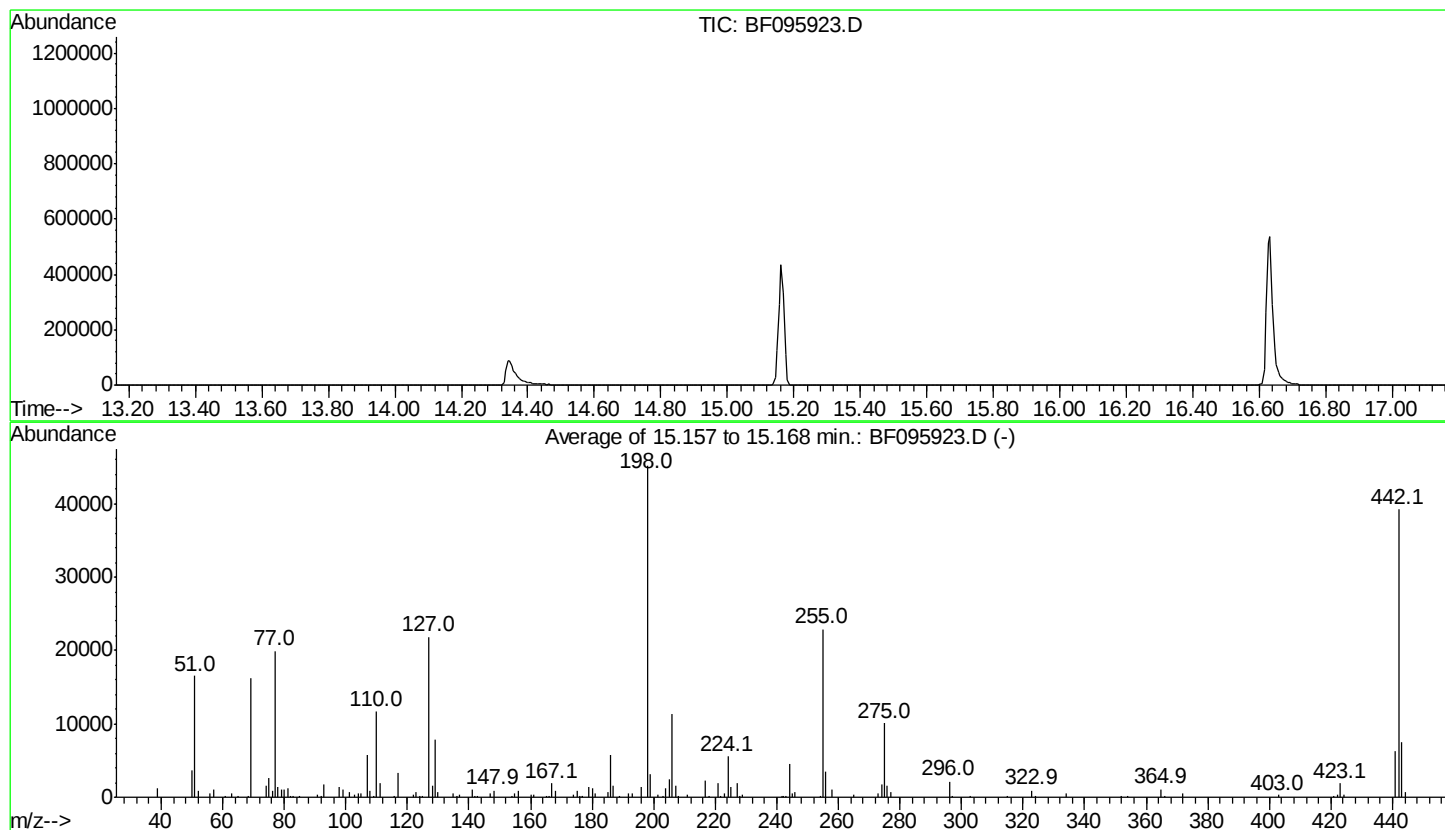

AutoFind: Scans 2307, 2308, 2309; Background Corrected with Scan 2300

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.5	16495	PASS
68	69	0.00	2	1.4	225	PASS
69	198	0.00	100	35.7	16149	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.4	21893	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	45197	PASS
199	198	5	9	6.9	3099	PASS
275	198	10	60	22.3	10091	PASS
365	198	1	100	2.5	1128	PASS
441	442	0.01	24	16.1	6307	PASS
442	198	50	100	86.8	39216	PASS
443	442	15	24	19.2	7549	PASS