


Data Path : Z:\HPCHEM1\BNA F\Data\BF061417\  
 Data File : BF095946.D  
 Acq On : 15 Jun 2017 4:36  
 Operator : SJ/MA  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF060517.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon Jun 05 16:15:31 2017

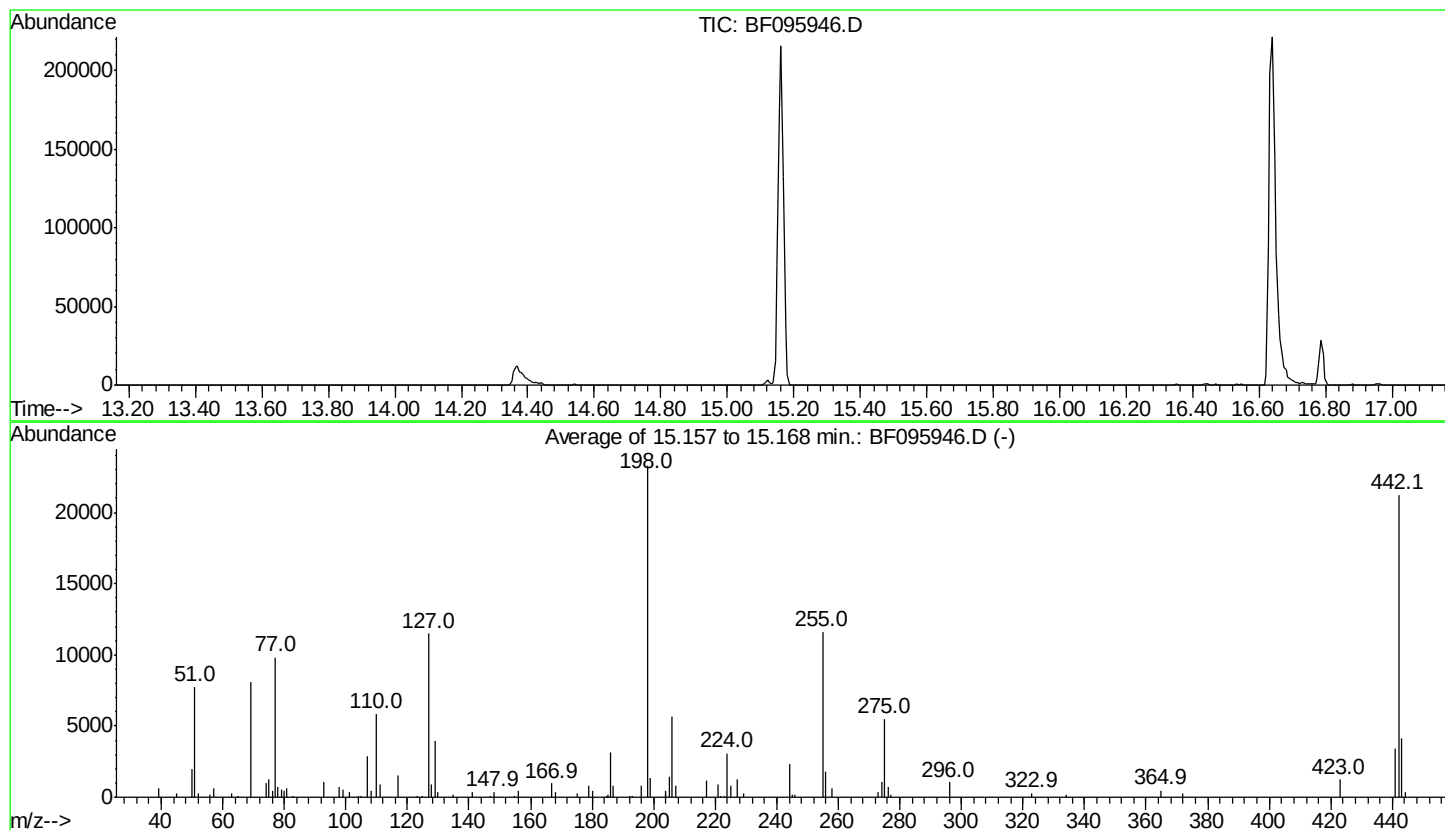

AutoFind: Scans 2307, 2308, 2309; Background Corrected with Scan 2301

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 33.3         | 7760       | PASS                |
| 68             | 69              | 0.00            | 2               | 0.0          | 0          | PASS                |
| 69             | 198             | 0.00            | 100             | 34.7         | 8072       | PASS                |
| 70             | 69              | 0.00            | 2               | 0.0          | 0          | PASS                |
| 127            | 198             | 10              | 80              | 49.4         | 11506      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 23288      | PASS                |
| 199            | 198             | 5               | 9               | 6.0          | 1396       | PASS                |
| 275            | 198             | 10              | 60              | 23.6         | 5495       | PASS                |
| 365            | 198             | 1               | 100             | 2.0          | 467        | PASS                |
| 441            | 442             | 0.01            | 24              | 16.3         | 3458       | PASS                |
| 442            | 198             | 50              | 100             | 91.3         | 21256      | PASS                |
| 443            | 442             | 15              | 24              | 19.4         | 4124       | PASS                |