
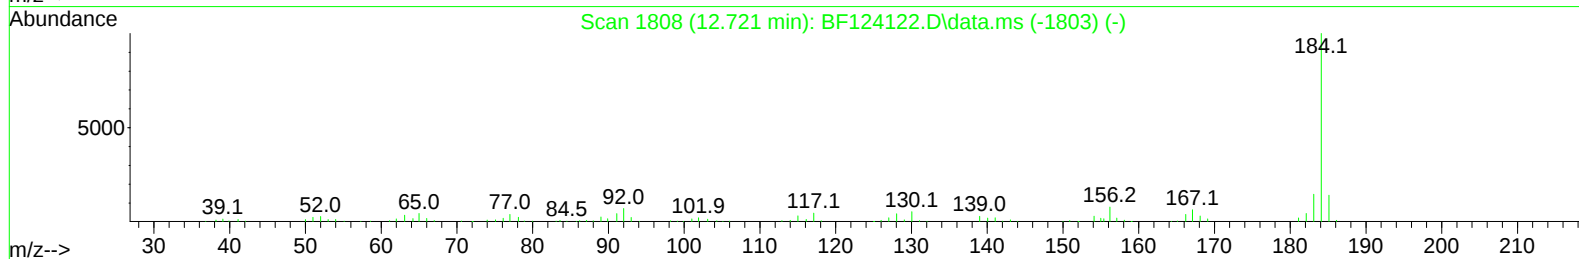
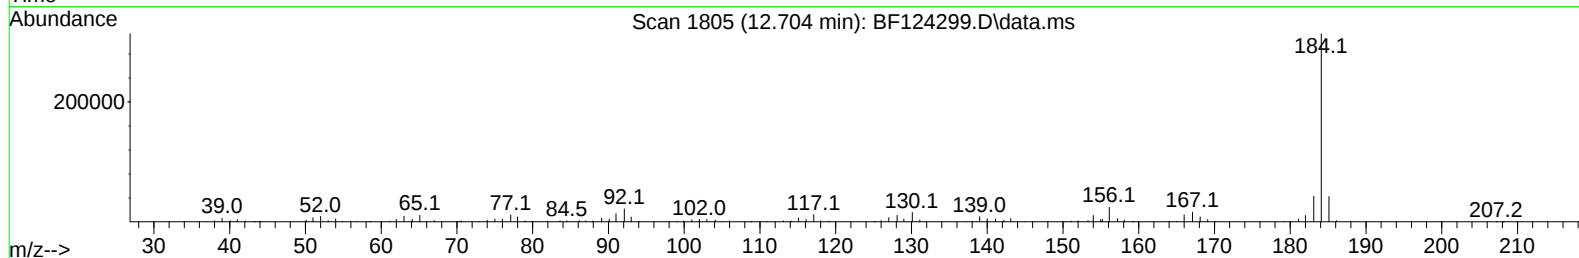


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061421\
 Data File : BF124299.D
 Acq On : 14 Jun 2021 10:19
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 14 11:00:10 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 10 01:53:56 2021
 Response via : Initial Calibration

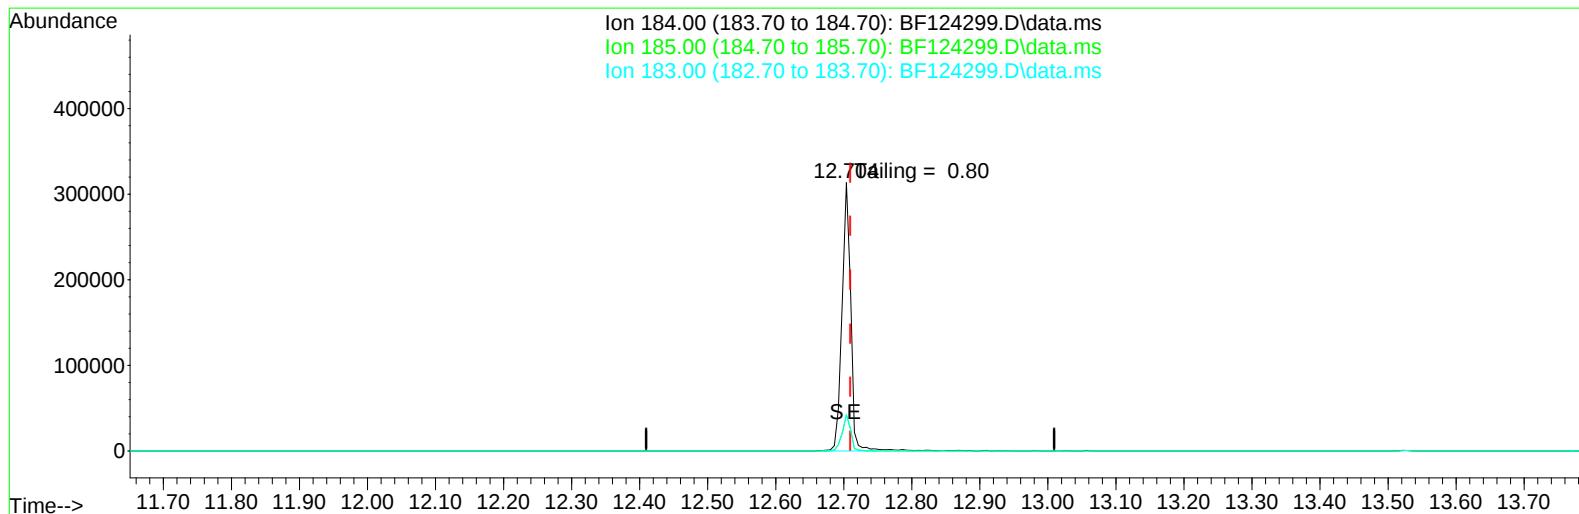

TIC: BF124299.D\data.ms

(77) Benzidine




12.704min (-0.006) 0.00 ng

response 280503

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.58
183.00	9.80	13.61#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061421\
Data File : BF124299.D
Acq On : 14 Jun 2021 10:19
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 14 11:00:10 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 10 01:53:56 2021
Response via : Initial Calibration

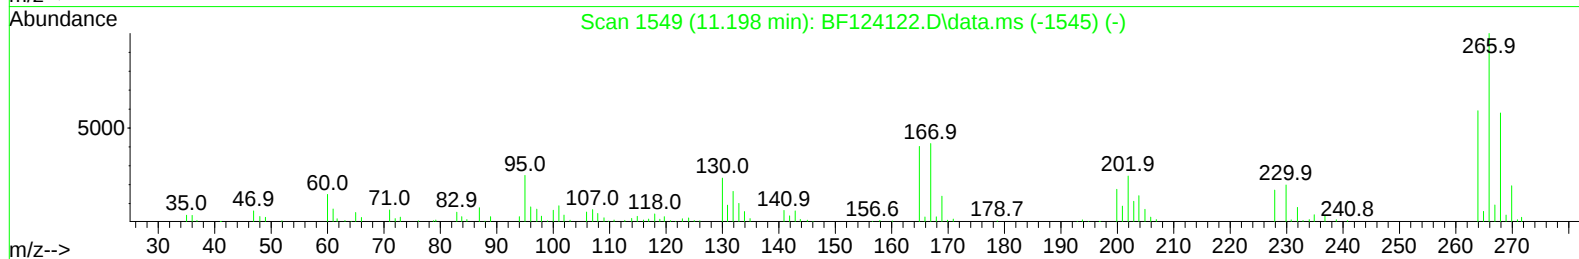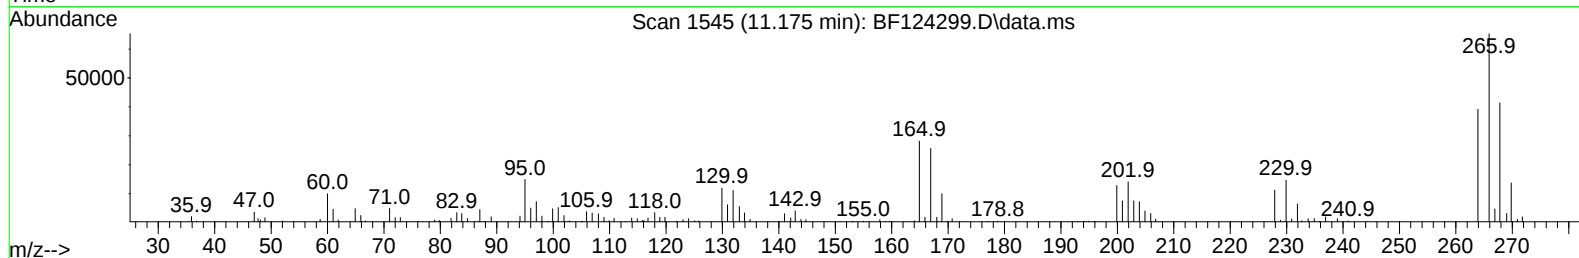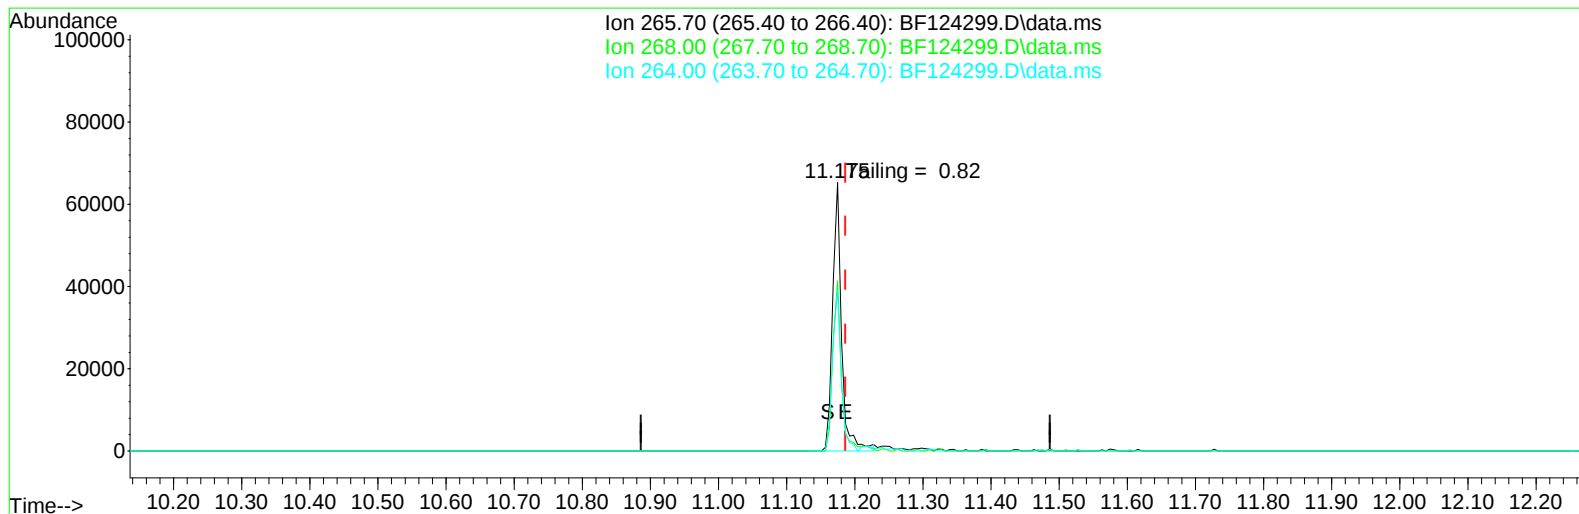

TIC: BF124299.D\data.ms

(70) Pentachlorophenol (C)

11.175min (-0.012) 23982.65 ng

response 60911

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.41
264.00	65.70	60.02
0.00	0.00	0.00