

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061421\
 Data File : BF124301.D
 Acq On : 14 Jun 2021 12:04
 Operator : JU/CG
 Sample : PB137074BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB137074BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124301.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.081	506	509	517	rBB2	24612	33467	1.63%	0.292%
2	5.475	571	576	579	rBV	1533363	1503713	73.28%	13.104%
3	6.481	742	747	750	rBV	1414829	1421892	69.30%	12.391%
4	6.828	803	806	810	rBV	362164	280281	13.66%	2.443%
5	7.398	897	903	906	rBV	1010077	985331	48.02%	8.587%
6	8.116	1020	1025	1028	rBV	385639	350415	17.08%	3.054%
7	9.192	1202	1208	1211	rBV	2112178	1947793	94.92%	16.974%
8	9.874	1319	1324	1327	rBV	491177	434850	21.19%	3.790%
9	10.669	1454	1459	1462	rBV	1567781	1339439	65.28%	11.673%
10	11.363	1573	1577	1580	rBV	524883	434038	21.15%	3.782%
11	12.957	1843	1848	1851	rBV	2260263	2051930	100.00%	17.882%
12	13.874	2001	2004	2007	rVB	40229	37767	1.84%	0.329%
13	14.010	2023	2027	2031	rVB	402519	343318	16.73%	2.992%
14	15.492	2273	2279	2284	rBV	223841	272507	13.28%	2.375%
15	17.009	2530	2537	2539	rBV6	17869	38278	1.87%	0.334%




Sum of corrected areas: 11475019

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061421\
Data File : BF124301.D
Acq On : 14 Jun 2021 12:04
Operator : JU/CG
Sample : PB137074BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137074BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

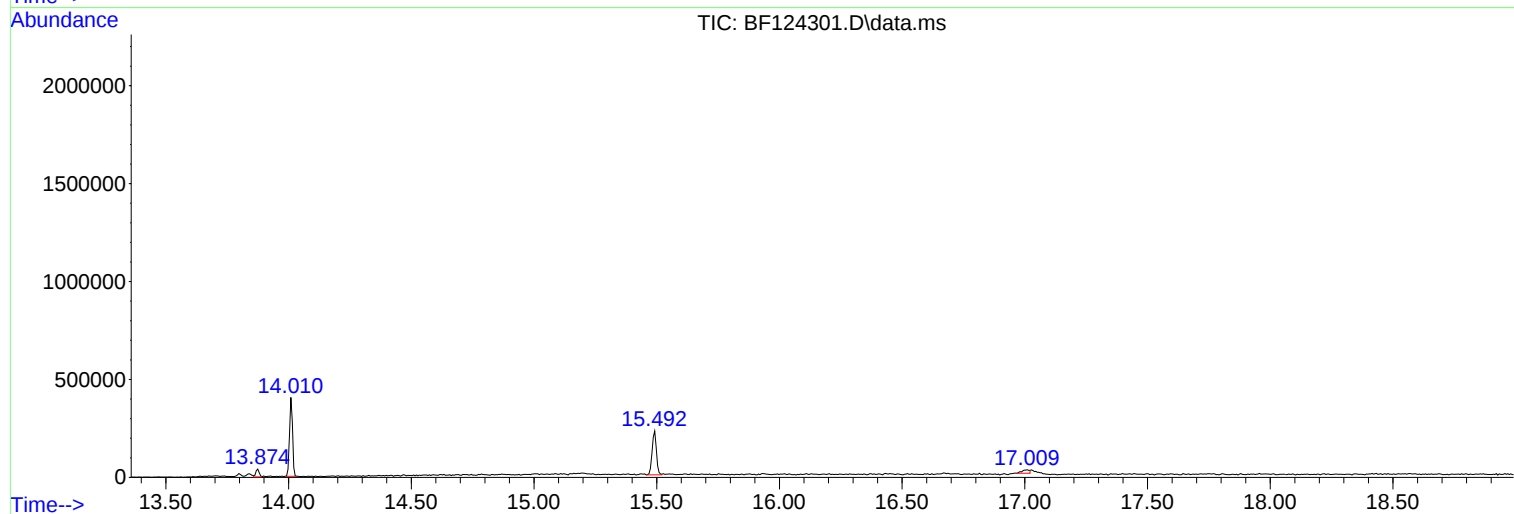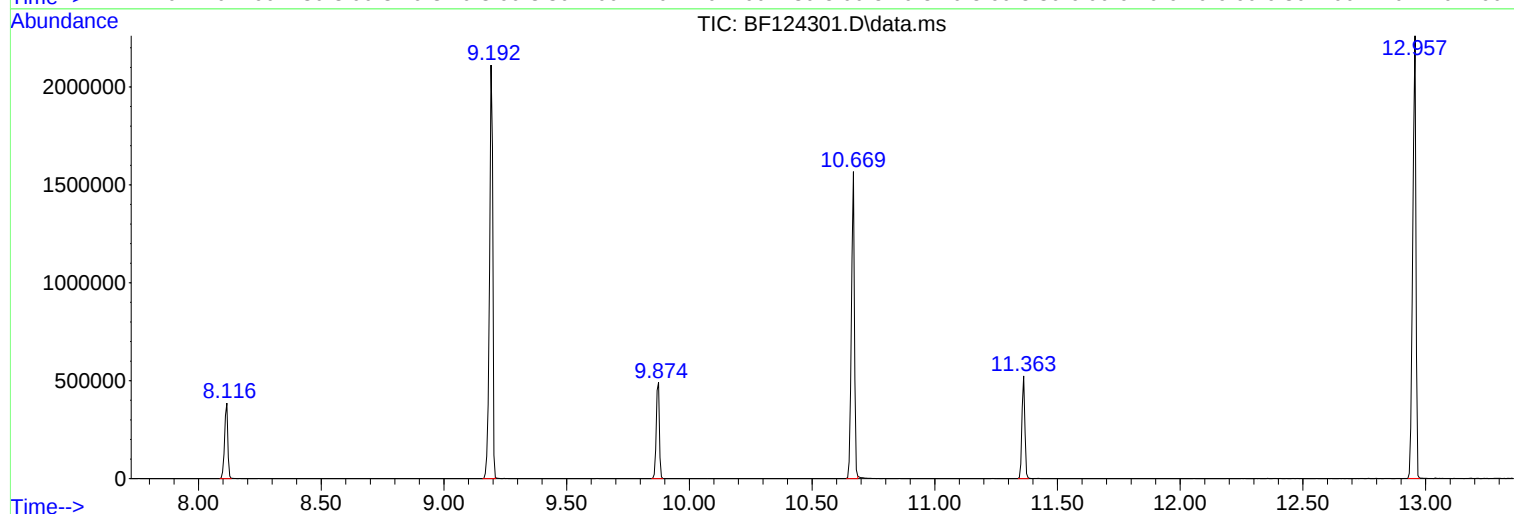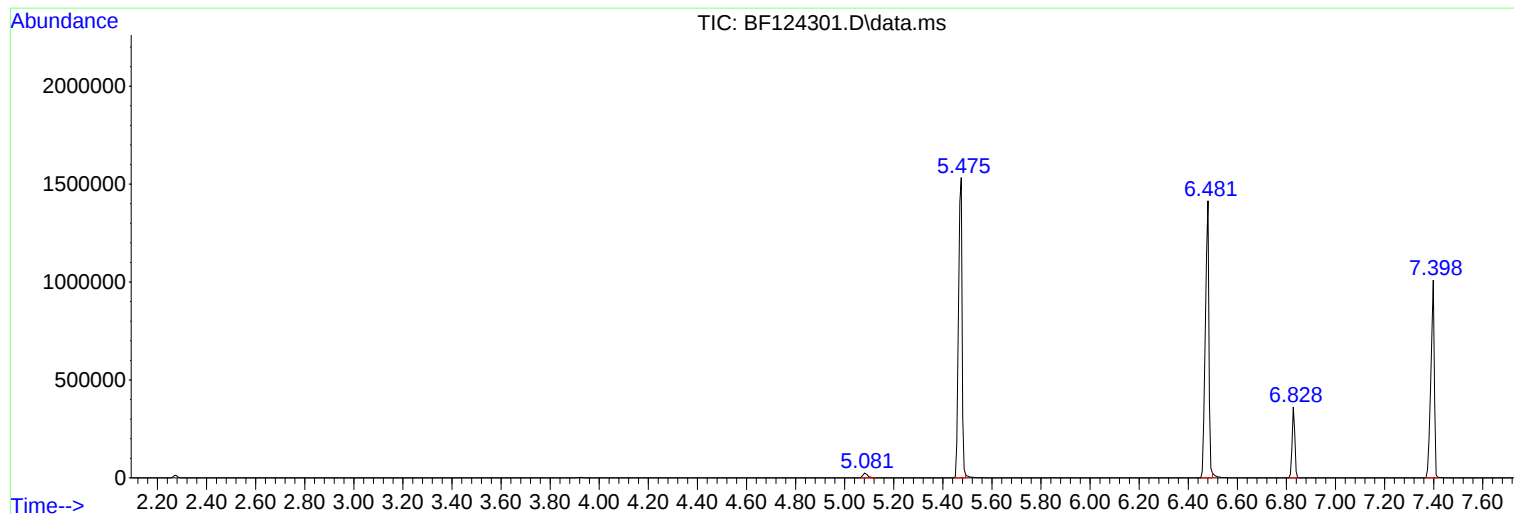

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061421\
Data File : BF124301.D
Acq On : 14 Jun 2021 12:04
Operator : JU/CG
Sample : PB137074BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137074BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061421\
Data File : BF124301.D
Acq On : 14 Jun 2021 12:04
Operator : JU/CG
Sample : PB137074BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137074BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------