
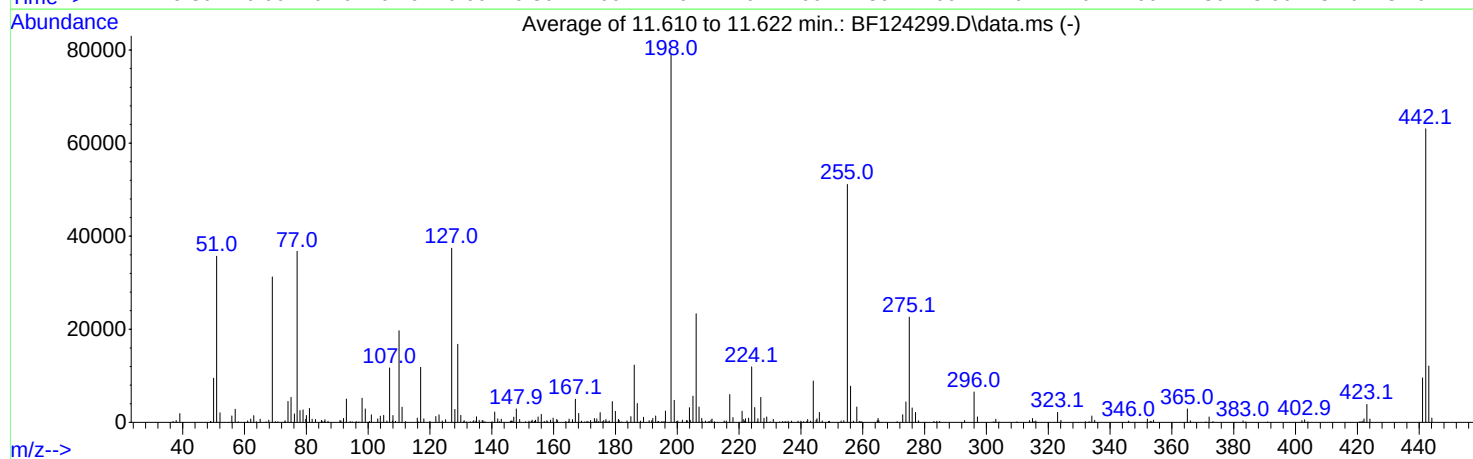


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061421\
 Data File : BF124299.D
 Acq On : 14 Jun 2021 10:19
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 14 12:10:02 2021

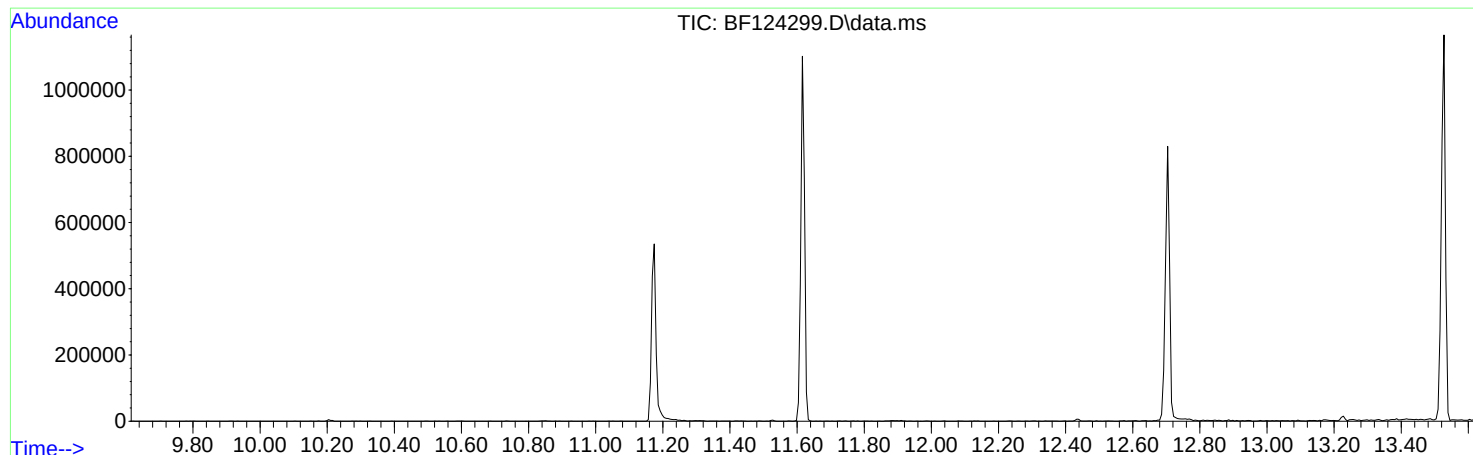




AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.2	35693	PASS
68	69	0.00	2	1.5	479	PASS
69	198	0.00	100	39.5	31243	PASS
70	69	0.00	2	0.4	134	PASS
127	198	10	80	47.3	37392	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	79037	PASS
199	198	5	9	6.0	4759	PASS
275	198	10	60	28.6	22619	PASS
365	198	1	100	3.6	2873	PASS
441	198	0.01	100	12.1	9559	PASS
442	442	50	100	100.0	63099	PASS
443	442	15	24	19.2	12098	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061421\
 Data File : BF124299.D
 Acq On : 14 Jun 2021 10:19
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jun 14 11:00:10 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 10 01:53:56 2021
 Response via : Initial Calibration

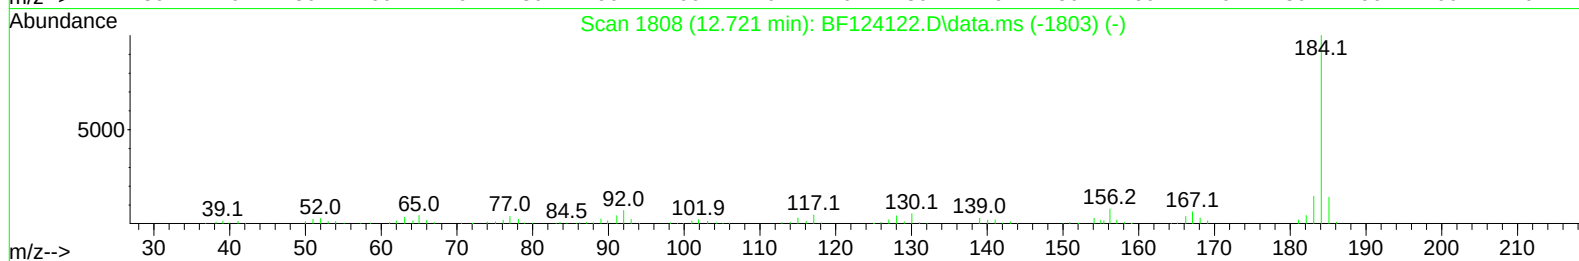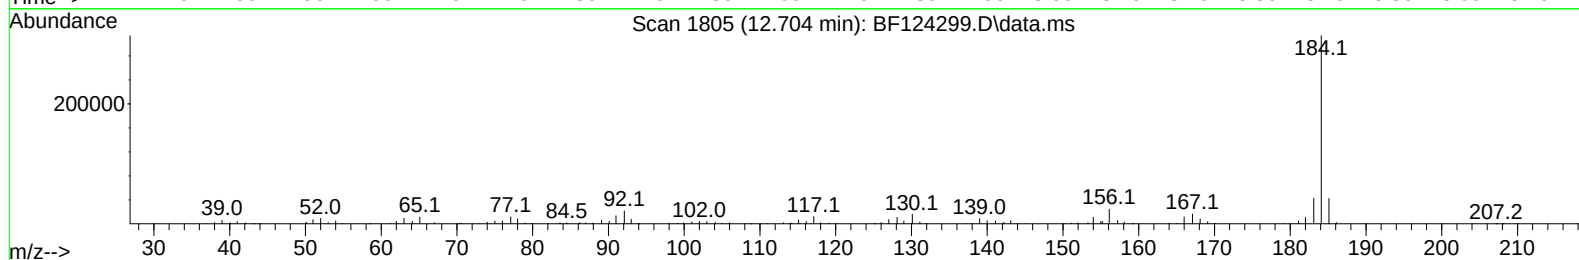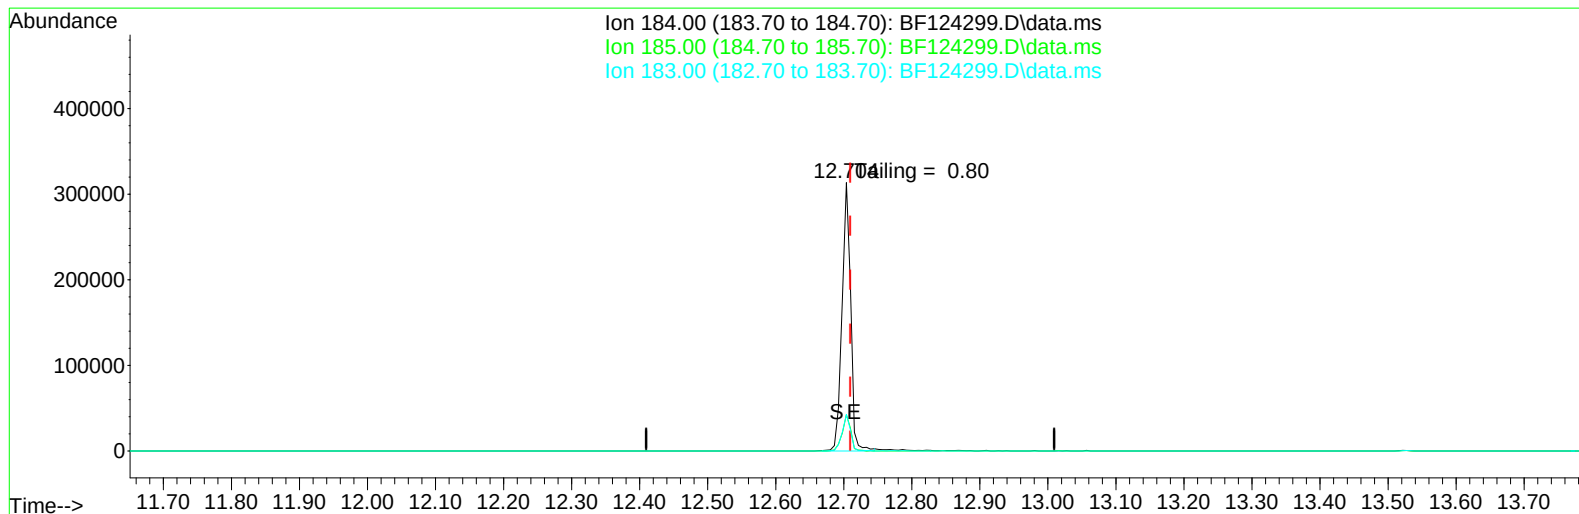

TIC: BF124299.D\data.ms

(77) Benzidine

12.704min (-0.006) 0.00 ng




response 280503

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.58
183.00	9.80	13.61#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061421\
 Data File : BF124299.D
 Acq On : 14 Jun 2021 10:19
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jun 14 11:00:10 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 10 01:53:56 2021
 Response via : Initial Calibration

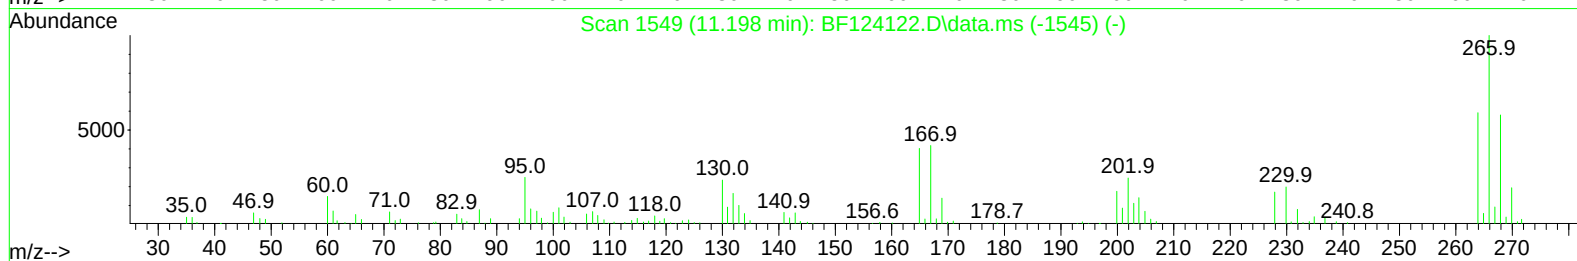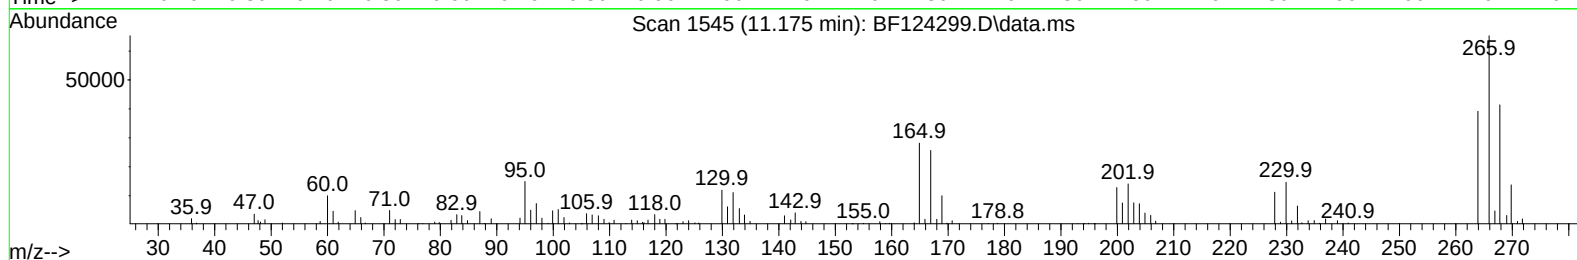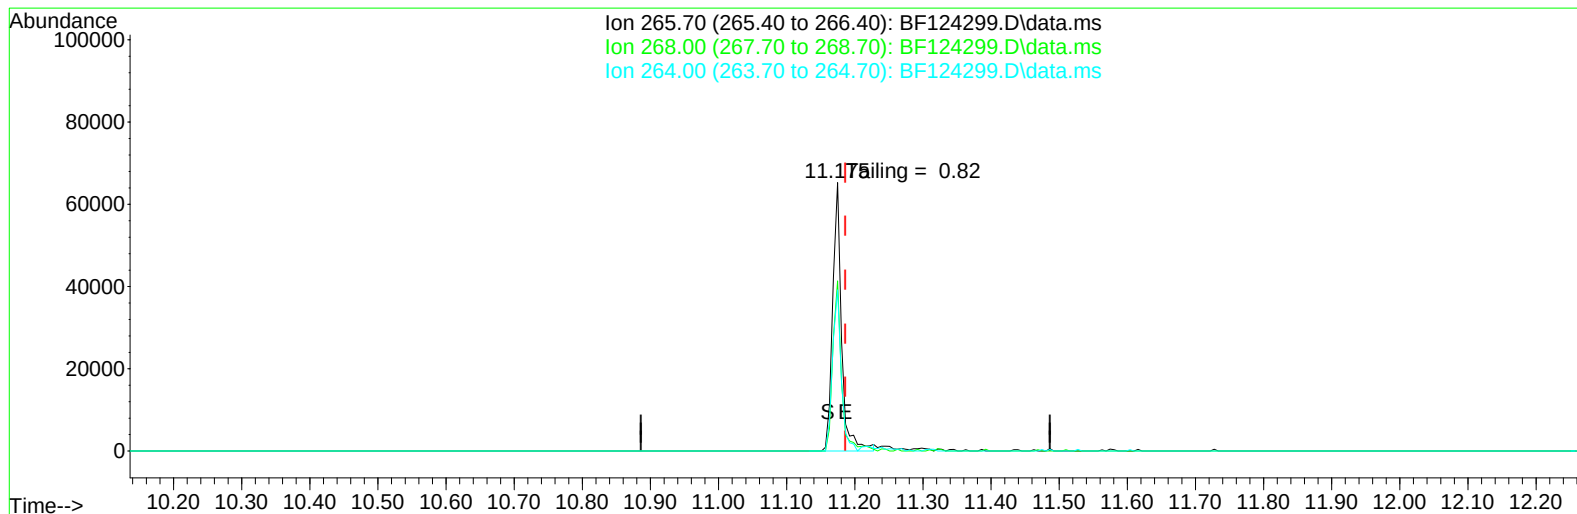

TIC: BF124299.D\data.ms

(70) Pentachlorophenol (C)

11.175min (-0.012) 23982.65 ng

response 60911

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.41
264.00	65.70	60.02
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_F
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
6/14/2021	BNA_F	<u>BF124299.D</u>
Compound Name	Response	Retention Time
DDT	177404	13.52
DDD	2602	13.22
DDE	618	12.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3220	180624	1.78