

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061422\
 Data File : BF128812.D
 Acq On : 14 Jun 2022 21:14
 Operator : CG\JU
 Sample : N3334-19
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WC-14A-1A-5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128812.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.963	451	455	460	rBV	481195	521491	6.32%	0.344%
2	5.169	484	490	493	rBV	423661	453049	5.49%	0.299%
3	5.416	528	532	536	rBV	713474	690532	8.37%	0.456%
4	5.534	549	552	557	rBV3	323070	494898	6.00%	0.327%
5	5.622	563	567	574	rVV3	348787	512369	6.21%	0.338%
6	5.792	590	596	600	rVB3	500565	787940	9.56%	0.520%
7	5.845	600	605	607	rBV	371579	501040	6.08%	0.331%
8	5.928	616	619	624	rVB3	853542	1023841	12.42%	0.676%
9	6.028	632	636	642	rVV	1869054	2259706	27.41%	1.491%
10	6.081	642	645	648	rVV	875925	740160	8.98%	0.488%
11	6.216	662	668	671	rBV2	984260	1251707	15.18%	0.826%
12	6.310	681	684	686	rBV2	1315533	1368725	16.60%	0.903%
13	6.334	686	688	692	rVB3	497209	468777	5.69%	0.309%
14	6.381	692	696	702	rBV3	366691	687713	8.34%	0.454%
15	6.434	702	705	711	rBV3	1505248	1954486	23.70%	1.290%
16	6.522	715	720	724	rBV4	863612	1554262	18.85%	1.026%
17	6.610	732	735	738	rBV3	862203	1213996	14.72%	0.801%
18	6.798	760	767	771	rVB2	1839360	2547087	30.89%	1.681%
19	6.839	771	774	777	rBV	953567	942577	11.43%	0.622%
20	6.928	786	789	793	rBV	1581233	1568318	19.02%	1.035%
21	6.963	793	795	798	rVB	638961	488294	5.92%	0.322%
22	7.016	801	804	805	rBV	539573	511193	6.20%	0.337%
23	7.057	808	811	814	rVB3	1321441	1490031	18.07%	0.983%
24	7.104	814	819	821	rBV2	692756	948442	11.50%	0.626%
25	7.181	826	832	834	rBV2	1137123	1314357	15.94%	0.867%
26	7.210	834	837	841	rVB4	396638	513574	6.23%	0.339%
27	7.322	850	856	858	rBV2	1795047	2289683	27.77%	1.511%
28	7.351	858	861	865	rVB3	827964	1011660	12.27%	0.668%
29	7.381	865	866	869	rVB2	784471	577660	7.01%	0.381%
30	7.428	869	874	878	rVB5	1179073	1788589	21.69%	1.180%
31	7.498	878	886	888	rBV5	811500	1845243	22.38%	1.218%
32	7.569	894	898	899	rBV3	742476	831400	10.08%	0.549%
33	7.592	899	902	905	rVB2	1272263	1350809	16.38%	0.891%
34	7.669	912	915	916	rBV2	638924	622280	7.55%	0.411%
35	7.686	916	918	920	rBV2	754179	513245	6.22%	0.339%
36	7.710	920	922	926	rVB4	1170986	1104572	13.40%	0.729%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061422\
 Data File : BF128812.D
 Acq On : 14 Jun 2022 21:14
 Operator : CG\JU
 Sample : N3334-19
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WC-14A-1A-5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	7.751	926	929	932	rVB3	764549	895458	10.86%	0.591%
38	7.810	936	939	947	rVB4	1141371	1666374	20.21%	1.100%
39	7.886	950	952	957	rVB5	832734	957365	11.61%	0.632%
40	7.939	958	961	965	rBV2	806974	1032000	12.52%	0.681%

41	8.010	970	973	974	rBV2	599206	591138	7.17%	0.390%
42	8.057	978	981	985	rBV4	1690948	2179597	26.43%	1.438%
43	8.133	989	994	997	rVB2	2719957	3173681	38.49%	2.094%
44	8.157	997	998	1002	rBV2	783430	634288	7.69%	0.419%
45	8.228	1006	1010	1011	rBV3	683841	779596	9.46%	0.514%

46	8.275	1015	1018	1020	rVB2	1038402	936220	11.35%	0.618%
47	8.363	1025	1033	1036	rBV5	2306342	3517063	42.66%	2.321%
48	8.416	1040	1042	1045	rBV3	846804	804589	9.76%	0.531%
49	8.451	1045	1048	1052	rVB3	1294154	1409999	17.10%	0.930%
50	8.498	1052	1056	1061	rBV2	3896623	5124331	62.15%	3.382%

51	8.533	1061	1062	1065	rVB2	963574	792957	9.62%	0.523%
52	8.580	1067	1070	1072	rBV2	852046	734778	8.91%	0.485%
53	8.616	1072	1076	1078	rBV4	1016638	1227394	14.89%	0.810%
54	8.669	1082	1085	1088	rBV3	1697316	1809420	21.95%	1.194%
55	8.728	1093	1095	1098	rVV2	1017997	1272259	15.43%	0.840%

56	8.763	1098	1101	1104	rVV3	1734660	1909403	23.16%	1.260%
57	8.786	1104	1105	1108	rVB	1124661	784633	9.52%	0.518%
58	8.851	1113	1116	1118	rBV3	609919	808040	9.80%	0.533%
59	8.886	1119	1122	1126	rVV3	1174868	1521419	18.45%	1.004%
60	8.951	1130	1133	1135	rBV3	1030251	1159657	14.06%	0.765%

61	8.980	1135	1138	1143	rVV4	1526656	2123361	25.75%	1.401%
62	9.033	1143	1147	1150	rVV4	529515	829757	10.06%	0.548%
63	9.069	1151	1153	1155	rVV3	712228	660991	8.02%	0.436%
64	9.104	1155	1159	1162	rVV	4112998	4009119	48.62%	2.646%
65	9.145	1164	1166	1169	rVB	1375312	1176344	14.27%	0.776%

66	9.233	1177	1181	1186	rBV5	1706744	2837108	34.41%	1.872%
67	9.275	1186	1188	1191	rBV3	604299	769440	9.33%	0.508%
68	9.351	1198	1201	1204	rVB	1266150	1371235	16.63%	0.905%
69	9.422	1209	1213	1216	rVB2	2199304	2797203	33.93%	1.846%
70	9.492	1222	1225	1227	rBV	2414623	2466375	29.91%	1.628%

71	9.522	1227	1230	1232	rVV3	1655808	1667803	20.23%	1.101%
72	9.557	1232	1236	1239	rVV2	4264930	5053714	61.29%	3.335%
73	9.610	1243	1245	1247	rBV	1188124	931137	11.29%	0.614%
74	9.692	1257	1259	1264	rBV2	1155735	1525721	18.50%	1.007%
75	9.739	1264	1267	1270	rBV3	1168270	1106084	13.41%	0.730%

76	9.769	1270	1272	1276	rBV2	793963	797474	9.67%	0.526%
----	-------	------	------	------	------	--------	--------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061422\
 Data File : BF128812.D
 Acq On : 14 Jun 2022 21:14
 Operator : CG\JU
 Sample : N3334-19
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WC-14A-1A-5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	9.810	1276	1279	1281	rBV3	1368927	1731675	21.00%	1.143%
78	9.869	1288	1289	1291	rVB	744134	456879	5.54%	0.301%
79	9.939	1298	1301	1305	rVB	1671453	1945634	23.60%	1.284%
80	9.992	1305	1310	1314	rBV6	846894	1929464	23.40%	1.273%
81	10.033	1314	1317	1322	rVB3	1733604	2333596	28.30%	1.540%
82	10.080	1322	1325	1326	rBV	1901877	1564456	18.97%	1.032%
83	10.151	1334	1337	1340	rBV2	1681586	1944926	23.59%	1.283%
84	10.180	1340	1342	1344	rVV	914897	819670	9.94%	0.541%
85	10.245	1349	1353	1354	rBV2	1671440	1715884	20.81%	1.132%
86	10.263	1354	1356	1359	rVB2	1109845	859348	10.42%	0.567%
87	10.292	1359	1361	1364	rBV2	598817	681305	8.26%	0.450%
88	10.322	1364	1366	1371	rVB5	905661	1331325	16.15%	0.879%
89	10.380	1373	1376	1377	rBV2	974051	967137	11.73%	0.638%
90	10.492	1389	1395	1398	rBV	4293057	4987855	60.49%	3.291%
91	10.539	1400	1403	1407	rVB3	1119994	1597246	19.37%	1.054%
92	10.580	1407	1410	1412	rBV4	744737	917997	11.13%	0.606%
93	10.604	1412	1414	1416	rVB2	1126640	820785	9.95%	0.542%
94	10.763	1436	1441	1447	rBV	5593837	8245224	100.00%	5.441%
95	10.821	1449	1451	1456	rBV4	665083	897680	10.89%	0.592%
96	11.086	1491	1496	1500	rBV5	1169776	1745671	21.17%	1.152%
97	11.233	1517	1521	1526	rVB	4214549	5250170	63.68%	3.465%
98	11.333	1535	1538	1539	rBV2	887011	961225	11.66%	0.634%
99	11.580	1577	1580	1583	rVB2	1375053	1360521	16.50%	0.898%
100	12.321	1704	1706	1711	rVB	1585508	1884786	22.86%	1.244%




Sum of corrected areas: 151538690

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061422\
Data File : BF128812.D
Acq On : 14 Jun 2022 21:14
Operator : CG\JU
Sample : N3334-19
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-14A-1A-5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

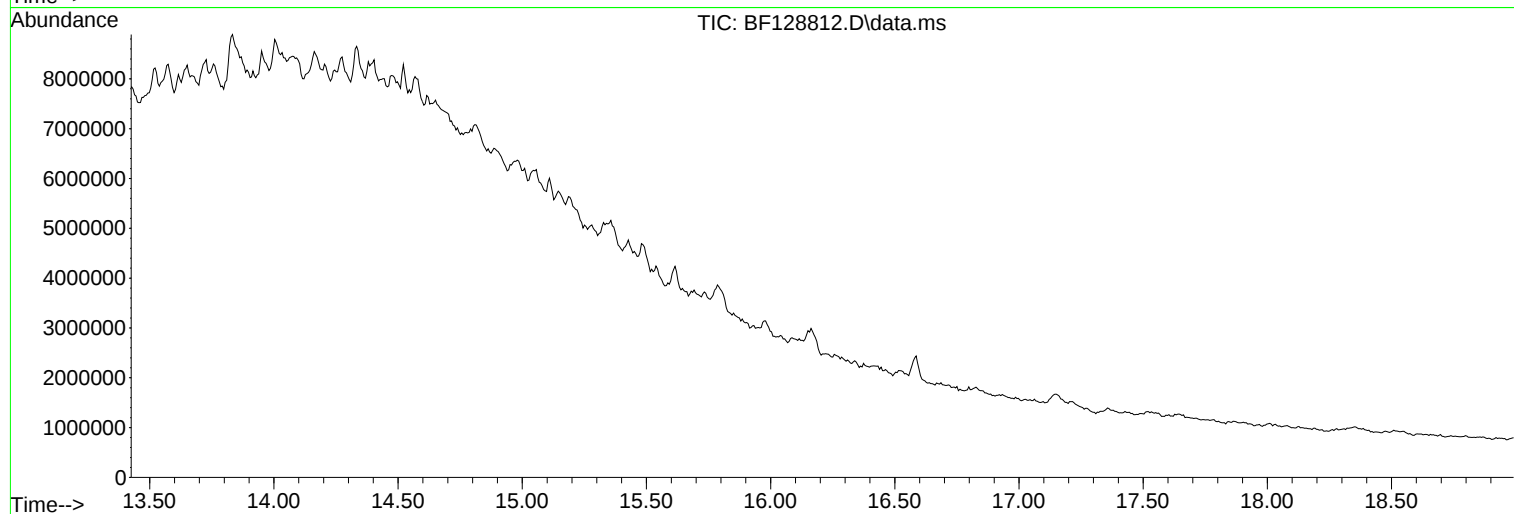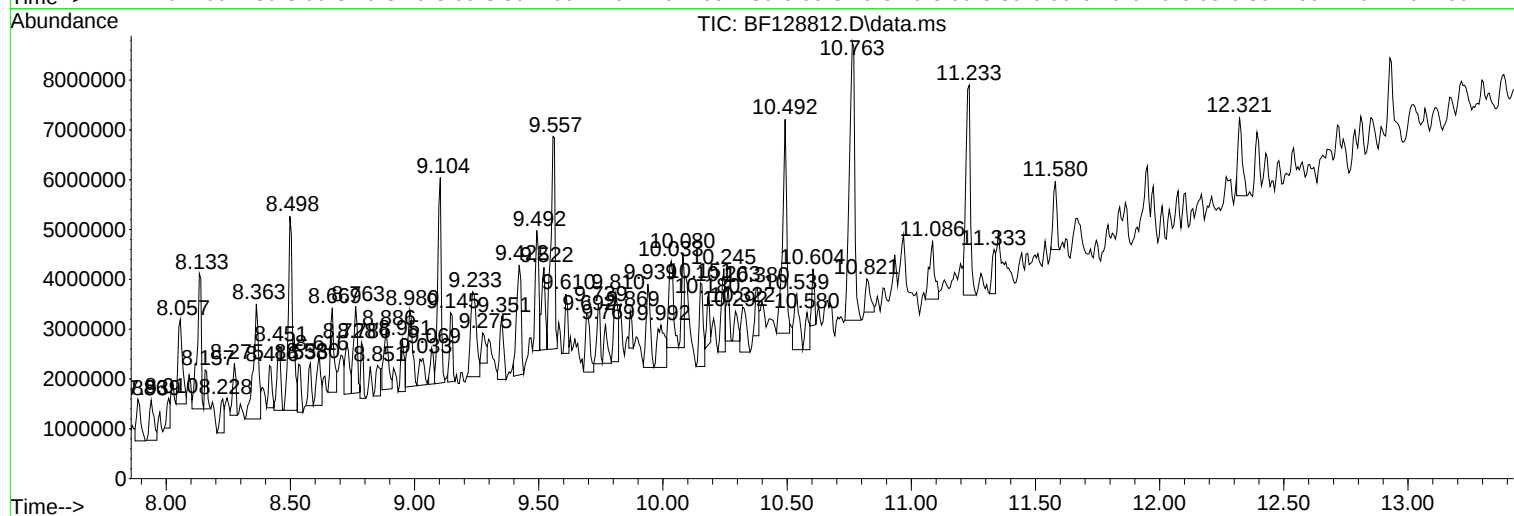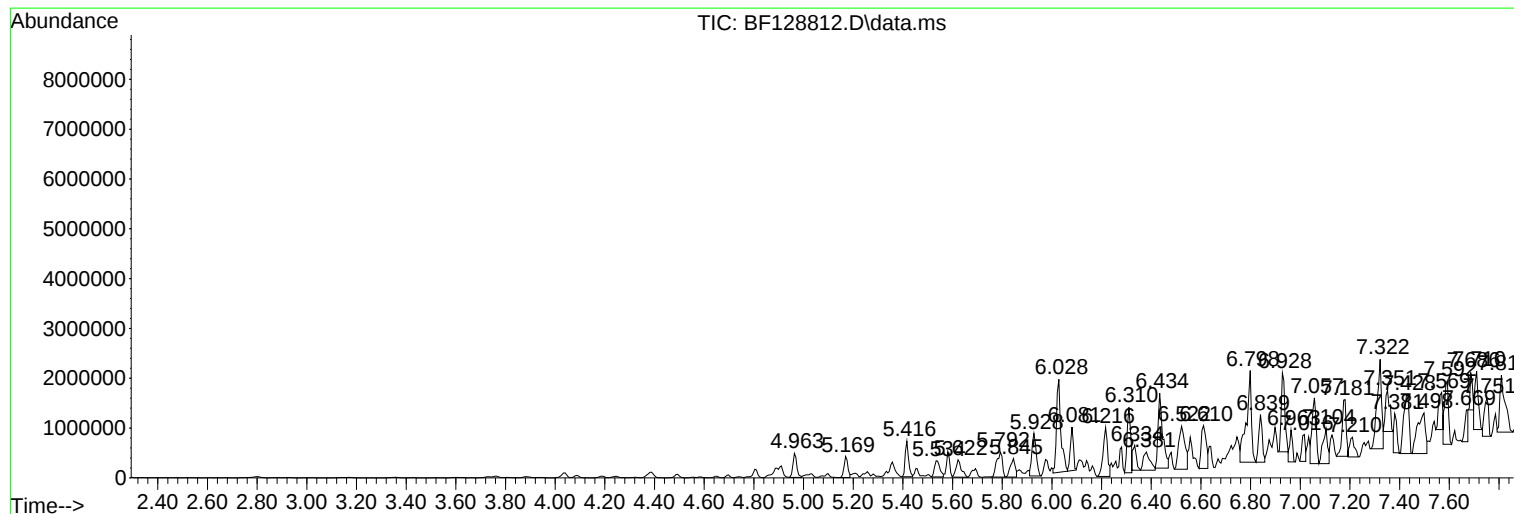

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061422\
Data File : BF128812.D
Acq On : 14 Jun 2022 21:14
Operator : CG\JU
Sample : N3334-19
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-14A-1A-5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061422\
Data File : BF128812.D
Acq On : 14 Jun 2022 21:14
Operator : CG\JU
Sample : N3334-19
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-14A-1A-5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------