
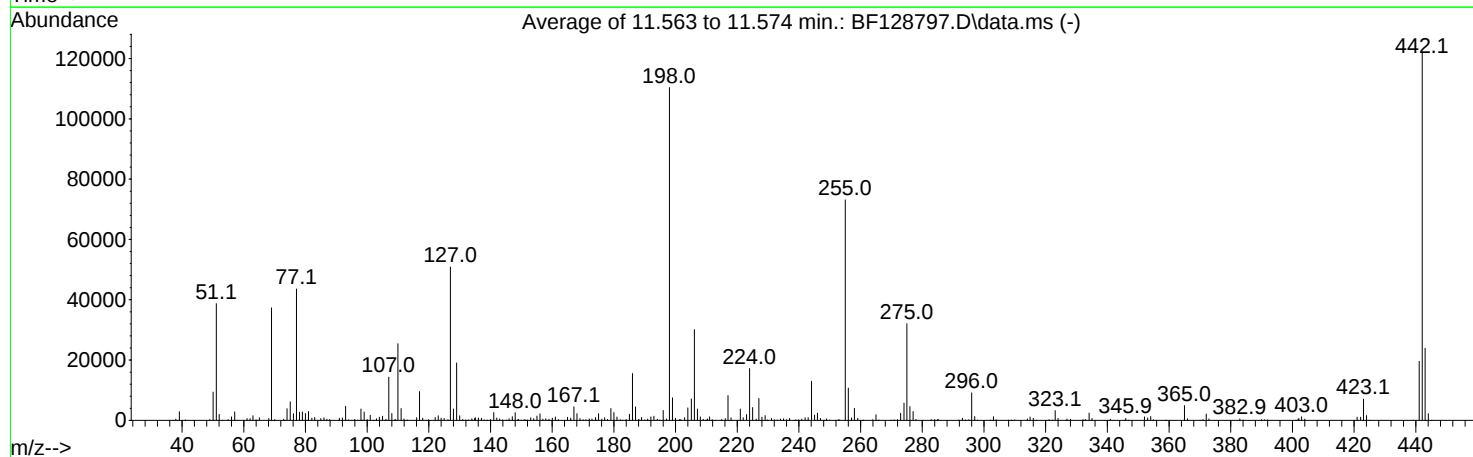


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061422\
 Data File : BF128797.D
 Acq On : 14 Jun 2022 12:24
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 14 14:53:53 2022

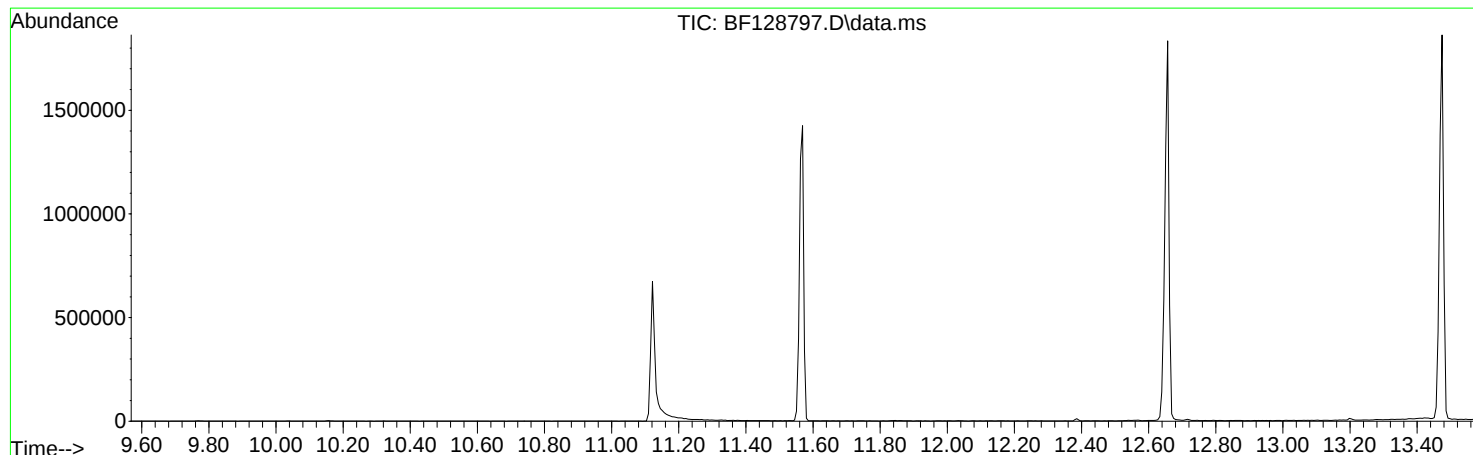




AutoFind: Scans 1577, 1578, 1579; Background Corrected with Scan 1571

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	38745	PASS
68	69	0.00	2	1.6	611	PASS
69	198	0.00	100	33.8	37324	PASS
70	69	0.00	2	0.7	248	PASS
127	198	10	80	46.0	50824	PASS
197	198	0.00	2	0.5	505	PASS
198	198	100	100	100.0	110371	PASS
199	198	5	9	6.8	7468	PASS
275	198	10	60	29.0	32033	PASS
365	198	1	100	4.4	4879	PASS
441	198	0.01	100	17.7	19572	PASS
442	442	50	100	100.0	122003	PASS
443	442	15	24	19.6	23937	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061422\
Data File : BF128797.D
Acq On : 14 Jun 2022 12:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 15 03:59:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 14 14:53:53 2022
Response via : Initial Calibration

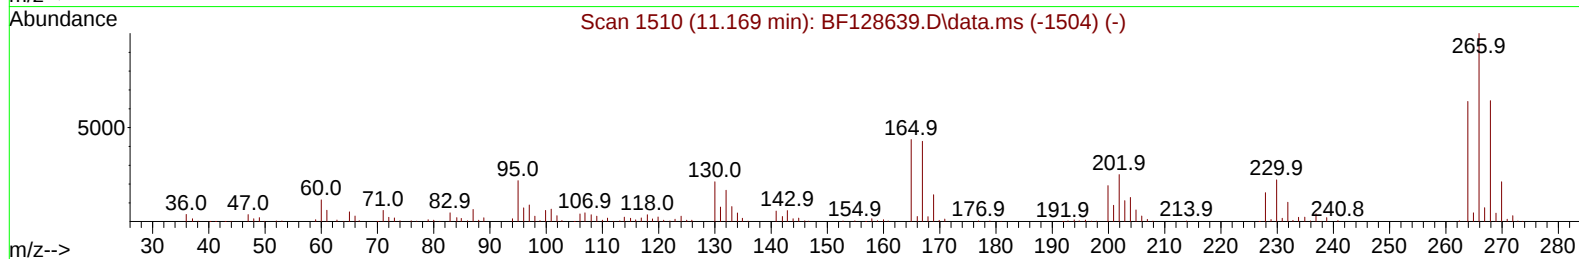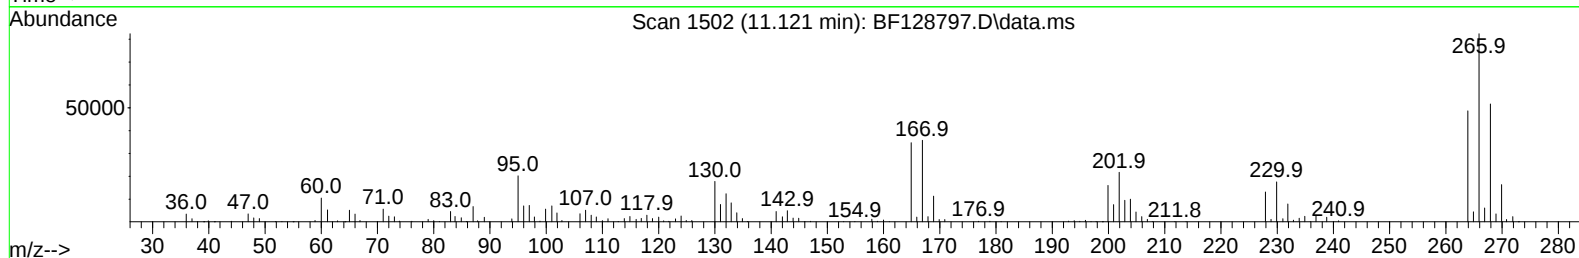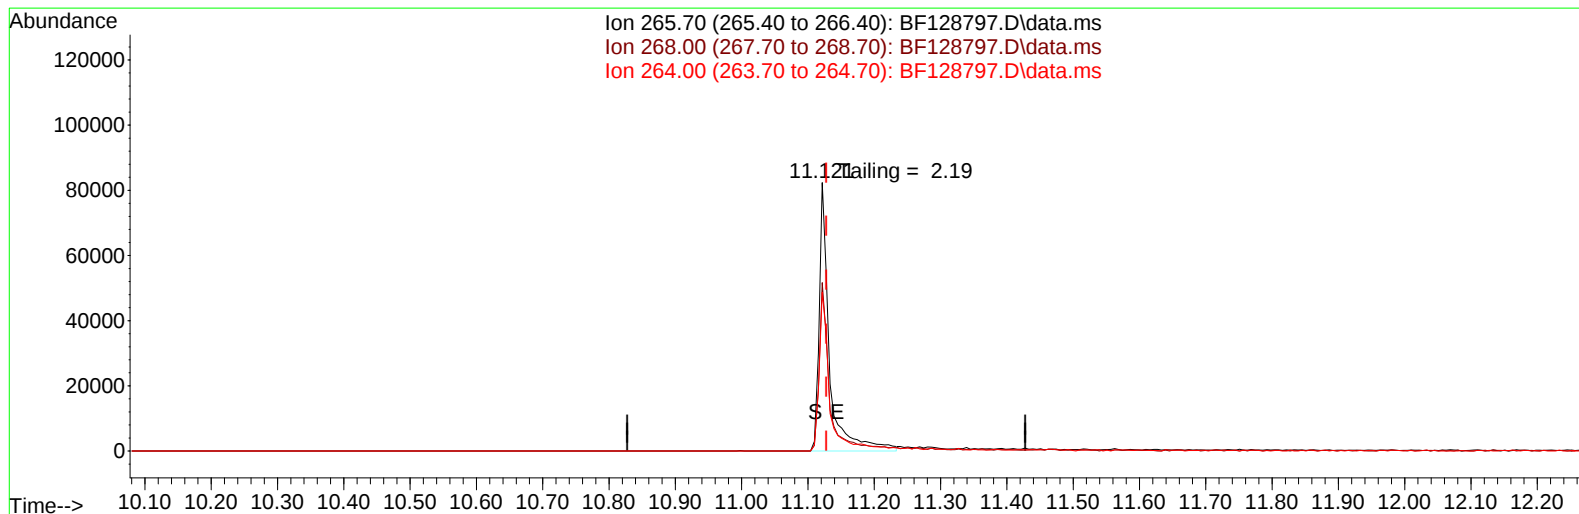

TIC: BF128797.D\data.ms

(70) Pentachlorophenol (C)

11.121min (-0.006) 31479.64 ng




response 91858

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	62.73
264.00	61.80	59.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061422\
 Data File : BF128797.D
 Acq On : 14 Jun 2022 12:24
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jun 15 03:59:44 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 14 14:53:53 2022
 Response via : Initial Calibration

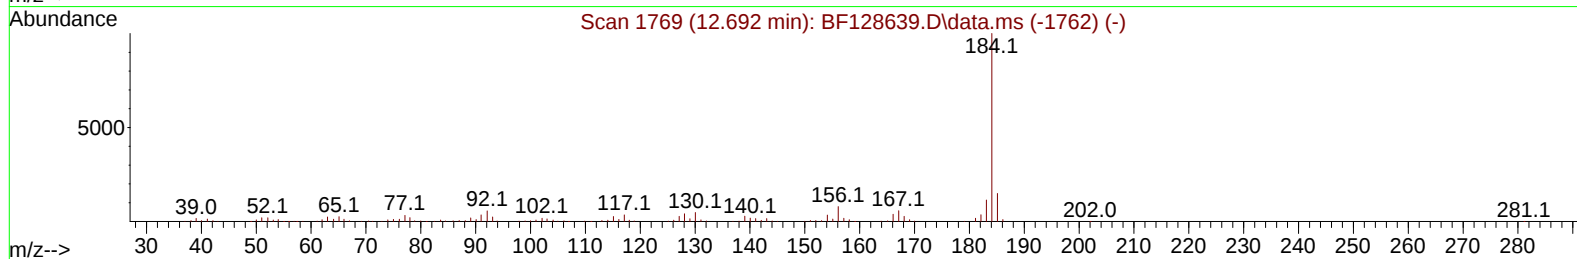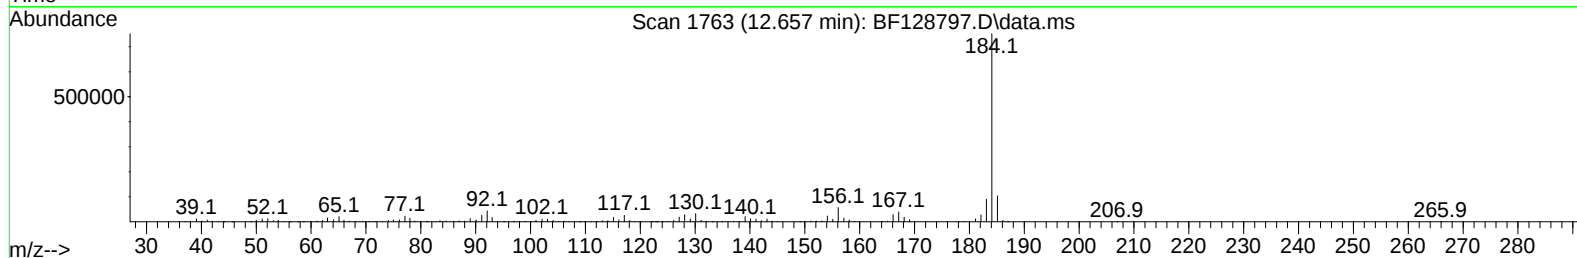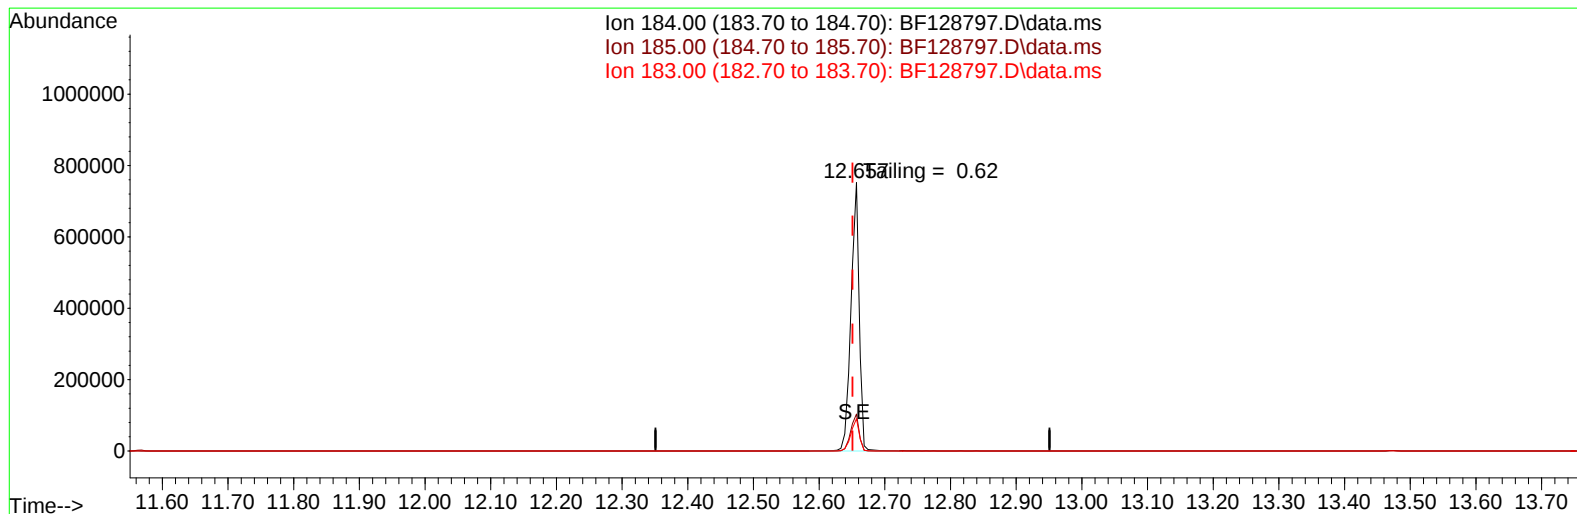

TIC: BF128797.D\data.ms

(77) Benzidine

12.657min (+ 0.006) 0.00 ng

response 653412

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	13.80
183.00	11.60	12.06
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/14/2022	BNA_F	<u>BF128797.D</u>
Compound Name	Response	Retention Time
DDT	303916	13.474
DDD	2163	13.198
DDE	157	12.839
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2320	306236	0.76

Instrument :
BNA_F
ClientSampleId :
DFTPP