
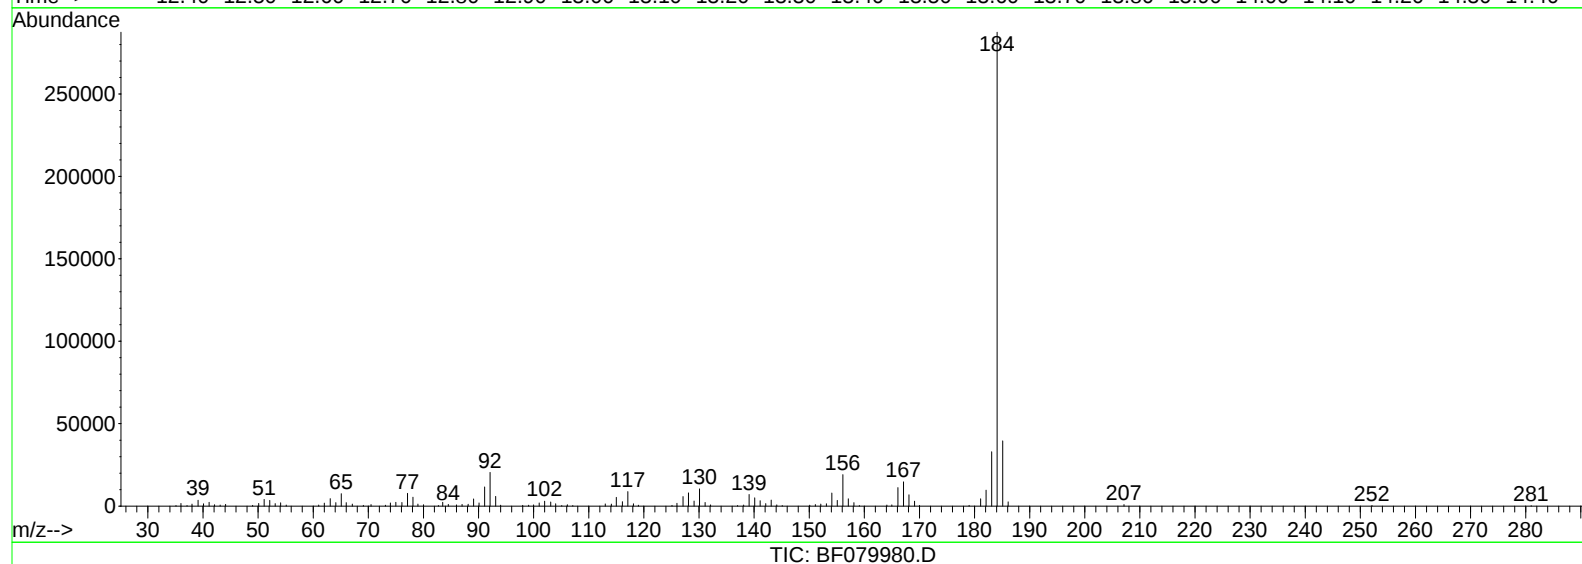


```

Data Path   : Z:\HPCHEM1\BNA F\Data\BF061515\
Data File   : BF079980.D
Acq On      : 15 Jun 2015   11:29
Operator    : TP/IZ
Sample      : DFTPP
Misc        :
ALS Vial    : 1      Sample Multiplier: 1

```

Quant Time: Jun 16 04:29:44 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF061115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 15 15:44:31 2015
Response via : Initial Calibration

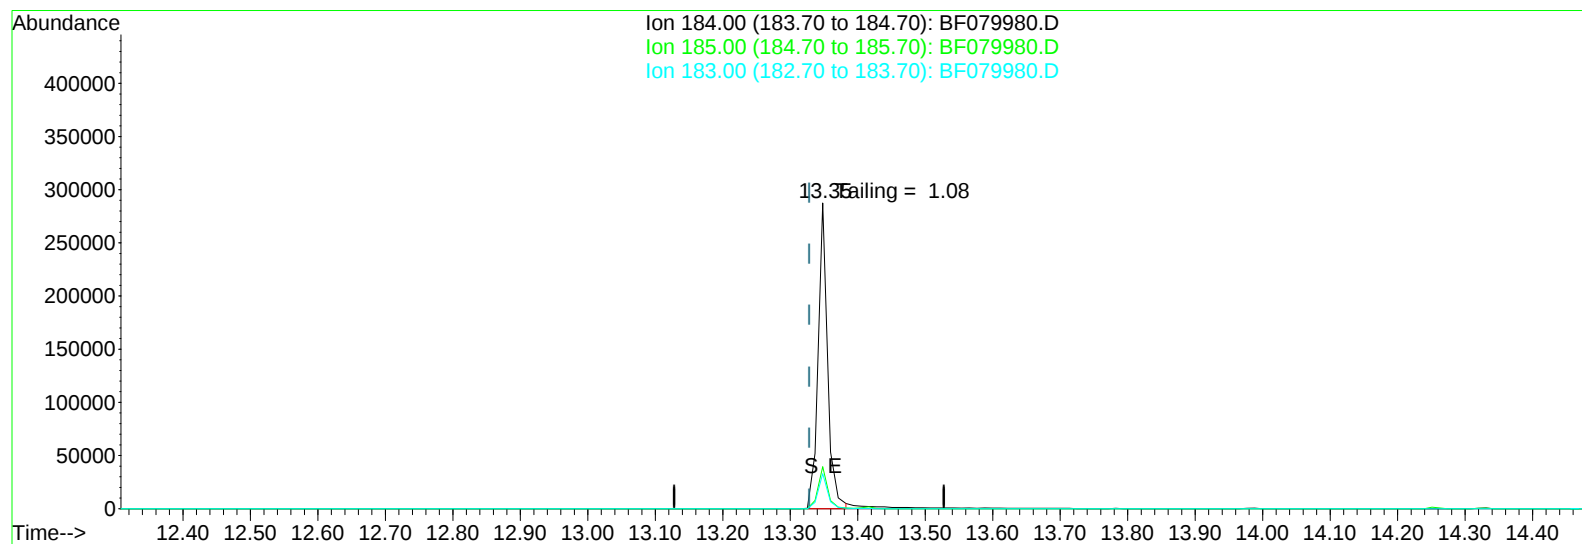

(76) Benzidine



13.348min (+0.020) 0.00ng

response 290300

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	13.75
183.00	11.30	11.46
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF061515\
Data File : BF079980.D
Acq On : 15 Jun 2015 11:29
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 16 04:29:44 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF061115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 15 15:44:31 2015
Response via : Initial Calibration

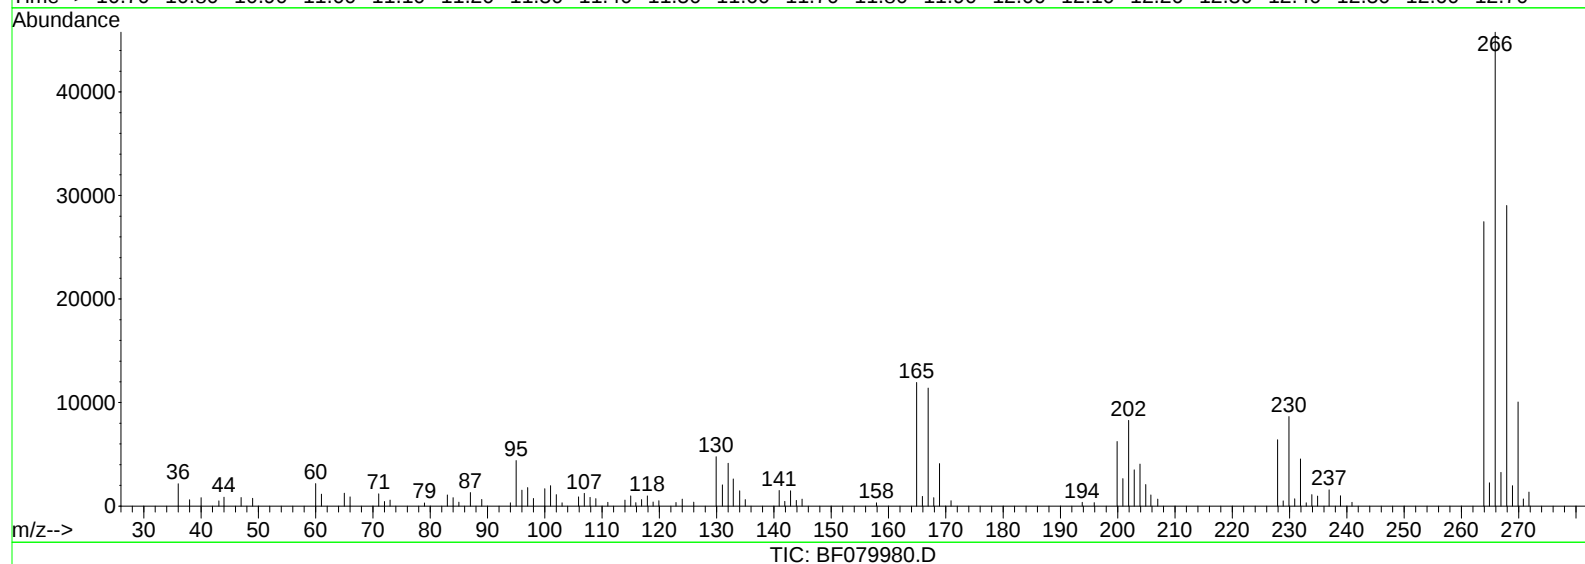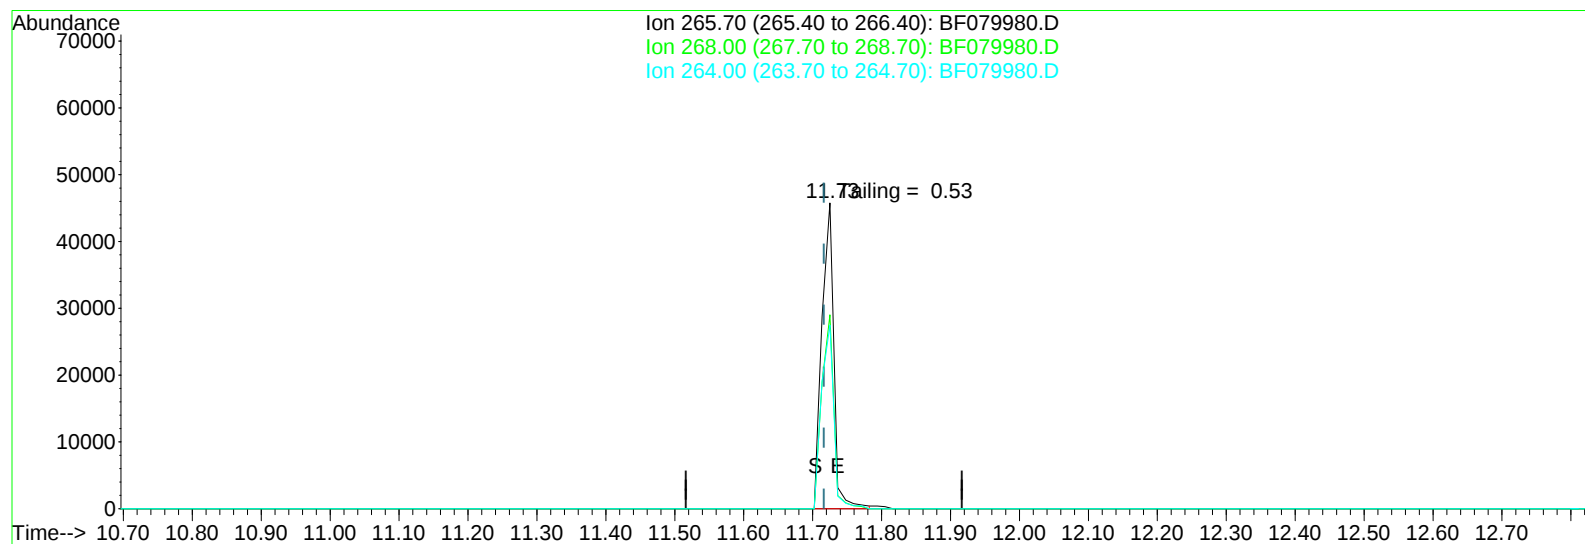

(69) Pentachlorophenol (C)

11.725min (+0.009) 0.00ng

response 55812

Ion	Exp%	Act%
265.70	100	100
268.00	61.80	63.42
264.00	59.60	60.00
0.00	0.00	0.00