

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061515\
 Data File : BF079986.D
 Acq On : 15 Jun 2015 18:15
 Operator : TP/IZ
 Sample : G2639-10
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SP15-JMW0801B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.567	215	217	224	rVB	79598	83435	3.56%	0.708%
2	5.956	249	251	254	rBV	491104	505475	21.58%	4.287%
3	6.950	335	338	340	rBV	400916	322539	13.77%	2.736%
4	7.122	350	353	355	rBV	906661	1066142	45.51%	9.043%
5	7.350	371	373	376	rBV	337454	278870	11.91%	2.365%
6	7.510	385	387	389	rVB	1397106	1126521	48.09%	9.555%
7	7.910	419	422	424	rBV	861856	824543	35.20%	6.994%
8	8.642	484	486	488	rBV	470087	372362	15.90%	3.158%
9	9.716	578	580	583	rVB	2307421	1855568	79.21%	15.739%
10	10.105	612	614	616	rBV	39127	30091	1.28%	0.255%
11	10.413	639	641	644	rBV	539801	444154	18.96%	3.767%
12	11.202	708	710	713	rBV2	946602	1087936	46.44%	9.228%
13	11.922	771	773	775	rBV	558555	482732	20.61%	4.094%
14	13.602	918	920	923	rBV	1903691	2342446	100.00%	19.868%
15	14.837	1025	1028	1029	rBV	48188	50588	2.16%	0.429%
16	14.871	1029	1031	1034	rVV	452933	467323	19.95%	3.964%
17	16.745	1192	1195	1202	rBV	301785	449107	19.17%	3.809%


Sum of corrected areas: 11789832

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061515\
Data File : BF079986.D
Acq On : 15 Jun 2015 18:15
Operator : TP/IZ
Sample : G2639-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP15-JMW0801B

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

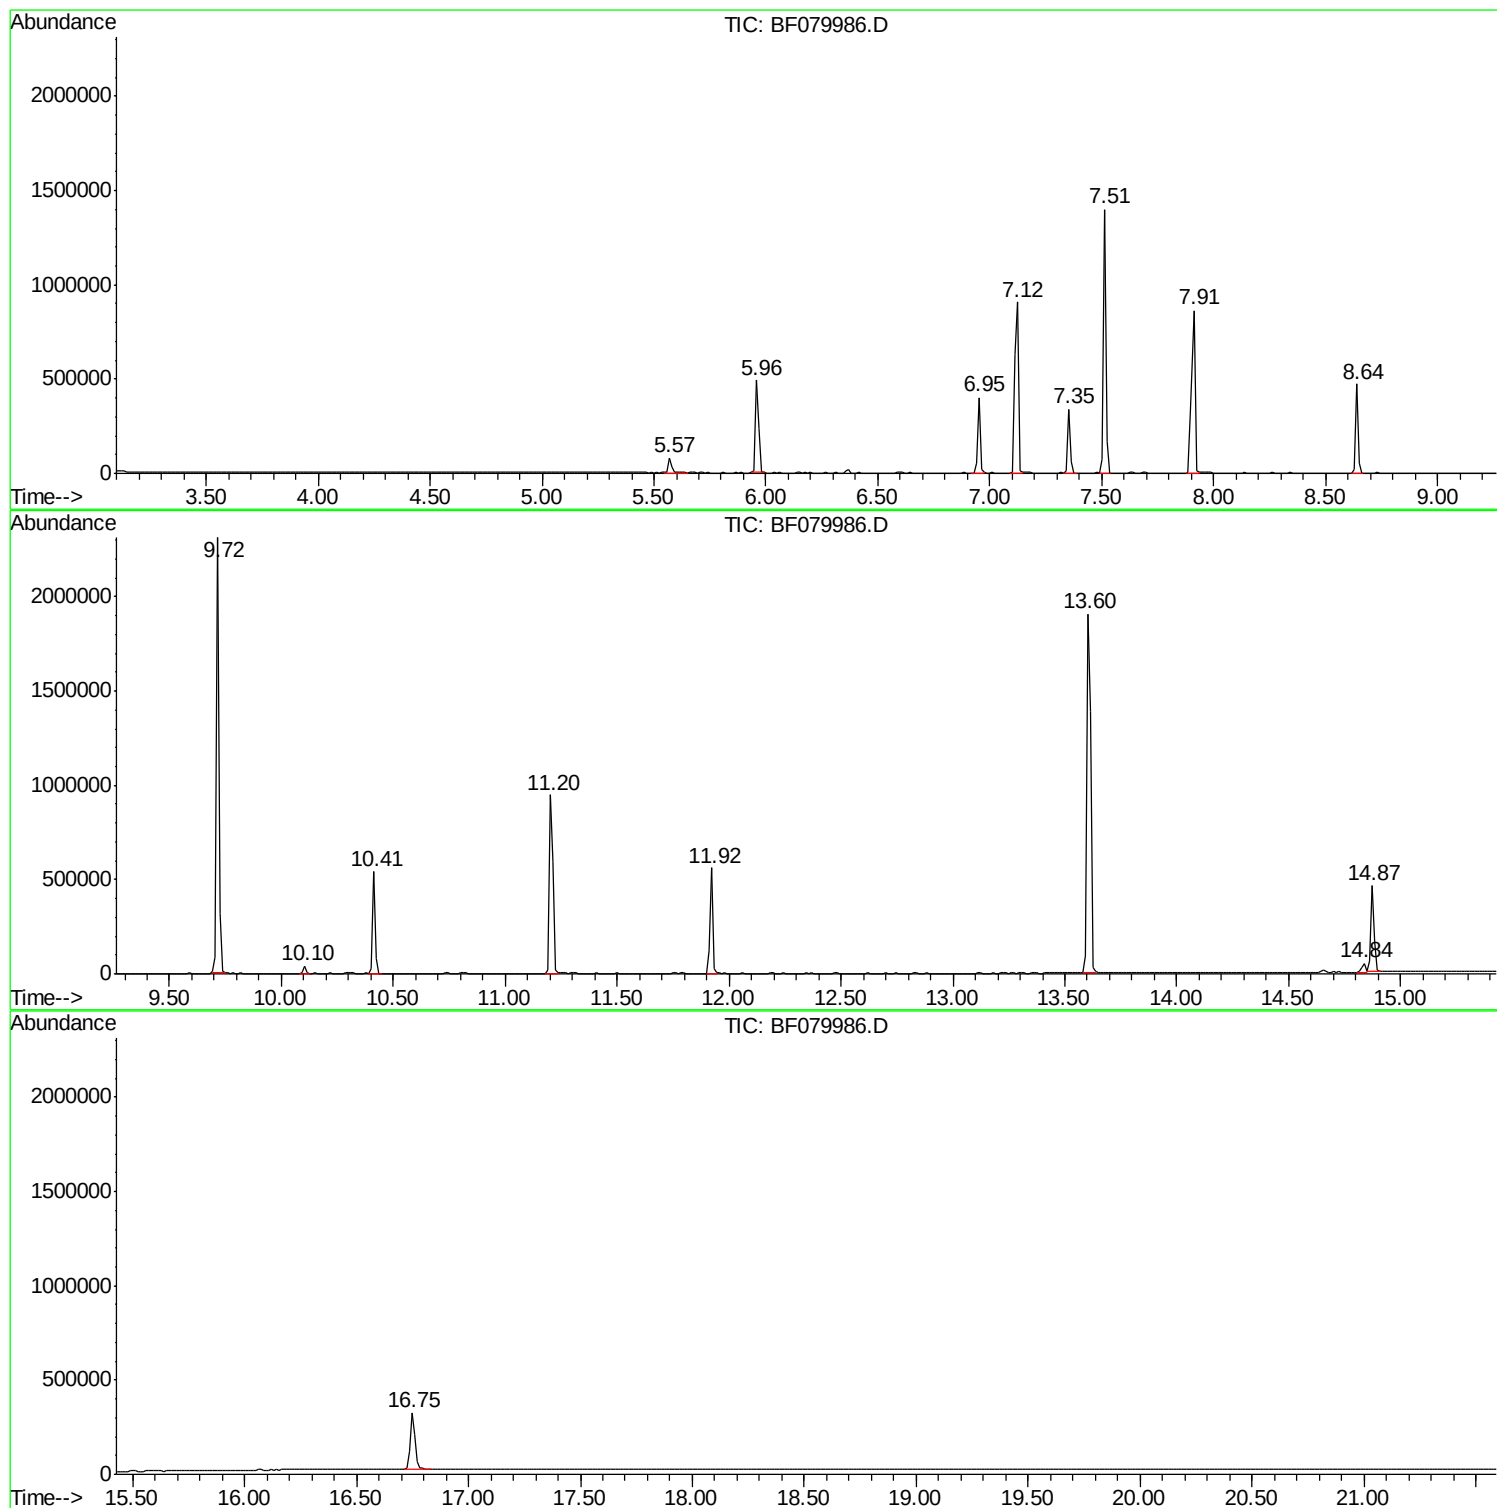

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061515\
Data File : BF079986.D
Acq On : 15 Jun 2015 18:15
Operator : TP/IZ
Sample : G2639-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP15-JMW0801B










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.57	5.98 ng	83435	1,4-Dichlorobenzene-d4	7.35

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	59
2		Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	28
3		2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	16
4		Formamide, N,N-diethyl-	101	C5H11NO	000617-84-5	9
5		1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	9

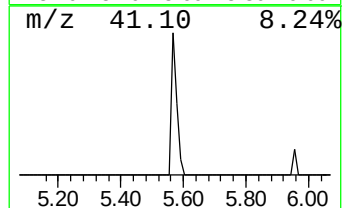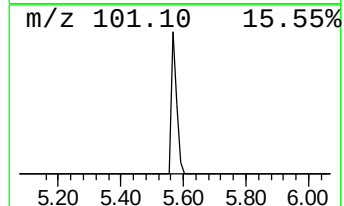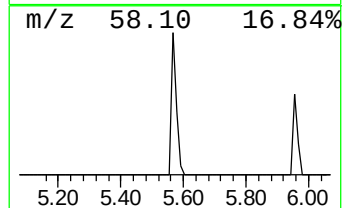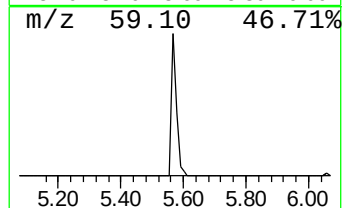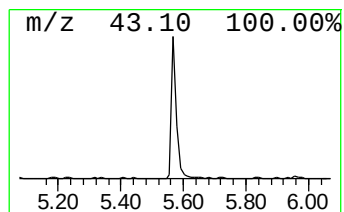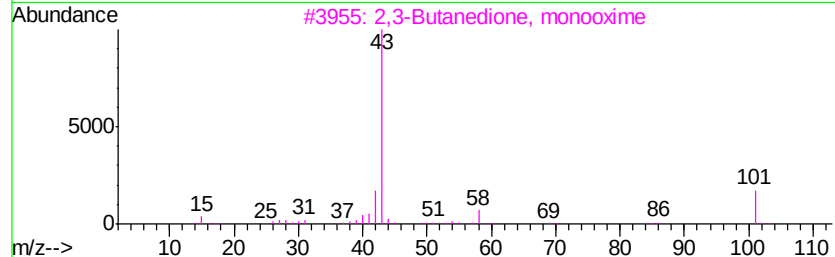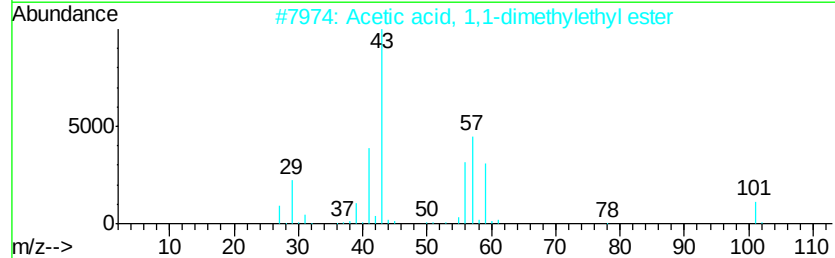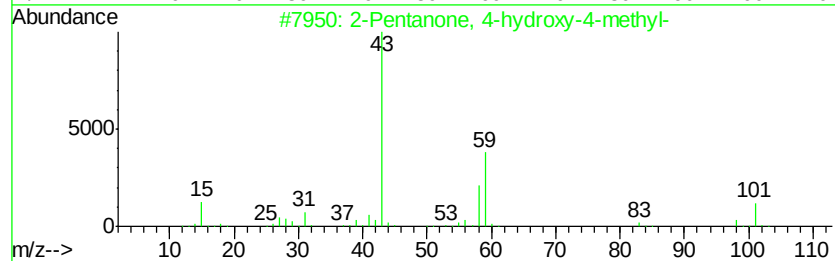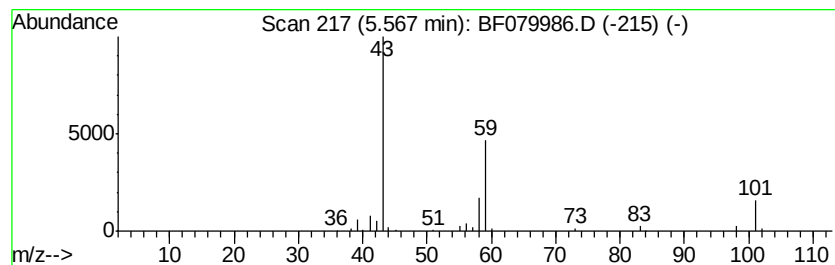

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061515\
Data File : BF079986.D
Acq On : 15 Jun 2015 18:15
Operator : TP/IZ
Sample : G2639-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP15-JMW0801B










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.12 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.12	76.46 ng	1066140	1,4-Dichlorobenzene-d4	7.35

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	38
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		Xenon	132	Xe	007440-63-3	9
5		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9

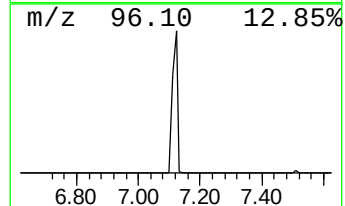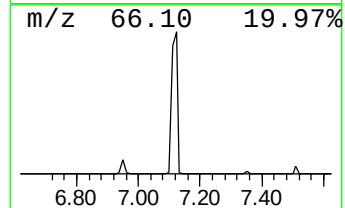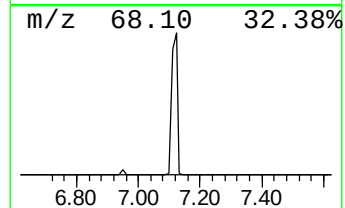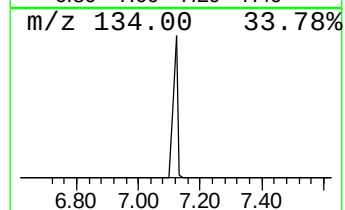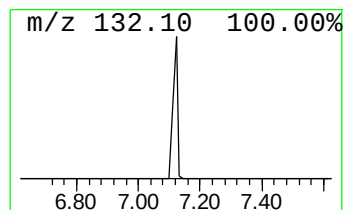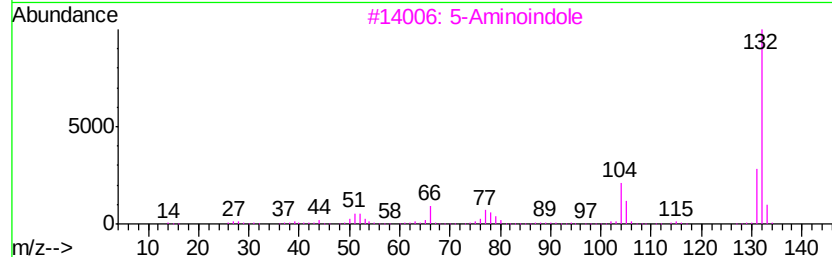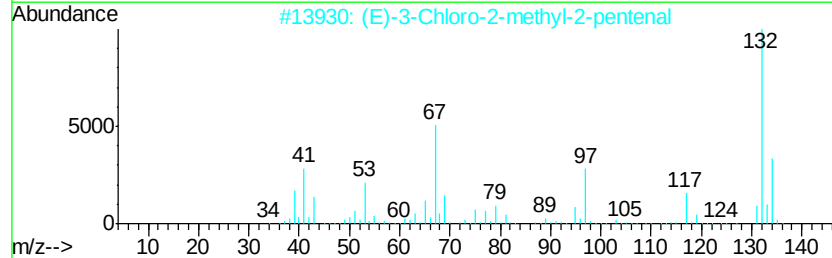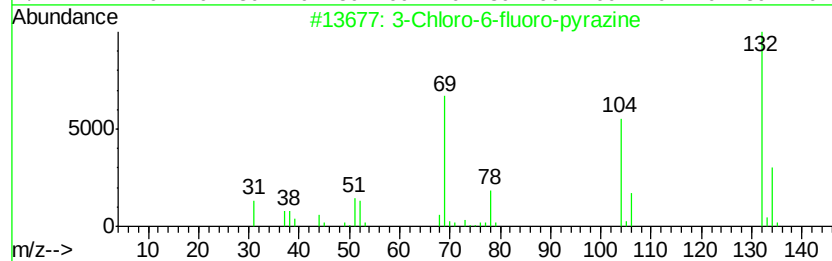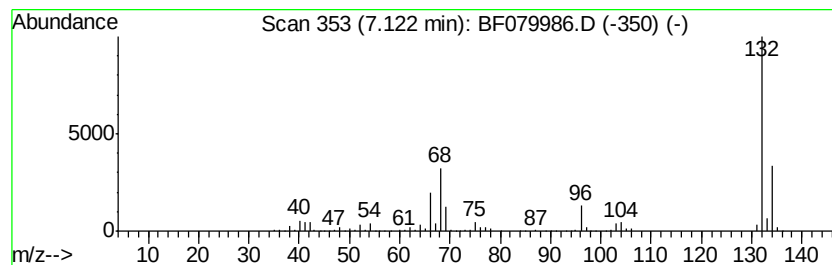

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061515\
Data File : BF079986.D
Acq On : 15 Jun 2015 18:15
Operator : TP/IZ
Sample : G2639-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP15-JMW0801B

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.57	6.0	ng	83435	1	7.35	278870	20.0
unknown7.12	7.12	76.5	ng	1066140	1	7.35	278870	20.0