


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061515\
 Data File : BF079980.D
 Acq On : 15 Jun 2015 11:29
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 15 15:44:31 2015

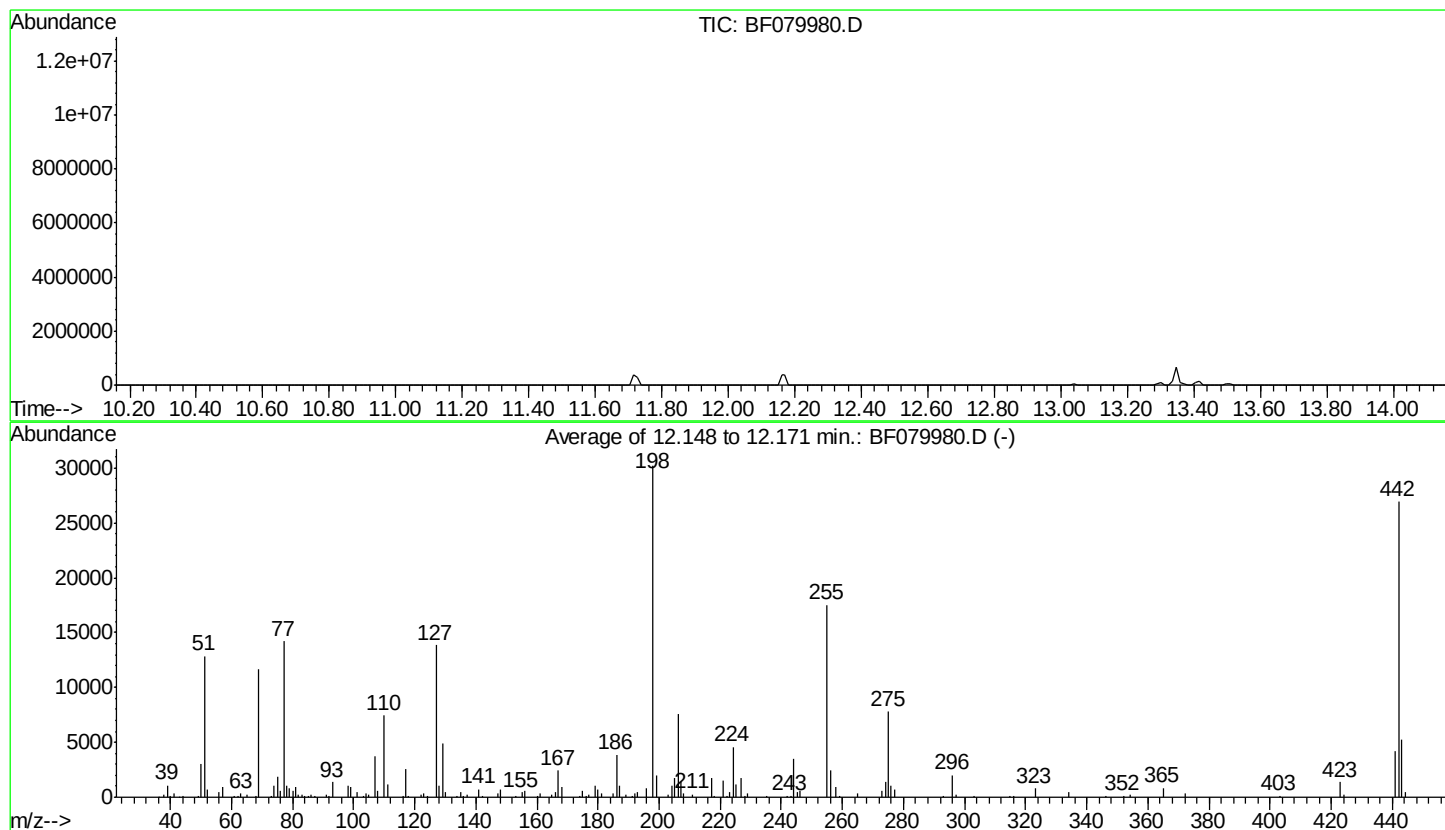

AutoFind: Scans 959, 960, 961; Background Corrected with Scan 957

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.6	12872	PASS
68	69	0.00	2	1.5	176	PASS
69	198	0.00	100	38.6	11664	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.8	13842	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	30224	PASS
199	198	5	9	6.6	2003	PASS
275	198	10	60	25.8	7789	PASS
365	198	1	100	2.8	859	PASS
441	442	0.01	24	15.4	4157	PASS
442	198	50	100	89.1	26934	PASS
443	442	15	24	19.3	5210	PASS