
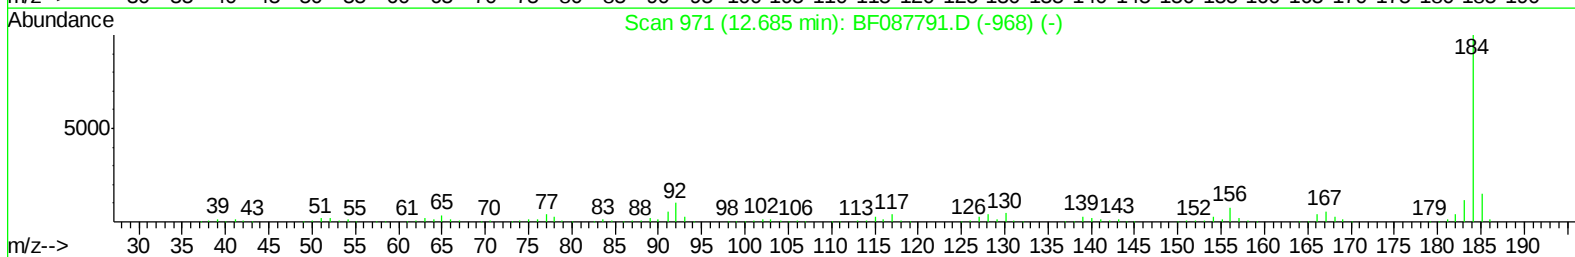
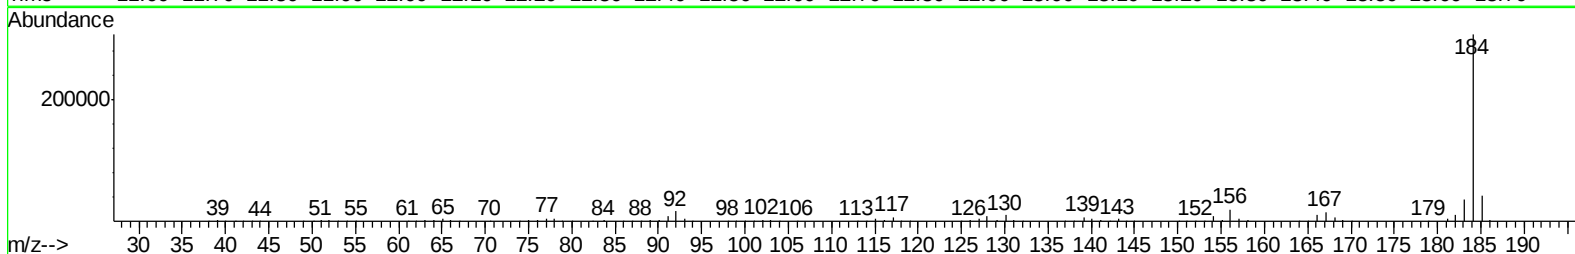


Data Path : Z:\HPCHEM1\BNA F\DATA\BF061516\
Data File : BF088039.D
Acq On : 15 Jun 2016 16:13
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 16 11:35:41 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 13 14:10:49 2016
Response via : Initial Calibration

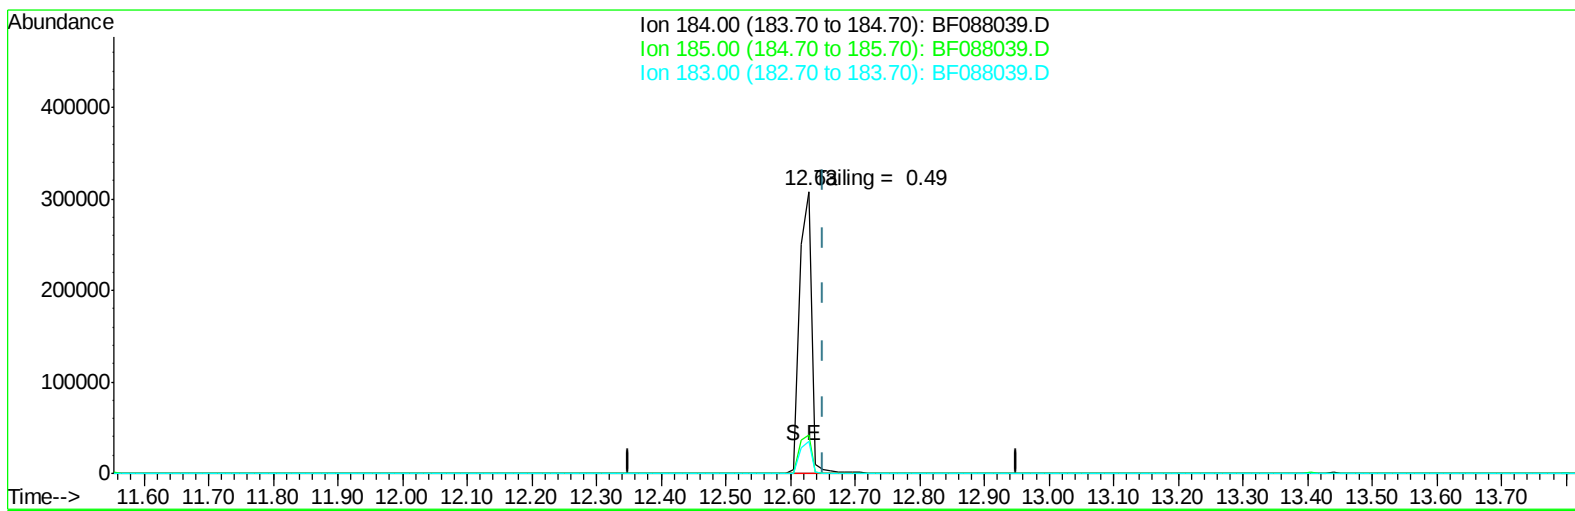

TIC: BF088039.D

(76) Benzidine




12.628min (-0.023) 0.00ng

response 402950

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	13.83
183.00	11.60	11.52
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF061516\
Data File : BF088039.D
Acq On : 15 Jun 2016 16:13
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 16 11:35:41 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 13 14:10:49 2016
Response via : Initial Calibration

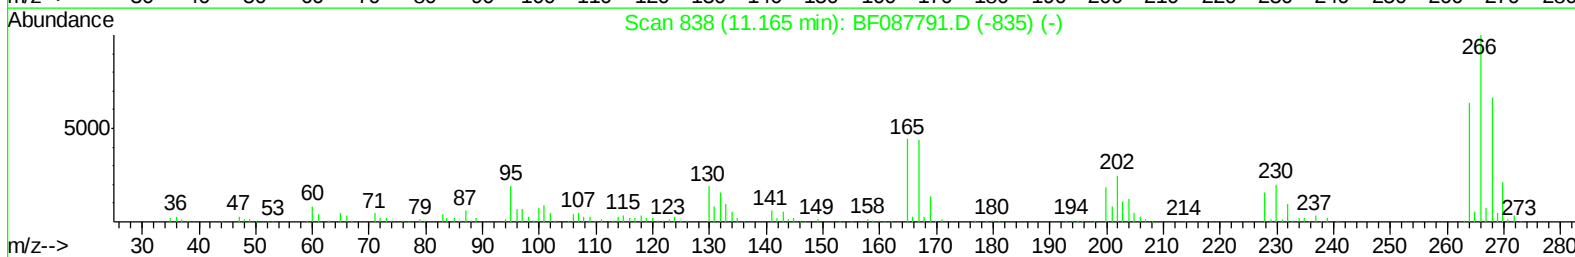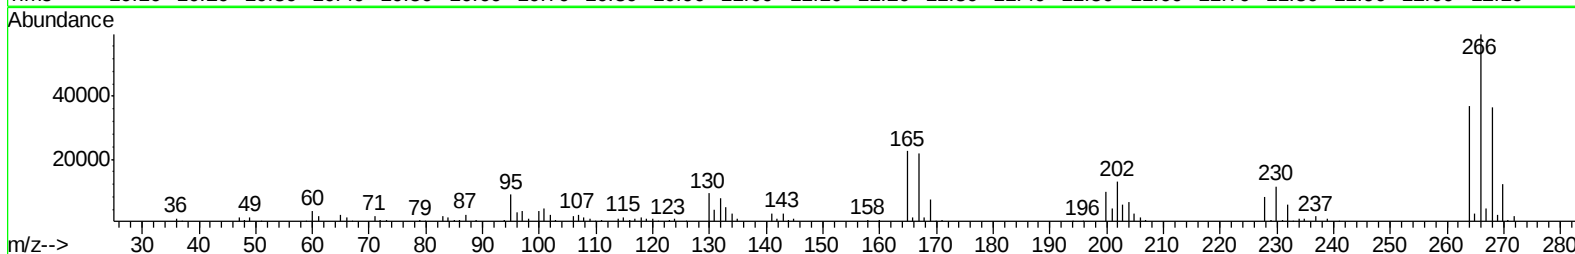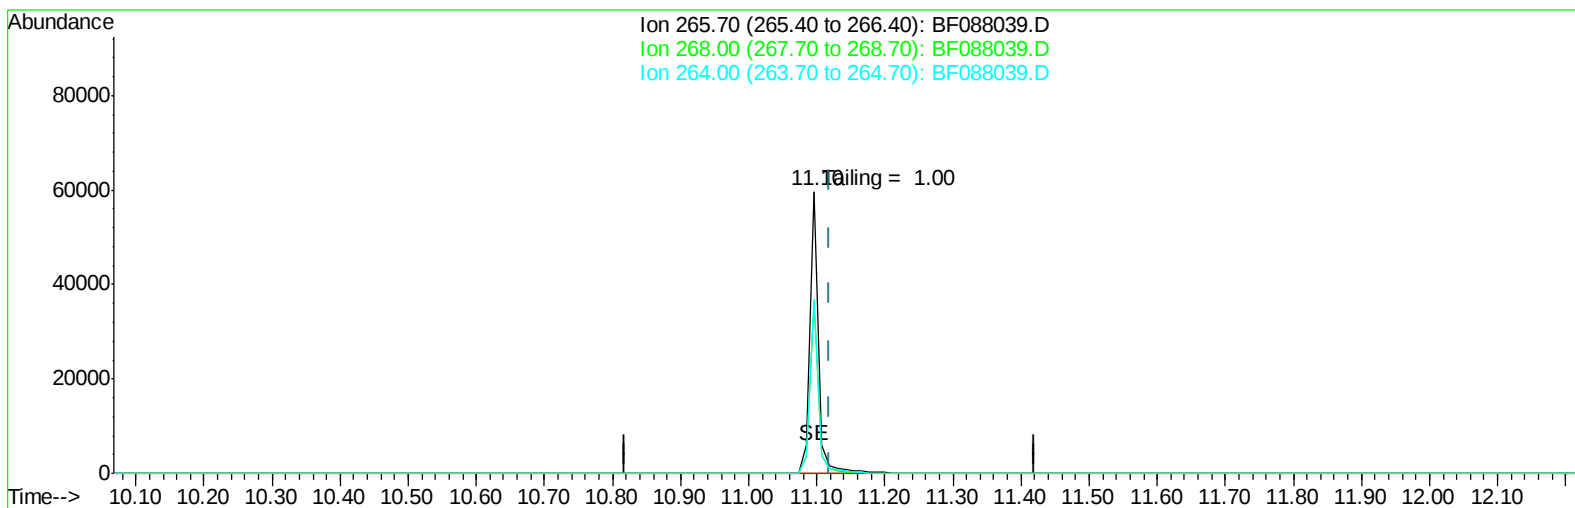

TIC: BF088039.D

(69) Pentachlorophenol (C)

11.096min (-0.023) 40199.66ng

response 52910

Ion	Exp%	Act%
265.70	100	100
268.00	66.00	61.41
264.00	62.00	61.99
0.00	0.00	0.00