
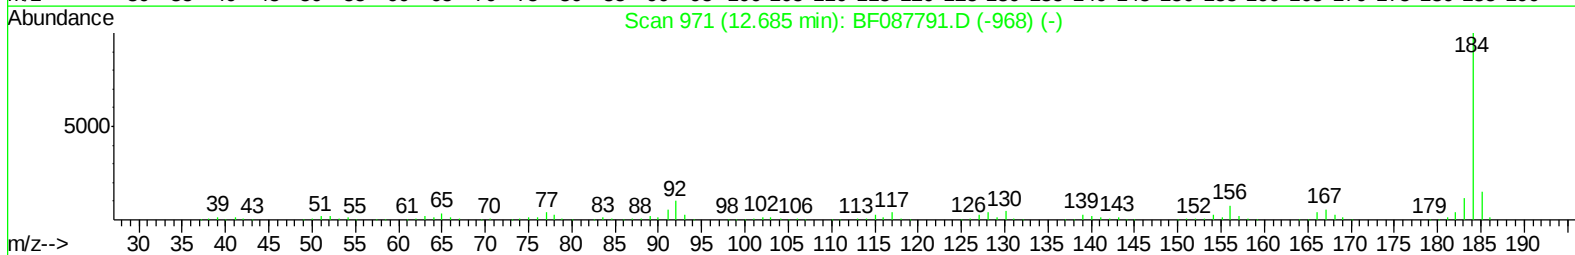
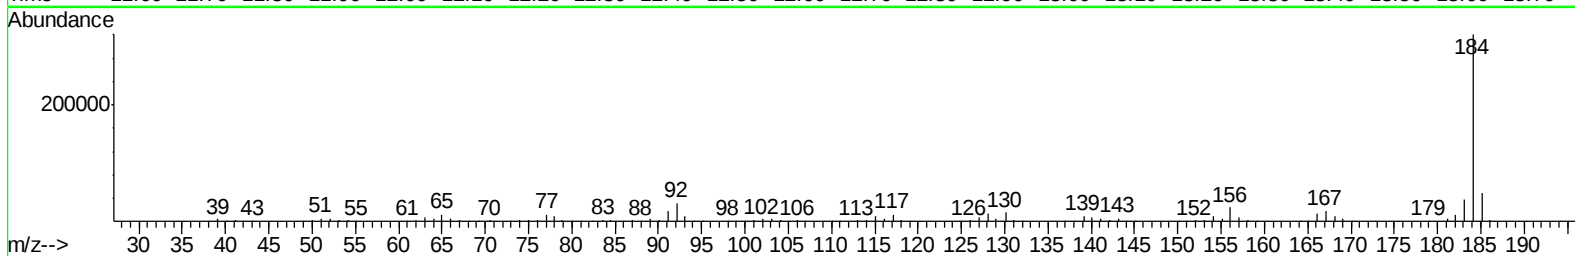


Data Path : Z:\HPCHEM1\BNA F\DATA\BF061516\
Data File : BF088058.D
Acq On : 16 Jun 2016 2:58
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 16 14:00:48 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 13 14:10:49 2016
Response via : Initial Calibration

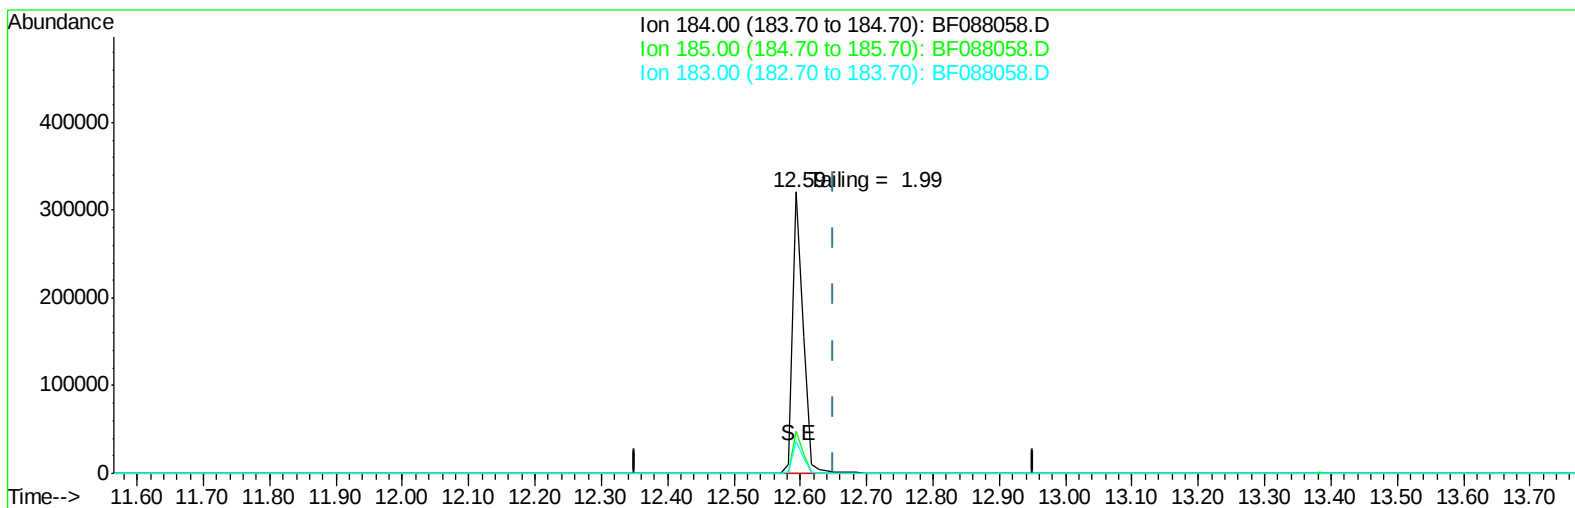

TIC: BF088058.D

(76) Benzidine




12.594min (-0.057) 0.00ng

response 350312

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	15.09
183.00	11.60	11.53
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF061516\
Data File : BF088058.D
Acq On : 16 Jun 2016 2:58
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 16 14:00:48 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 13 14:10:49 2016
Response via : Initial Calibration

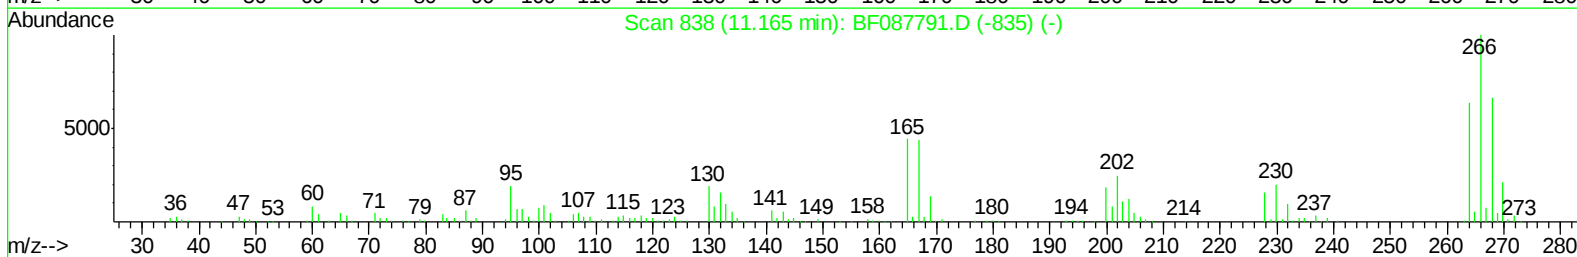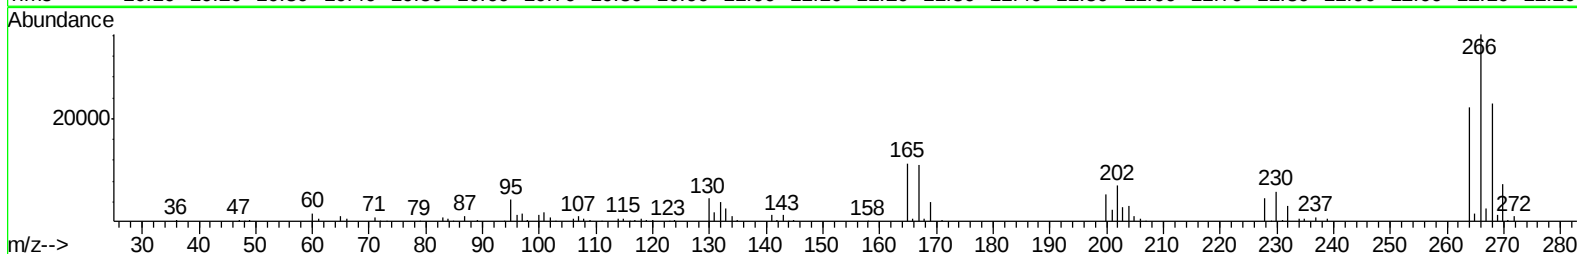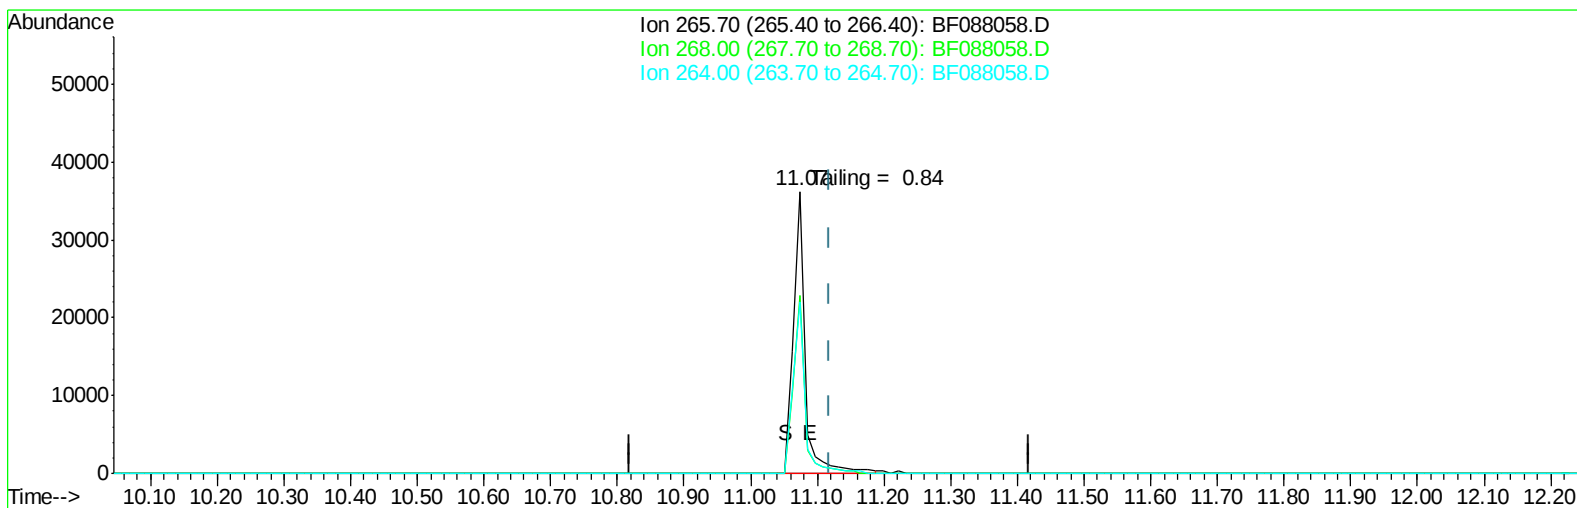

TIC: BF088058.D

(69) Pentachlorophenol (C)

11.073min (-0.046) 0.00ng

response 44742

Ion	Exp%	Act%
265.70	100	100
268.00	66.00	63.26
264.00	62.00	61.03
0.00	0.00	0.00