


Data Path : Z:\HPCHEM1\BNA F\DATA\BF061516\
 Data File : BF088058.D
 Acq On : 16 Jun 2016 2:58
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 13 14:10:49 2016

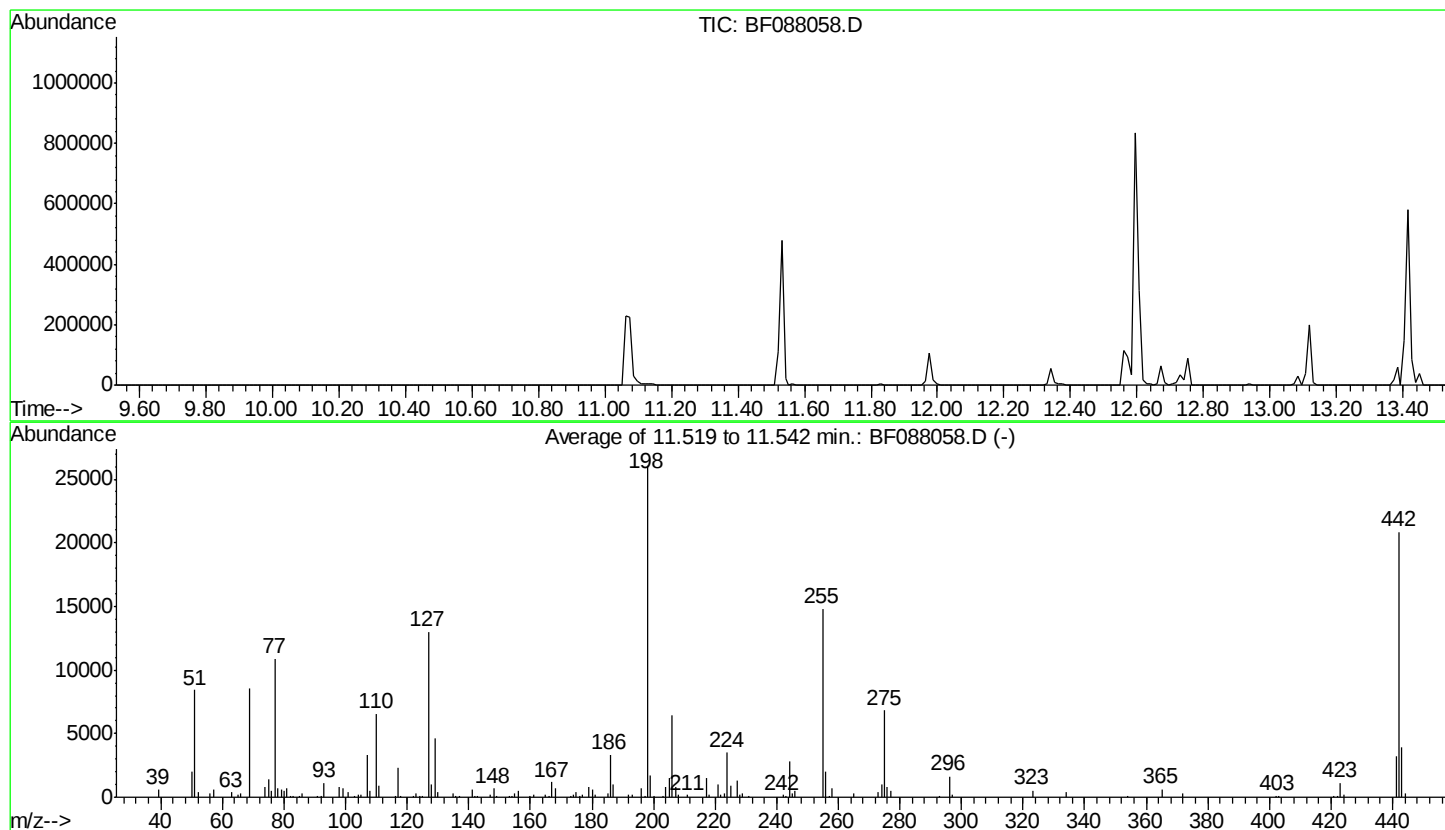

AutoFind: Scans 869, 870, 871; Background Corrected with Scan 866

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.4	8437	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.9	8581	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.0	13023	PASS
197	198	0.00	2	0.5	130	PASS
198	198	100	100	100.0	26058	PASS
199	198	5	9	6.7	1741	PASS
275	198	10	60	26.1	6807	PASS
365	198	1	100	2.4	627	PASS
441	442	0.01	24	15.6	3262	PASS
442	198	50	100	80.0	20845	PASS
443	442	15	24	19.0	3965	PASS