
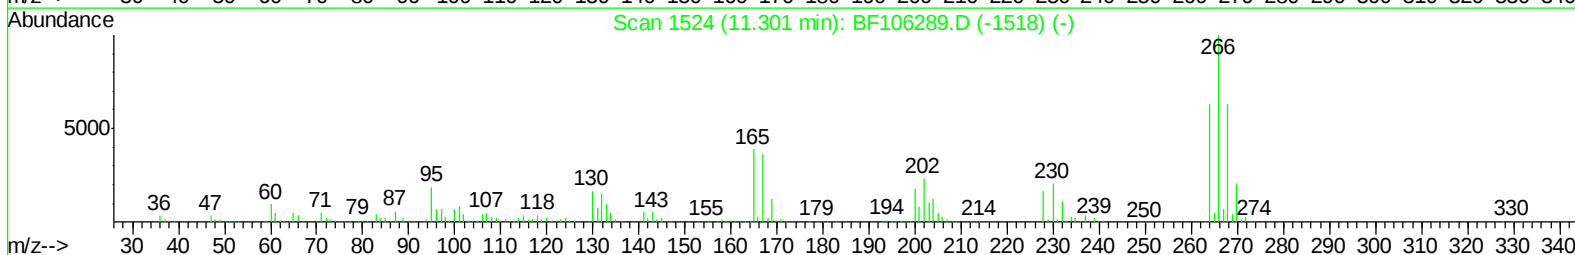
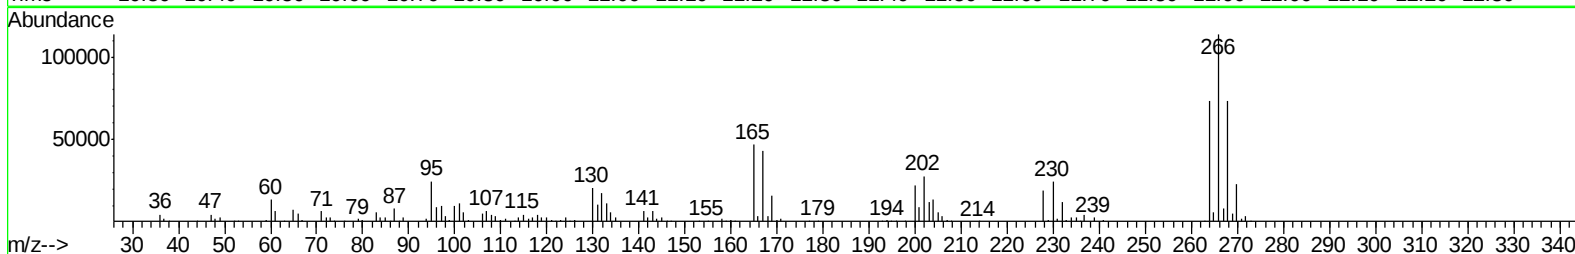


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061518\
Data File : BF106486.D
Acq On : 15 Jun 2018 12:43
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 18 00:47:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 15 11:11:47 2018
Response via : Initial Calibration

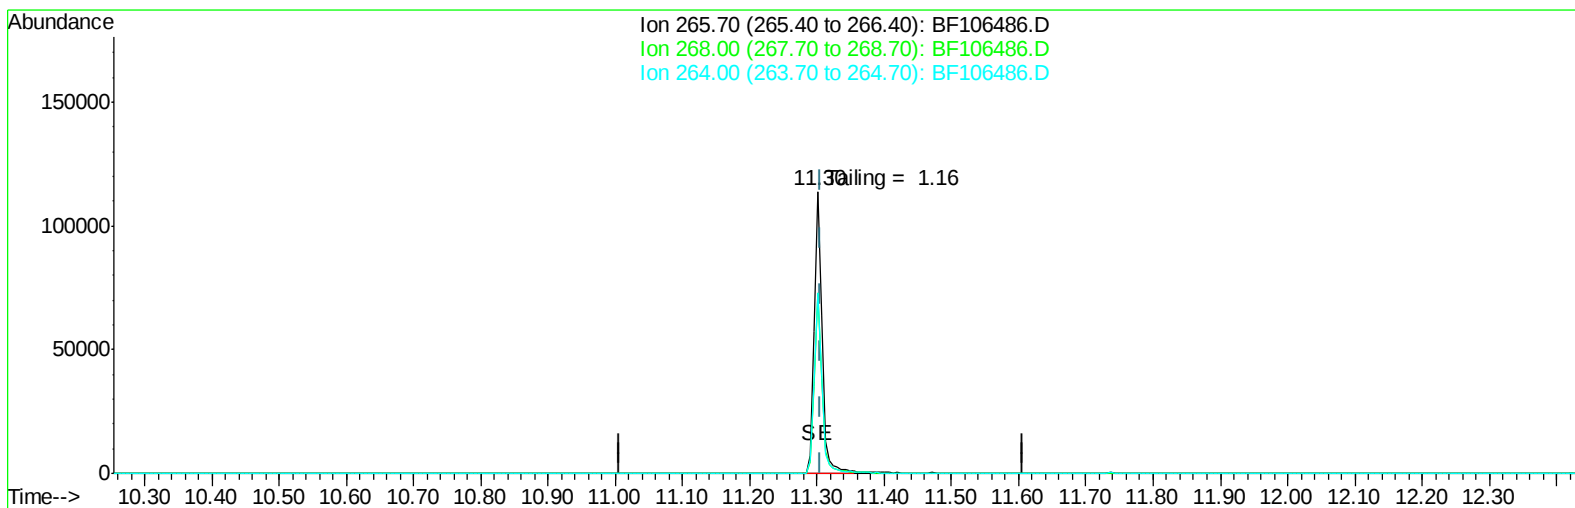

TIC: BF106486.D

(69) Pentachlorophenol (C)

11.301min (-0.006) 25048.03ng

response 97466

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.32
264.00	61.90	64.25
0.00	0.00	0.00

