

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061518\
 Data File : BF106496.D
 Acq On : 15 Jun 2018 17:14
 Operator : JU/SJ
 Sample : J3464-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-38-COMP

Quant Time: Jun 16 00:16:41 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 15 11:11:47 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.97	152	134062	20.00	ng	0.00
21) Naphthalene-d8	8.25	136	488806	20.00	ng	0.00
38) Acenaphthene-d10	10.01	164	215577	20.00	ng	0.00
63) Phenanthrene-d10	11.50	188	351137	20.00	ng	0.00
75) Chrysene-d12	14.16	240	352004	20.00	ng	0.00
86) Perylene-d12	15.71	264	313414	20.00	ng	0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.61	112	917253	115.80	ng	0.00
7) Phenol-d6	6.61	99	1112485	111.17	ng	0.00
23) Nitrobenzene-d5	7.53	82	771765	92.88	ng	0.00
41) 2,4,6-Tribromophenol	10.80	330	271301	130.80	ng	0.00
44) 2-Fluorobiphenyl	9.32	172	1071095	89.81	ng	0.00
78) Terphenyl-d14	13.08	244	966592	68.20	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.71	163	148572	9.646	ng	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061518\
Data File : BF106496.D
Acq On : 15 Jun 2018 17:14
Operator : JU/SJ
Sample : J3464-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-38-COMP

Quant Time: Jun 16 00:16:41 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 15 11:11:47 2018
Response via : Initial Calibration

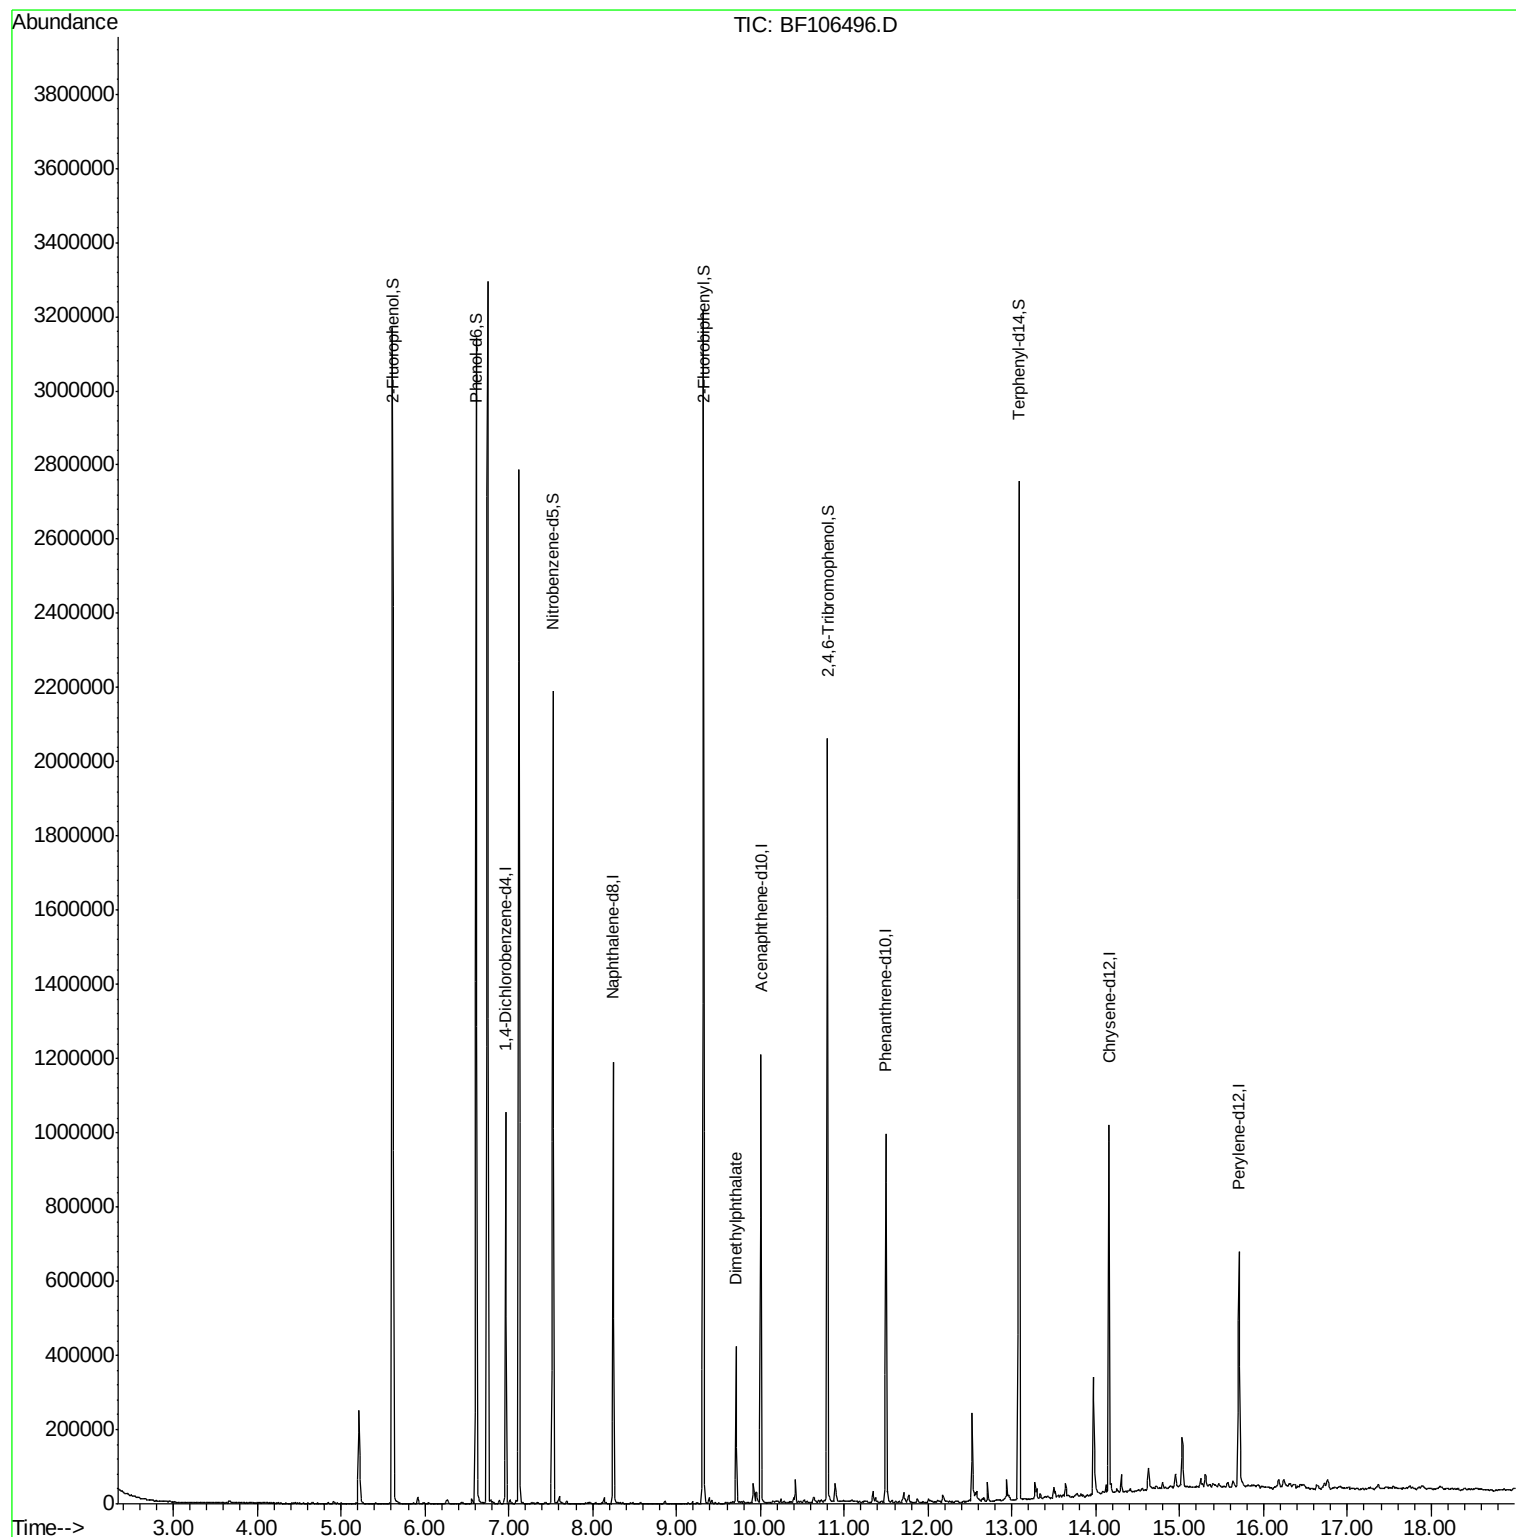

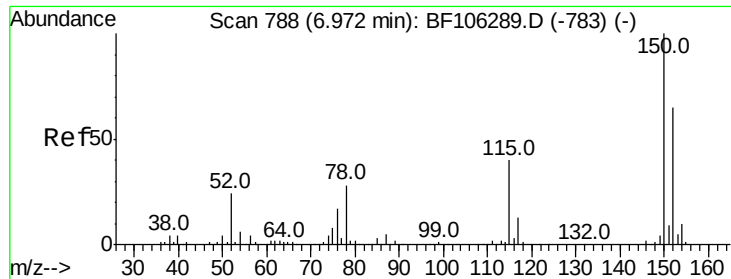


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.97 min Scan# 787
Delta R.T. 0.00 min
Lab File: BF106496.D
Acq: 15 Jun 2018 17:14

Instrument :
BNA_F
ClientSampleId :
SB-38-COMP

Tot Ion:152 Resp: 134062
Ion Ratio Lower Upper
152 100
150 157.4 124.6 186.8
115 62.6 50.1 75.1

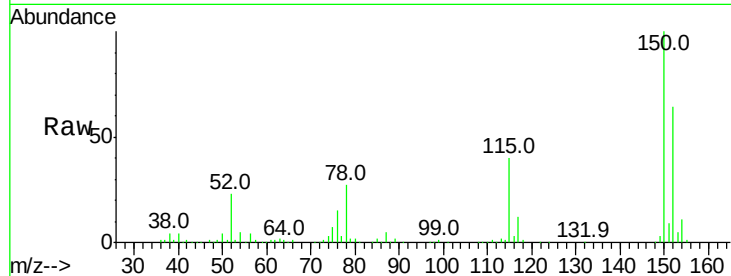


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

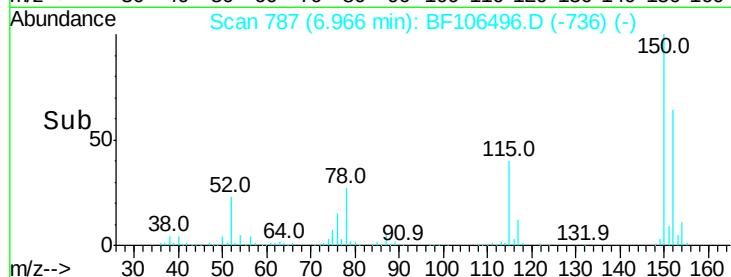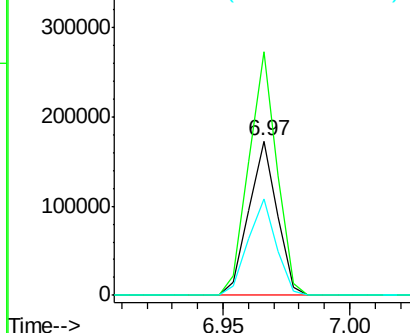



#5


2-Fluorophenol
Concen: 115.801 ng
RT: 5.61 min Scan# 557
Delta R.T. 0.00 min
Lab File: BF106496.D
Acq: 15 Jun 2018 17:14

Tgt Ion:112 Resp: 917253
Ion Ratio Lower Upper
112 100
64 60.7 47.9 71.9
63 31.3 23.7 35.5



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

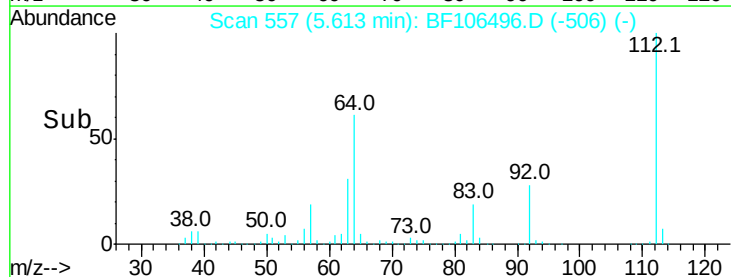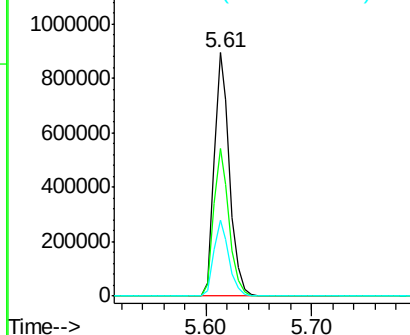

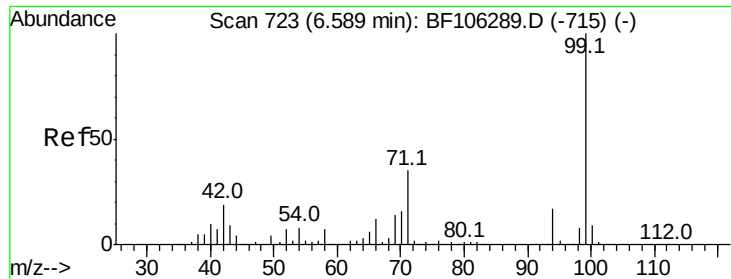

#7

Phenol-d6

Concen: 111.166 ng

RT: 6.61 min Scan# 727

Delta R.T. 0.00 min

Lab File: BF106496.D

Acq: 15 Jun 2018 17:14

Instrument :

BNA_F

ClientSampleId :

SB-38-COMP


Tot Ion: 99 Resp: 1112485

Ion Ratio Lower Upper




99 100

42 17.4 14.5 21.7

71 35.7 25.4 38.0

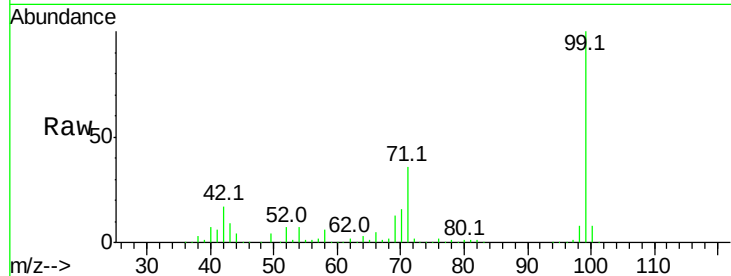

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

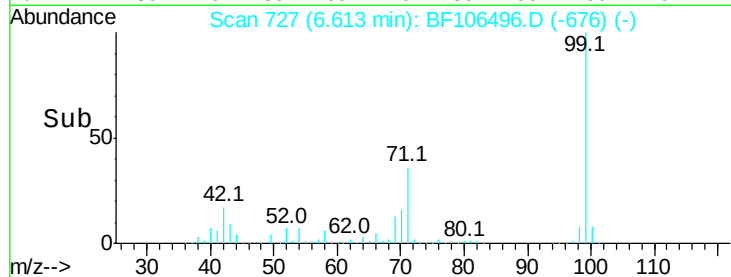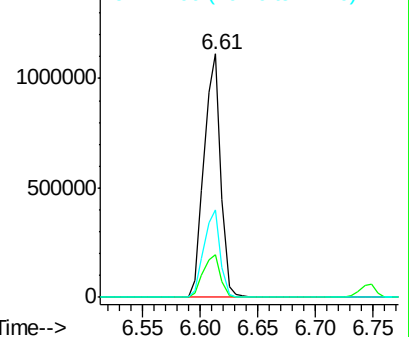

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.25 min Scan# 1005

Delta R.T. 0.00 min

Lab File: BF106496.D

Acq: 15 Jun 2018 17:14

Tgt Ion: 136 Resp: 488806


Ion Ratio Lower Upper

136 100



137 11.3 8.9 13.3


54 8.7 6.6 9.8

68 6.4 5.0 7.4



Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

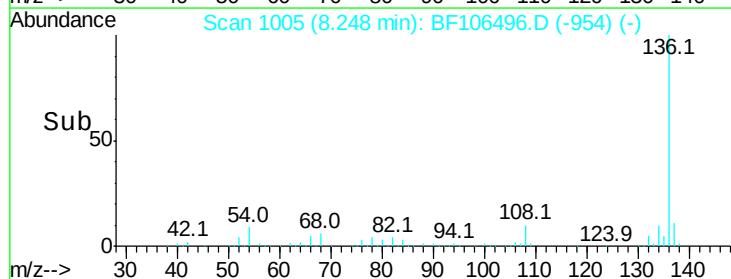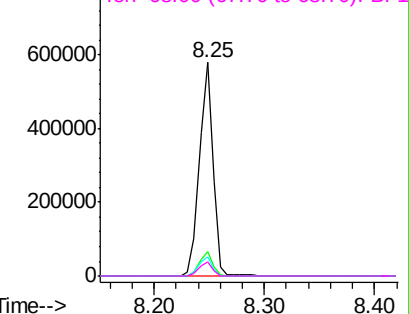

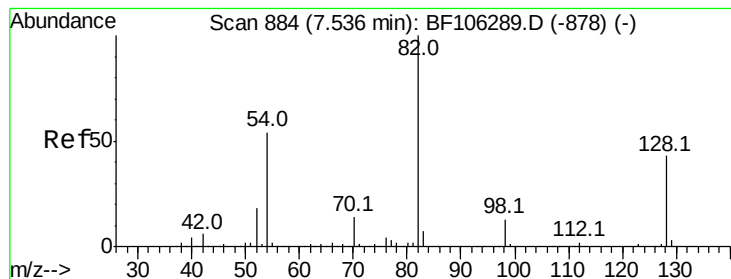

#23

Nitrobenzene-d5

Concen: 92.883 ng

RT: 7.53 min Scan# 883

Delta R.T. 0.00 min

Lab File: BF106496.D

Acq: 15 Jun 2018 17:14

Instrument :

BNA_F

ClientSampleId :

SB-38-COMP


Tot Ion: 82 Resp: 771765

Ion Ratio Lower Upper

82 100

128 43.8 36.1 54.1




54 51.2 41.4 62.2



Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): BF1

Ion 54.00 (53.70 to 54.70): BF1

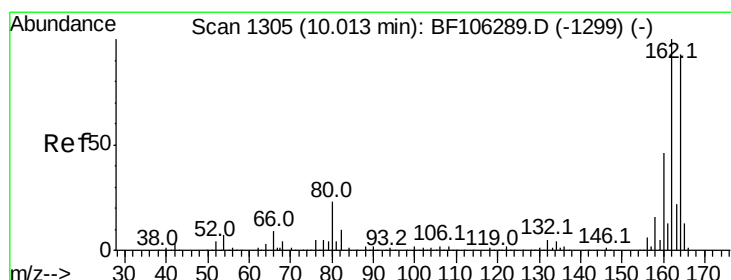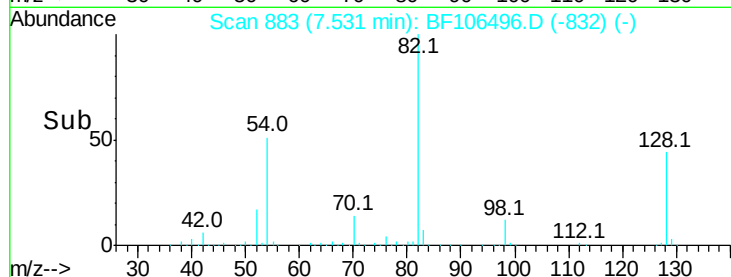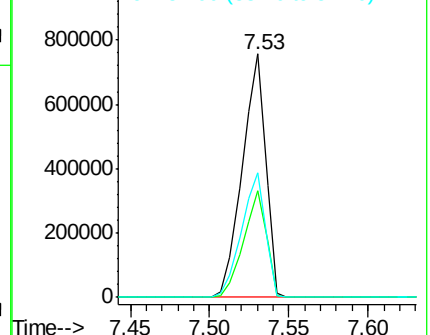

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 10.01 min Scan# 1304

Delta R.T. 0.00 min

Lab File: BF106496.D

Acq: 15 Jun 2018 17:14


Tgt Ion:164 Resp: 215577

Ion Ratio Lower Upper

164 100

162 105.6 86.1 129.1



160 48.7 38.3 57.5




Abundance Ion 164.00 (163.70 to 164.70): BF1

Ion 162.00 (161.70 to 162.70): BF1

Ion 160.00 (159.70 to 160.70): BF1

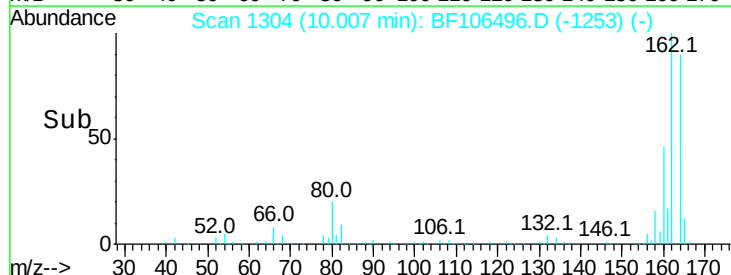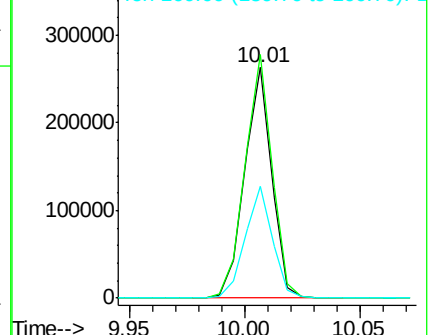


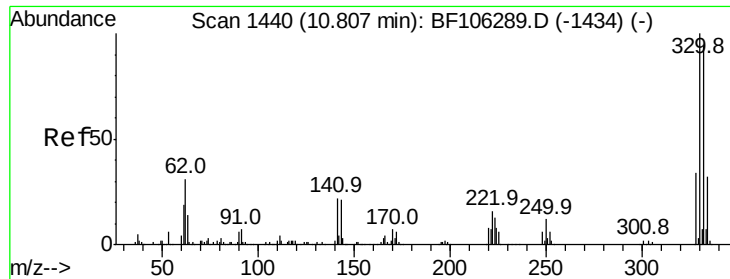




#41
 2,4,6-Tribromophenol
 Concen: 130.796 ng
 RT: 10.80 min Scan# 1439
 Delta R.T. 0.00 min
 Lab File: BF106496.D
 Acq: 15 Jun 2018 17:14

Instrument :
 BNA_F
 ClientSampleId :
 SB-38-COMP

Tot Ion:330 Resp: 271301
 Ion Ratio Lower Upper
 330 100
 332 95.9 77.0 115.6
 141 27.4 29.9 44.9#

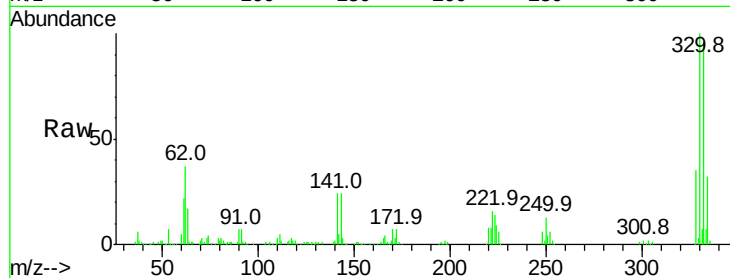


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

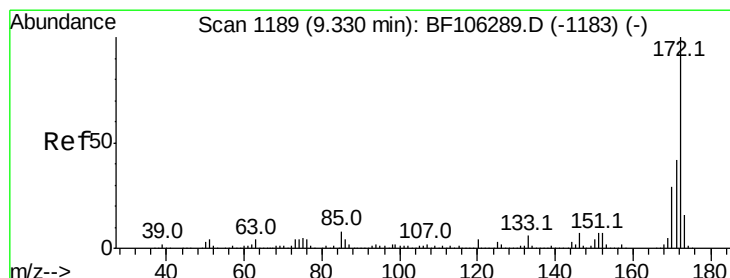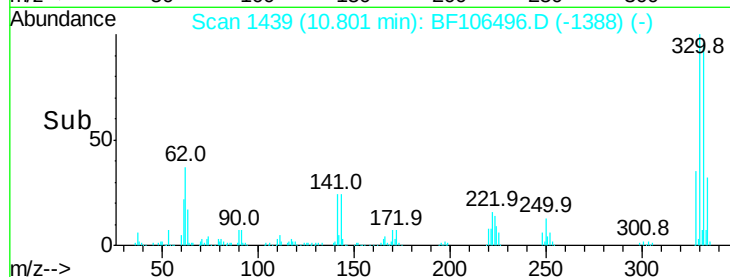
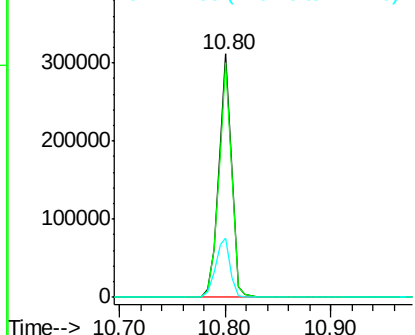



#44
 2-Fluorobiphenyl
 Concen: 89.814 ng
 RT: 9.32 min Scan# 1188
 Delta R.T. 0.00 min
 Lab File: BF106496.D
 Acq: 15 Jun 2018 17:14

Tgt Ion:172 Resp: 1071095
 Ion Ratio Lower Upper
 172 100
 171 37.7 29.7 44.5
 170 25.8 19.6 29.4

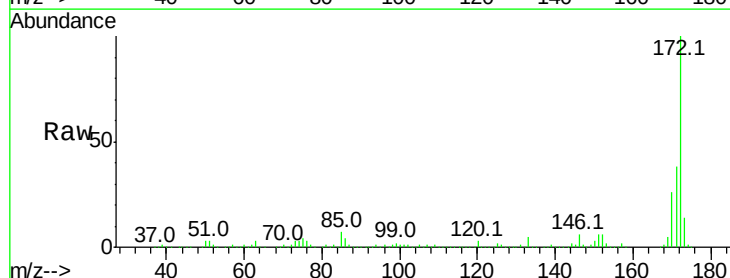

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

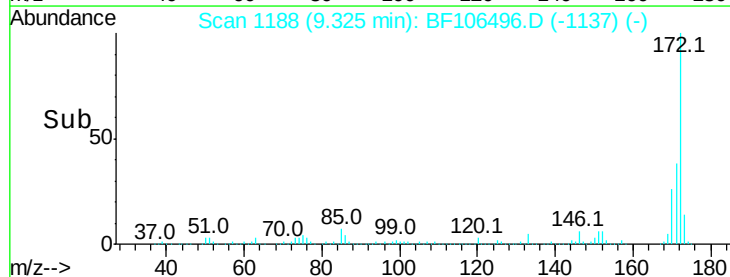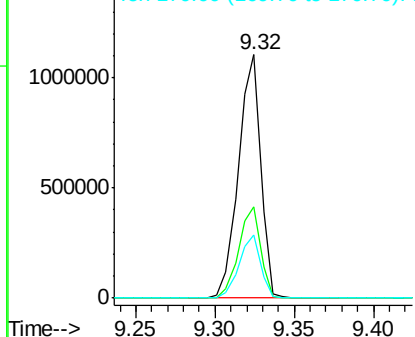

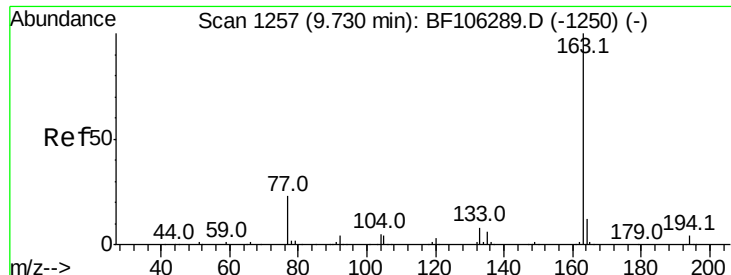

#49

Dimethylphthalate

Concen: 9.646 ng

RT: 9.71 min Scan# 1254

Delta R.T. -0.01 min

Lab File: BF106496.D

Acq: 15 Jun 2018 17:14

Instrument :

BNA_F

ClientSampleId :

SB-38-COMP


Tot Ion:163 Resp: 148572

Ion Ratio Lower Upper

163 100

194 3.6 2.7 4.1




164 10.3 8.2 12.2



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

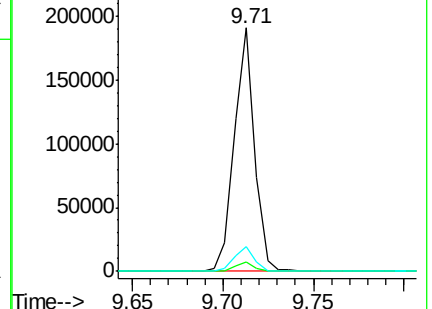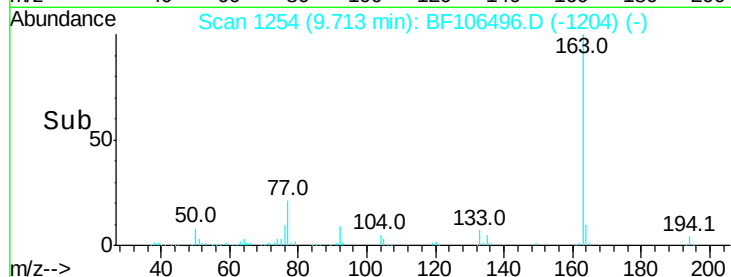

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.50 min Scan# 1557

Delta R.T. -0.01 min

Lab File: BF106496.D

Acq: 15 Jun 2018 17:14


Tgt Ion:188 Resp: 351137

Ion Ratio Lower Upper

188 100

94 10.5 8.5 12.7



80 11.5 9.2 13.8




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

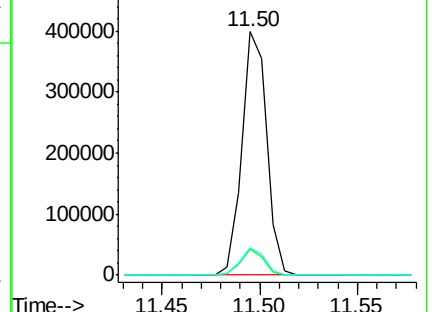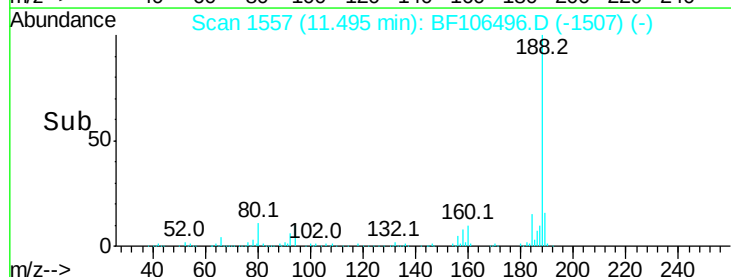

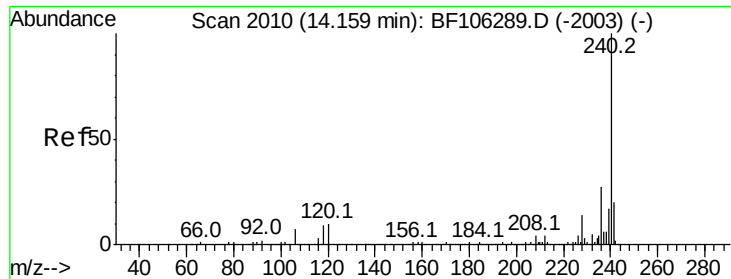

#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.16 min Scan# 2010

Delta R.T. 0.01 min

Lab File: BF106496.D

Acq: 15 Jun 2018 17:14

Instrument :

BNA_F

ClientSampleId :

SB-38-COMP


Tot Ion:240 Resp: 352004

Ion Ratio Lower Upper

240 100

120 10.1 9.5 14.3

236 26.4 20.7 31.1



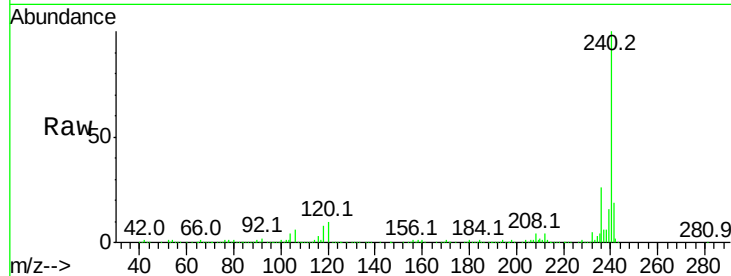


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

Time-->

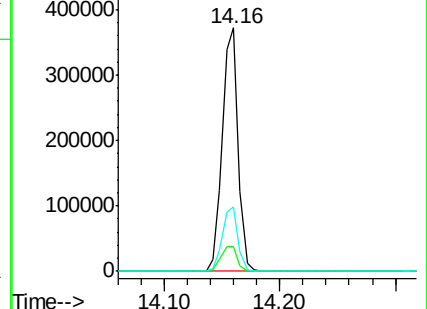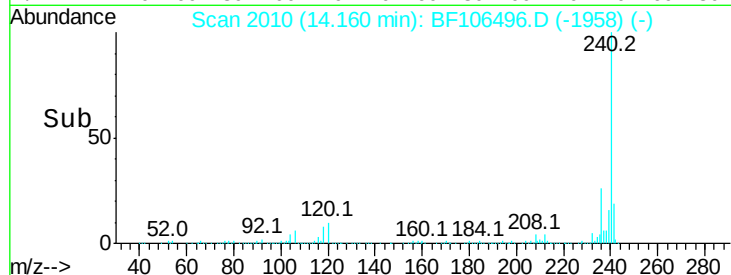

#78

Terphenyl-d14

Concen: 68.204 ng

RT: 13.08 min Scan# 1827

Delta R.T. 0.00 min

Lab File: BF106496.D

Acq: 15 Jun 2018 17:14


Tgt Ion:244 Resp: 966592

Ion Ratio Lower Upper

244 100

212 7.0 5.4 8.0

122 10.2 11.0 16.4#






Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

Time-->

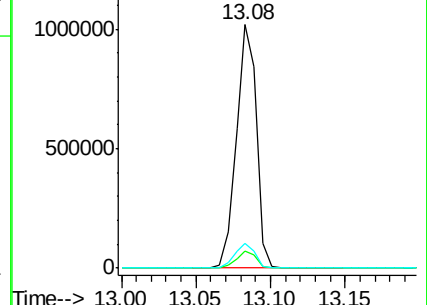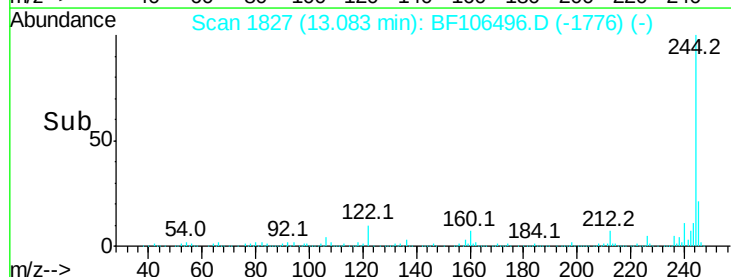

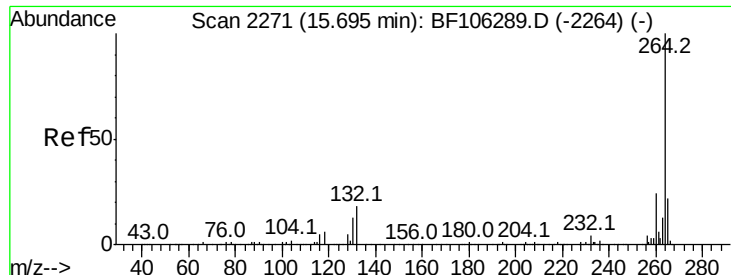

#86
 Pervlene-d12
 Concen: 20.000 ng
 RT: 15.71 min Scan# 2273
 Delta R.T. 0.02 min
 Lab File: BF106496.D
 Acq: 15 Jun 2018 17:14

Instrument :
 BNA_F
 ClientSampleId :
 SB-38-COMP

Tot Ion:264 Resp: 313414
 Ion Ratio Lower Upper
 264 100
 260 24.2 19.2 28.8
 265 22.1 17.5 26.3

