

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061518\
 Data File : BF106497.D
 Acq On : 15 Jun 2018 17:40
 Operator : JU/SJ
 Sample : J3464-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-41-COMP

Quant Time: Jun 16 00:21:00 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 15 11:11:47 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.97	152	134217	20.00	ng	0.00
21) Naphthalene-d8	8.25	136	503730	20.00	ng	0.00
38) Acenaphthene-d10	10.01	164	218628	20.00	ng	0.00
63) Phenanthrene-d10	11.50	188	356568	20.00	ng	0.00
75) Chrysene-d12	14.15	240	347646	20.00	ng	0.00
86) Perylene-d12	15.71	264	312702	20.00	ng	0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.61	112	761787	96.06	ng	0.00
7) Phenol-d6	6.61	99	918322	91.66	ng	0.00
23) Nitrobenzene-d5	7.53	82	622238	72.67	ng	0.00
41) 2,4,6-Tribromophenol	10.80	330	206696	98.26	ng	0.00
44) 2-Fluorobiphenyl	9.32	172	899279	68.51	ng	0.00
78) Terphenyl-d14	13.08	244	791938	56.58	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.71	163	133521	8.548	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061518\
Data File : BF106497.D
Acq On : 15 Jun 2018 17:40
Operator : JU/SJ
Sample : J3464-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-41-COMP

Quant Time: Jun 16 00:21:00 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 15 11:11:47 2018
Response via : Initial Calibration

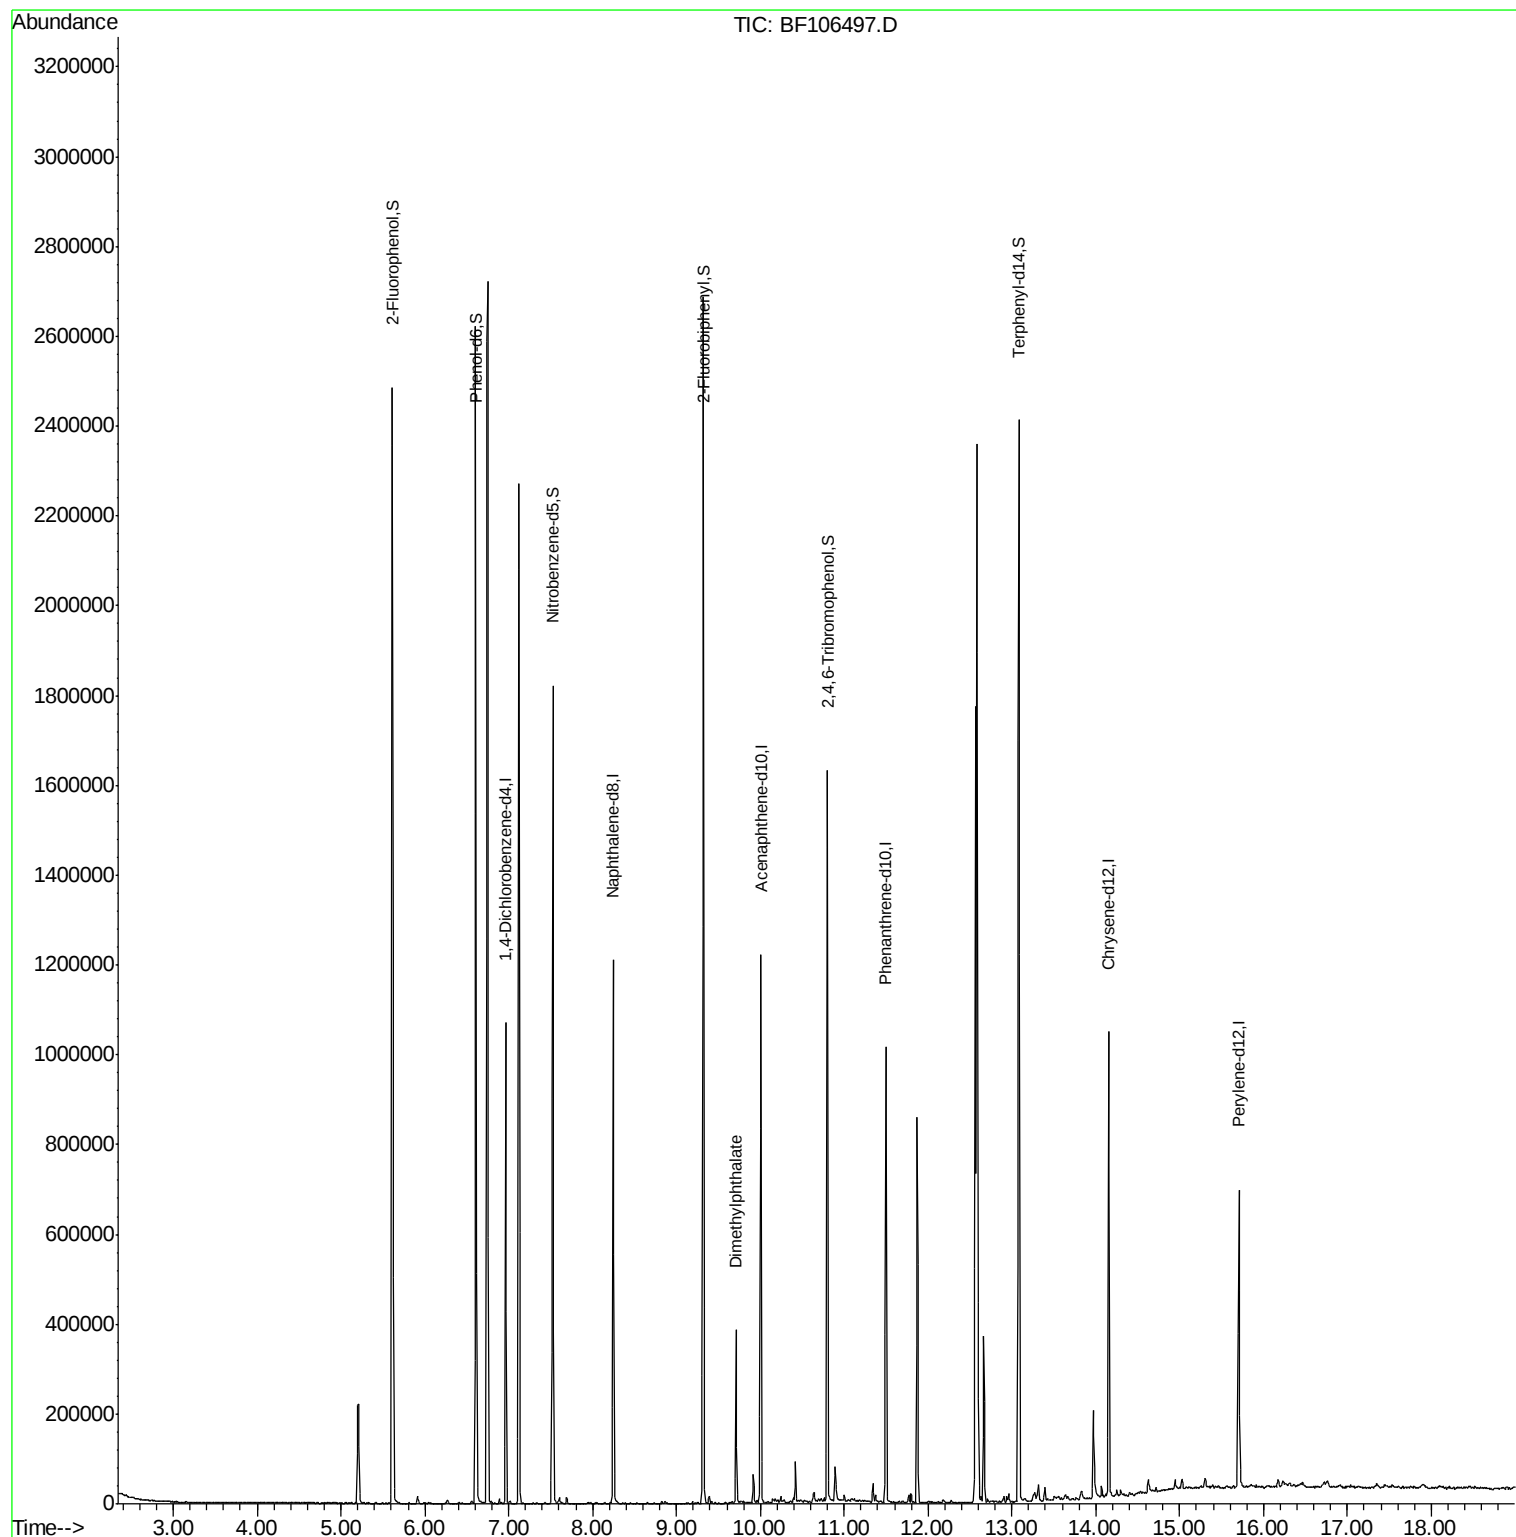

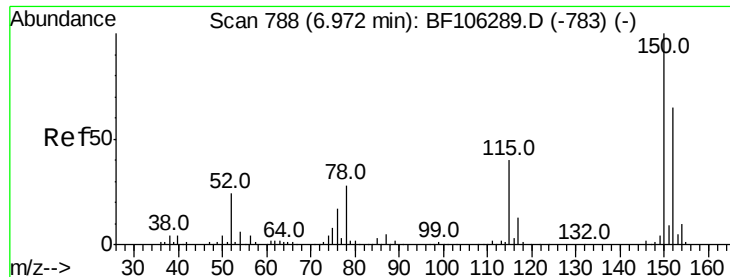


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.97 min Scan# 787
Delta R.T. 0.00 min
Lab File: BF106497.D
Acq: 15 Jun 2018 17:40

Instrument :
BNA_F
ClientSampleId :
SB-41-COMP

Tot Ion	Ratio	Lower	Upper
152	100		
150	163.8	124.6	186.8
115	63.2	50.1	75.1

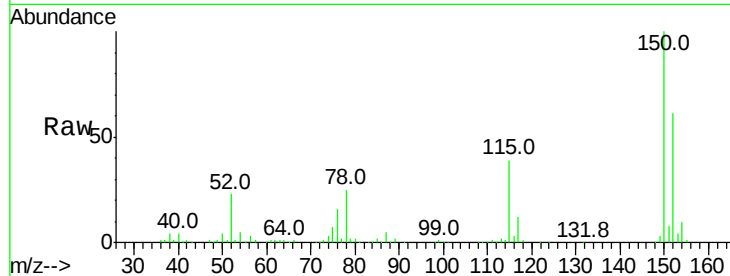


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

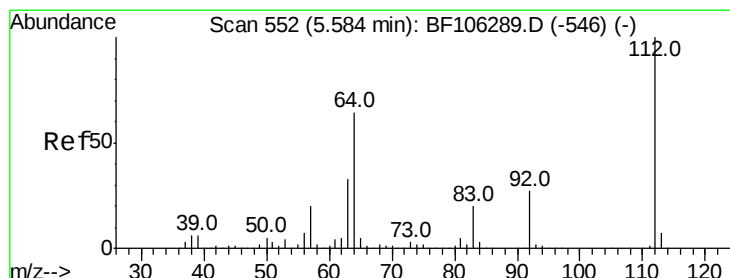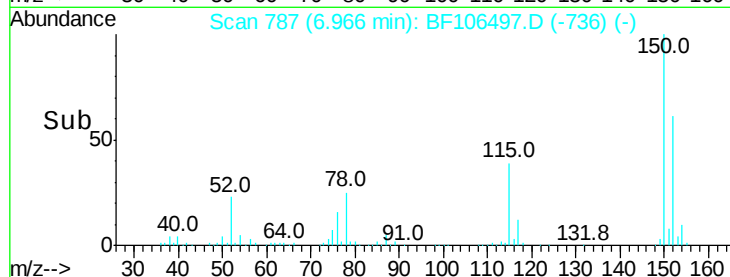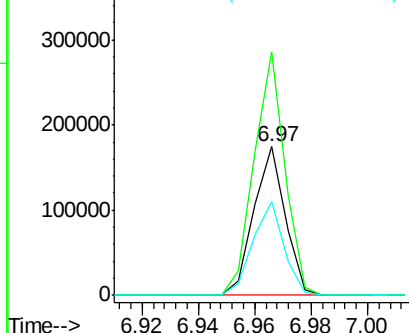



#5


2-Fluorophenol
Concen: 96.063 ng
RT: 5.61 min Scan# 557
Delta R.T. 0.00 min
Lab File: BF106497.D
Acq: 15 Jun 2018 17:40

Tgt Ion	Ratio	Lower	Upper
112	100		
64	59.0	47.9	71.9
63	29.8	23.7	35.5

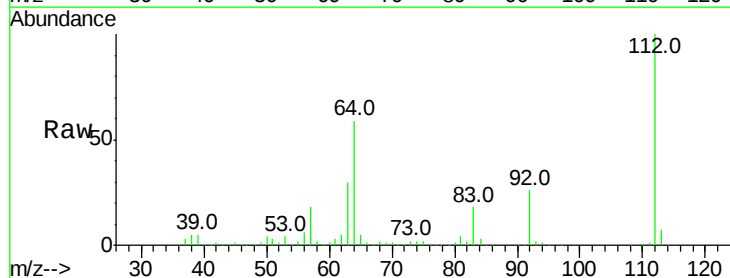

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

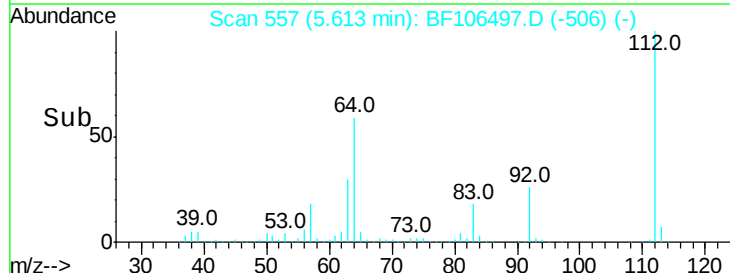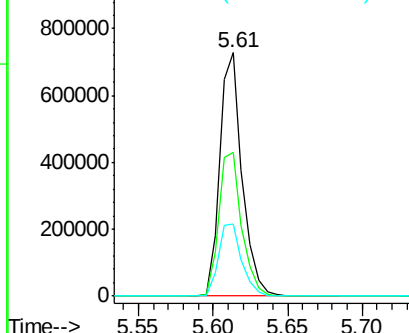

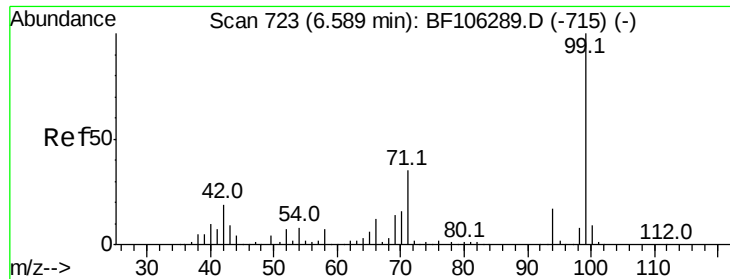

#7

Phenol-d6

Concen: 91.658 ng

RT: 6.61 min Scan# 726

Delta R.T. -0.01 min

Lab File: BF106497.D

Acq: 15 Jun 2018 17:40

Instrument :

BNA_F

ClientSampleId :

SB-41-COMP


Tot Ion: 99 Resp: 918322

Ion Ratio Lower Upper




99 100

42 18.2 14.5 21.7

71 35.9 25.4 38.0

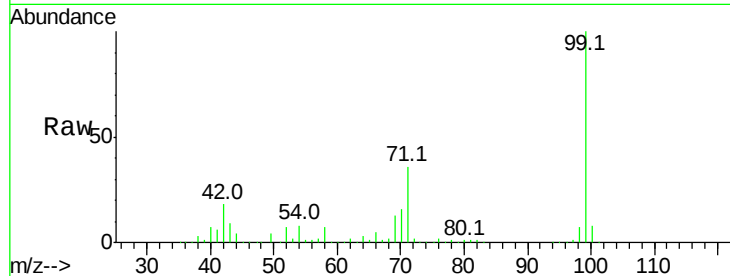

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

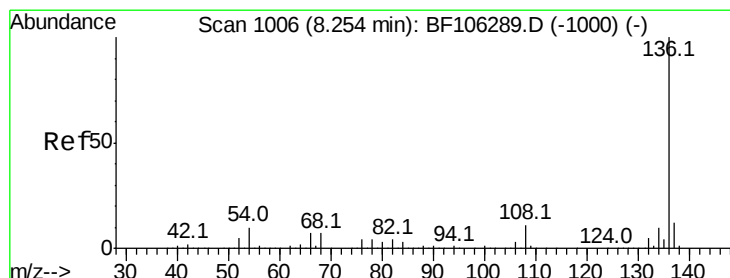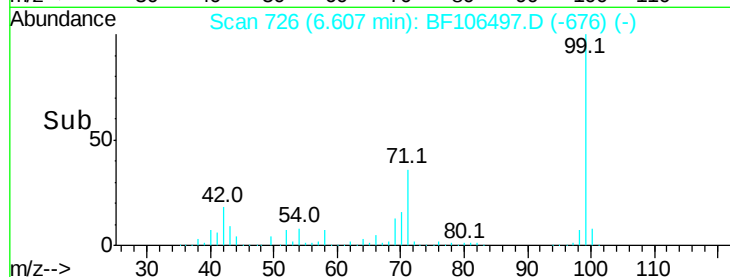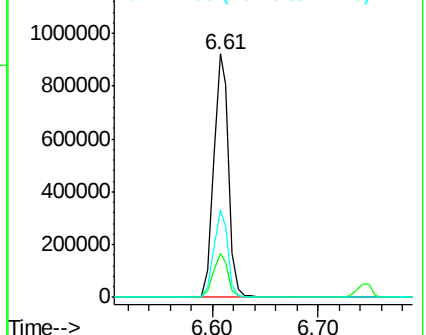

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.25 min Scan# 1005

Delta R.T. 0.00 min

Lab File: BF106497.D

Acq: 15 Jun 2018 17:40

Tgt Ion: 136 Resp: 503730


Ion Ratio Lower Upper

136 100



137 11.0 8.9 13.3


54 8.5 6.6 9.8

68 6.4 5.0 7.4

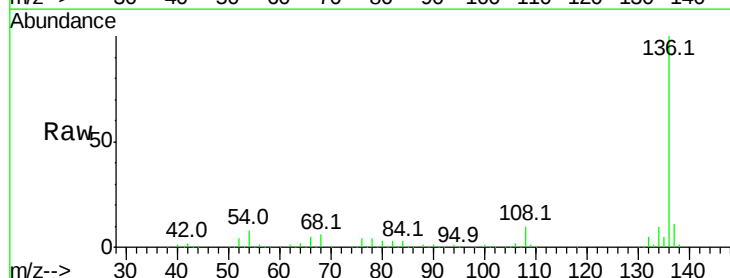

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

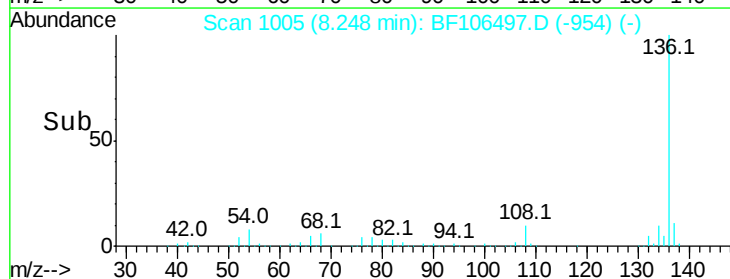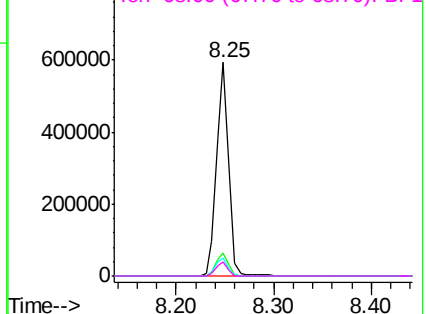


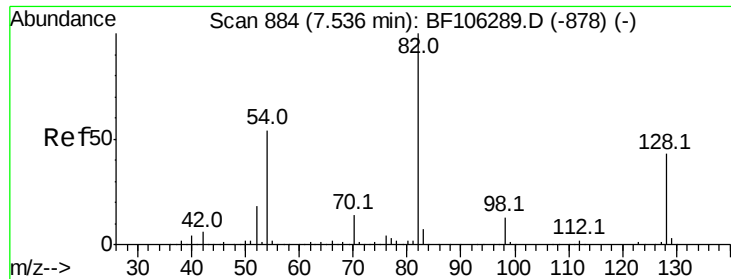




#23
Nitrobenzene-d5
Concen: 72.669 ng
RT: 7.53 min Scan# 883
Delta R.T. 0.00 min
Lab File: BF106497.D
Acq: 15 Jun 2018 17:40

Instrument :
BNA_F
ClientSampleId :
SB-41-COMP

Tot Ion: 82 Resp: 622238
Ion Ratio Lower Upper
82 100
128 44.4 36.1 54.1
54 51.5 41.4 62.2

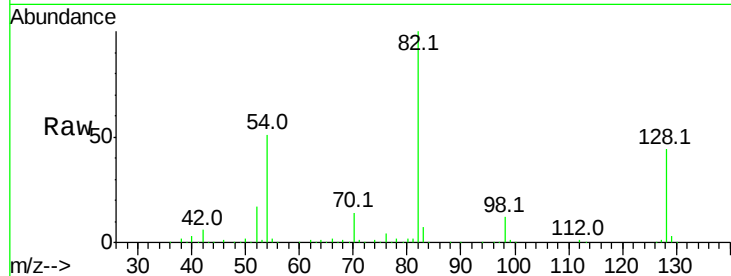


Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): BF1
Ion 54.00 (53.70 to 54.70): BF1

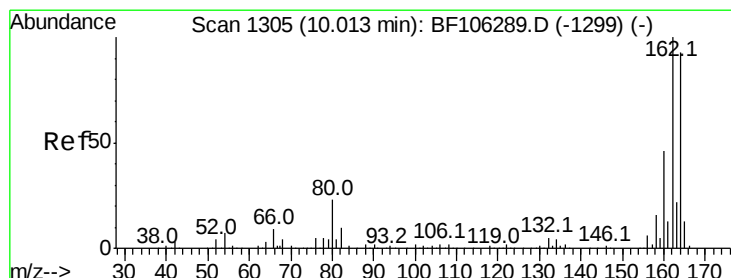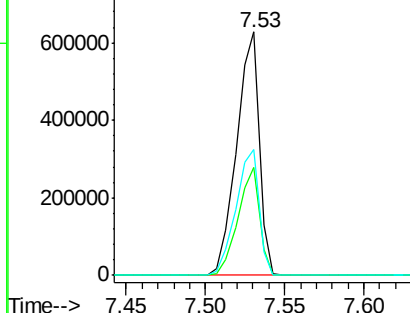
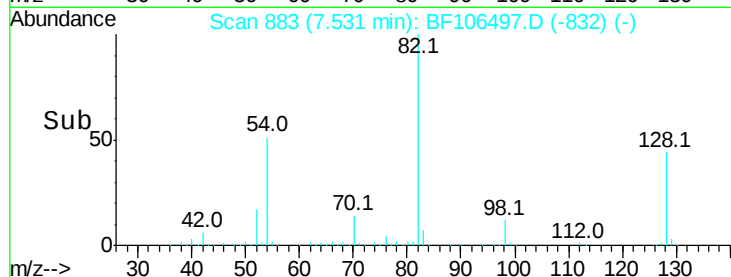



#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 10.01 min Scan# 1304
Delta R.T. 0.00 min
Lab File: BF106497.D
Acq: 15 Jun 2018 17:40

Tgt Ion:164 Resp: 218628
Ion Ratio Lower Upper
164 100
162 103.3 86.1 129.1
160 47.8 38.3 57.5

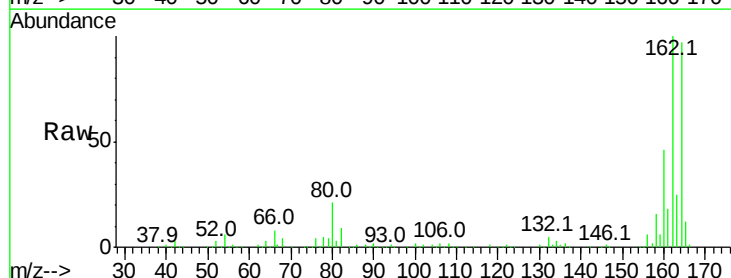

Abundance Ion 164.00 (163.70 to 164.70): BF1
Ion 162.00 (161.70 to 162.70): BF1
Ion 160.00 (159.70 to 160.70): BF1



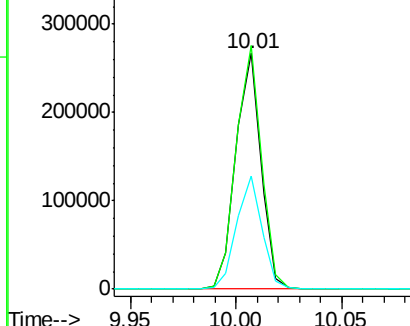
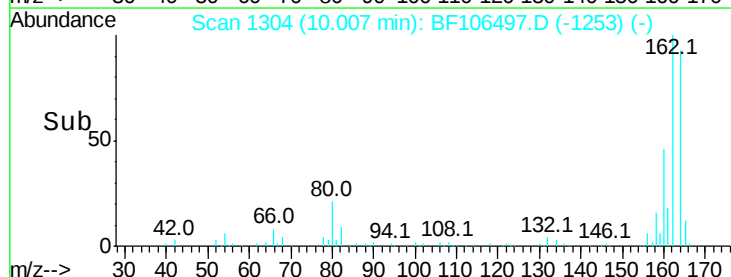


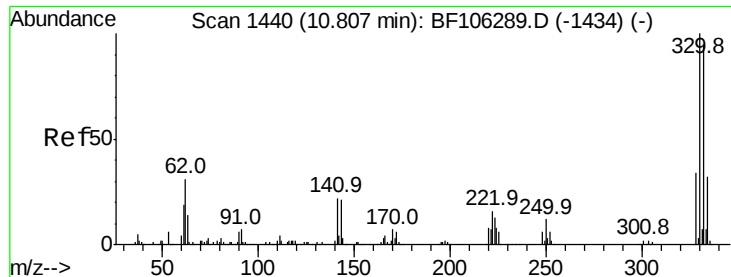

#41
 2,4,6-Tribromophenol
 Concen: 98.259 ng
 RT: 10.80 min Scan# 1439
 Delta R.T. 0.00 min
 Lab File: BF106497.D
 Acq: 15 Jun 2018 17:40




Instrument :
 BNA_F
 ClientSampleId :
 SB-41-COMP


Tot Ion	Ratio	Lower	Upper
330	100		
332	96.5	77.0	115.6
141	29.9	29.9	44.9#

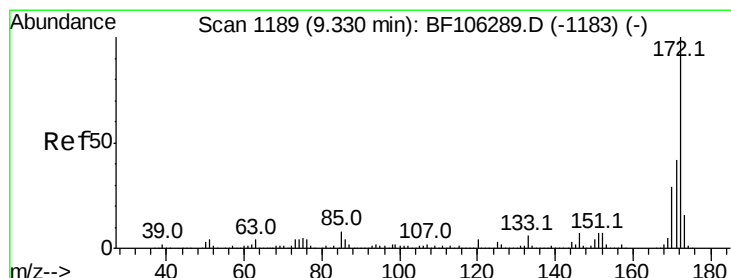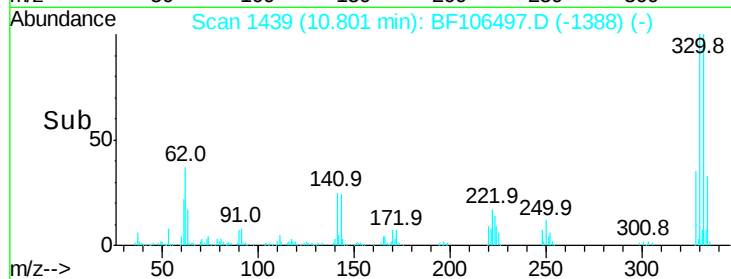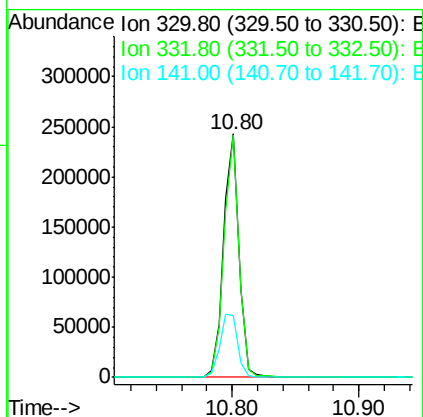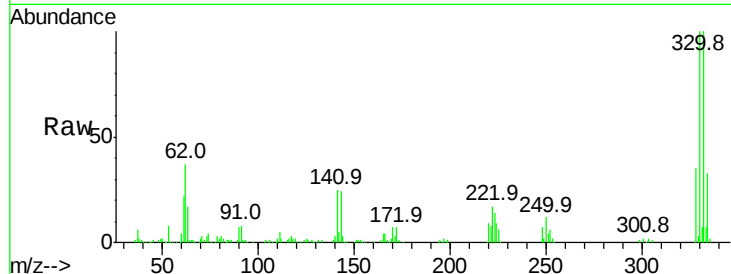

#44
 2-Fluorobiphenyl
 Concen: 68.508 ng
 RT: 9.32 min Scan# 1188
 Delta R.T. 0.00 min
 Lab File: BF106497.D
 Acq: 15 Jun 2018 17:40

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.8	29.7	44.5
170	25.1	19.6	29.4

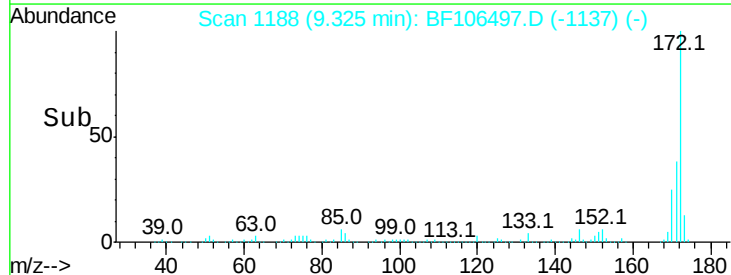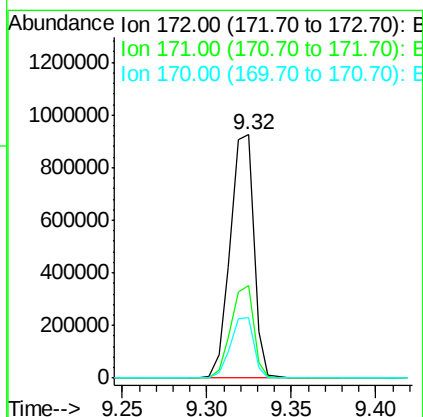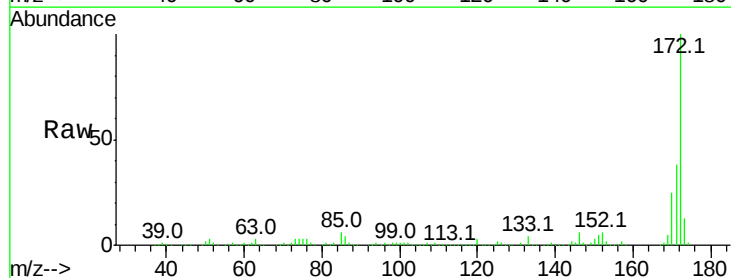

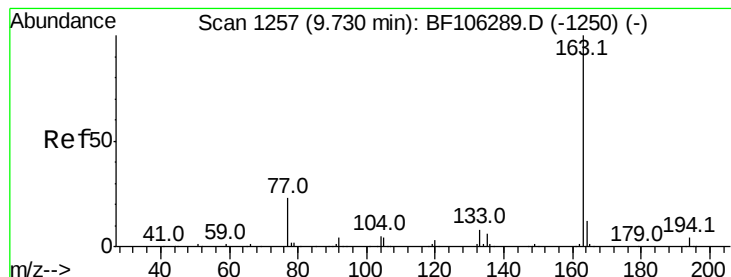

#49

Dimethylphthalate

Concen: 8.548 ng

RT: 9.71 min Scan# 1254

Delta R.T. -0.01 min

Lab File: BF106497.D

Acq: 15 Jun 2018 17:40

Instrument :

BNA_F

ClientSampleId :

SB-41-COMP


Tot Ion:163 Resp: 133521

Ion Ratio Lower Upper

163 100

194 3.9 2.7 4.1




164 9.8 8.2 12.2

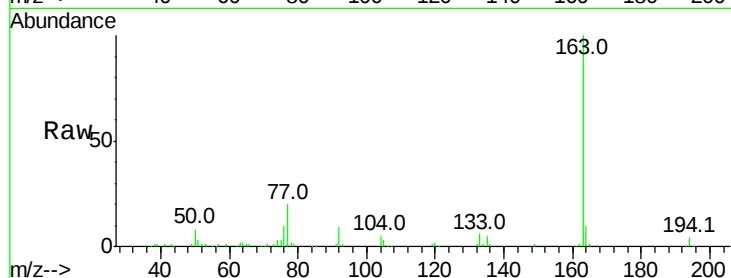

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

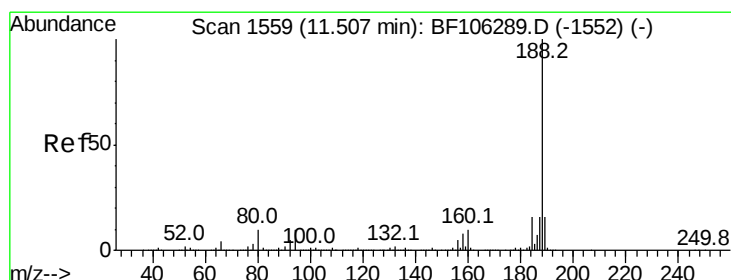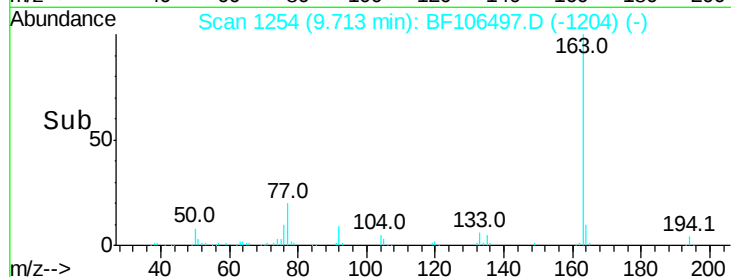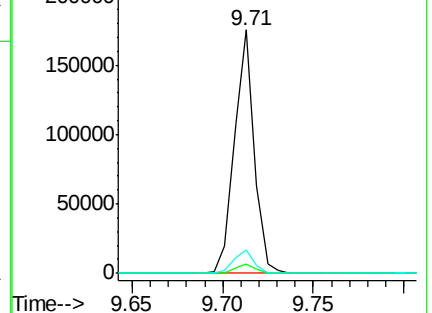

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.50 min Scan# 1557

Delta R.T. -0.01 min

Lab File: BF106497.D

Acq: 15 Jun 2018 17:40


Tgt Ion:188 Resp: 356568

Ion Ratio Lower Upper

188 100

94 11.0 8.5 12.7



80 11.4 9.2 13.8

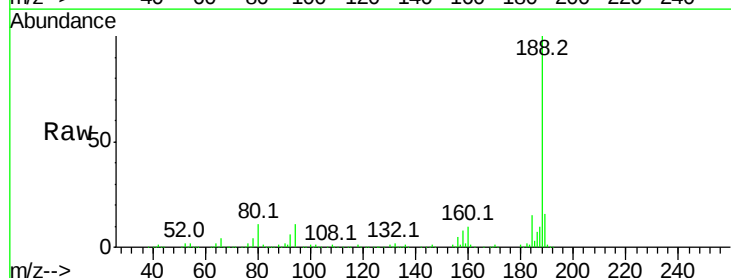


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

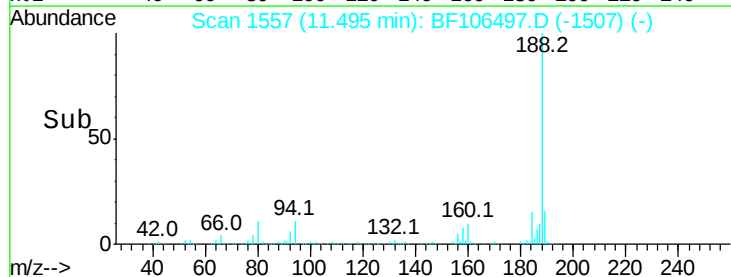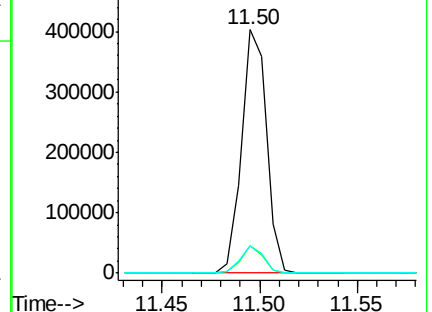

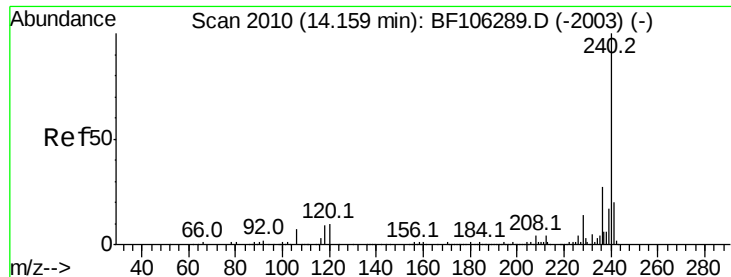

#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.15 min Scan# 2009

Delta R.T. 0.00 min

Lab File: BF106497.D

Acq: 15 Jun 2018 17:40

Instrument :

BNA_F

ClientSampleId :

SB-41-COMP


Tot Ion:240 Resp: 347646

Ion Ratio Lower Upper

240 100

120 10.8 9.5 14.3




236 26.9 20.7 31.1

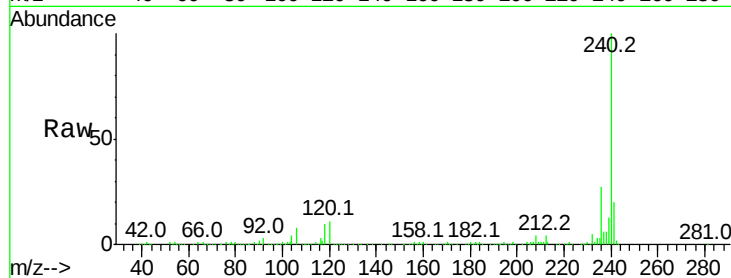

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

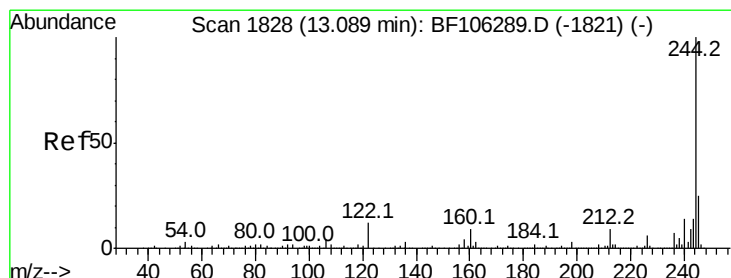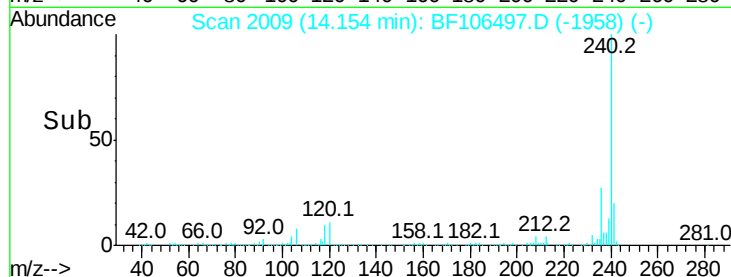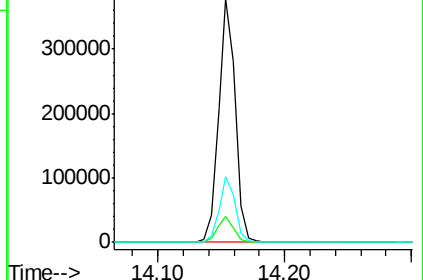

#78

Terphenyl-d14

Concen: 56.581 ng

RT: 13.08 min Scan# 1827

Delta R.T. 0.00 min

Lab File: BF106497.D

Acq: 15 Jun 2018 17:40


Tgt Ion:244 Resp: 791938

Ion Ratio Lower Upper

244 100

212 7.0 5.4 8.0



122 10.3 11.0 16.4#

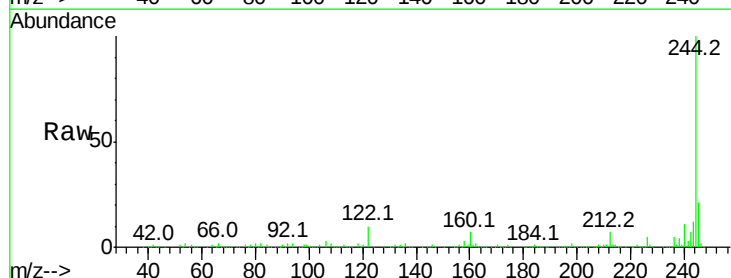


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

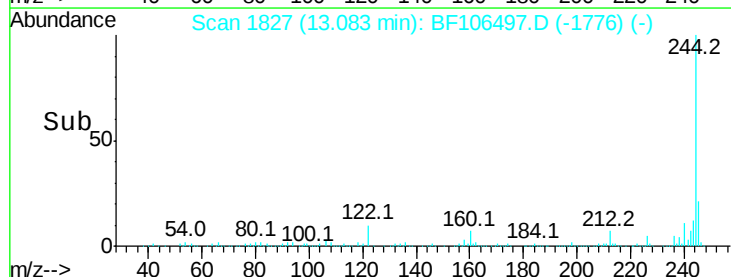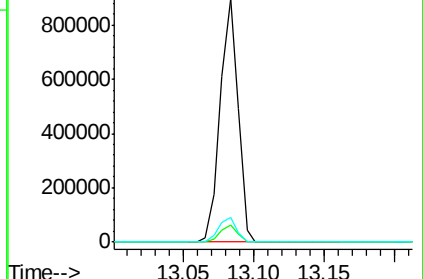

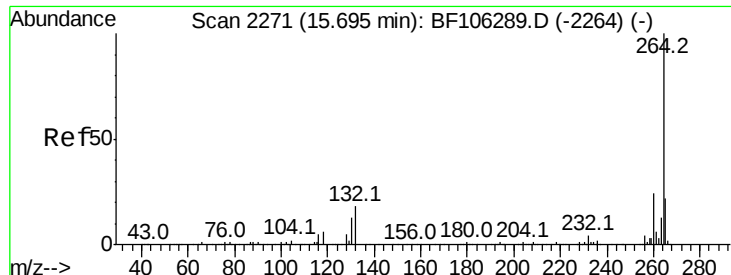

#86
 Pervlene-d12
 Concen: 20.000 ng
 RT: 15.71 min Scan# 2273
 Delta R.T. 0.02 min
 Lab File: BF106497.D
 Acq: 15 Jun 2018 17:40

Instrument :
 BNA_F
 ClientSampleId :
 SB-41-COMP

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.5	19.2	28.8
265	20.7	17.5	26.3

