


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061518\
 Data File : BF106513.D
 Acq On : 16 Jun 2018 1:36
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 15 11:11:47 2018

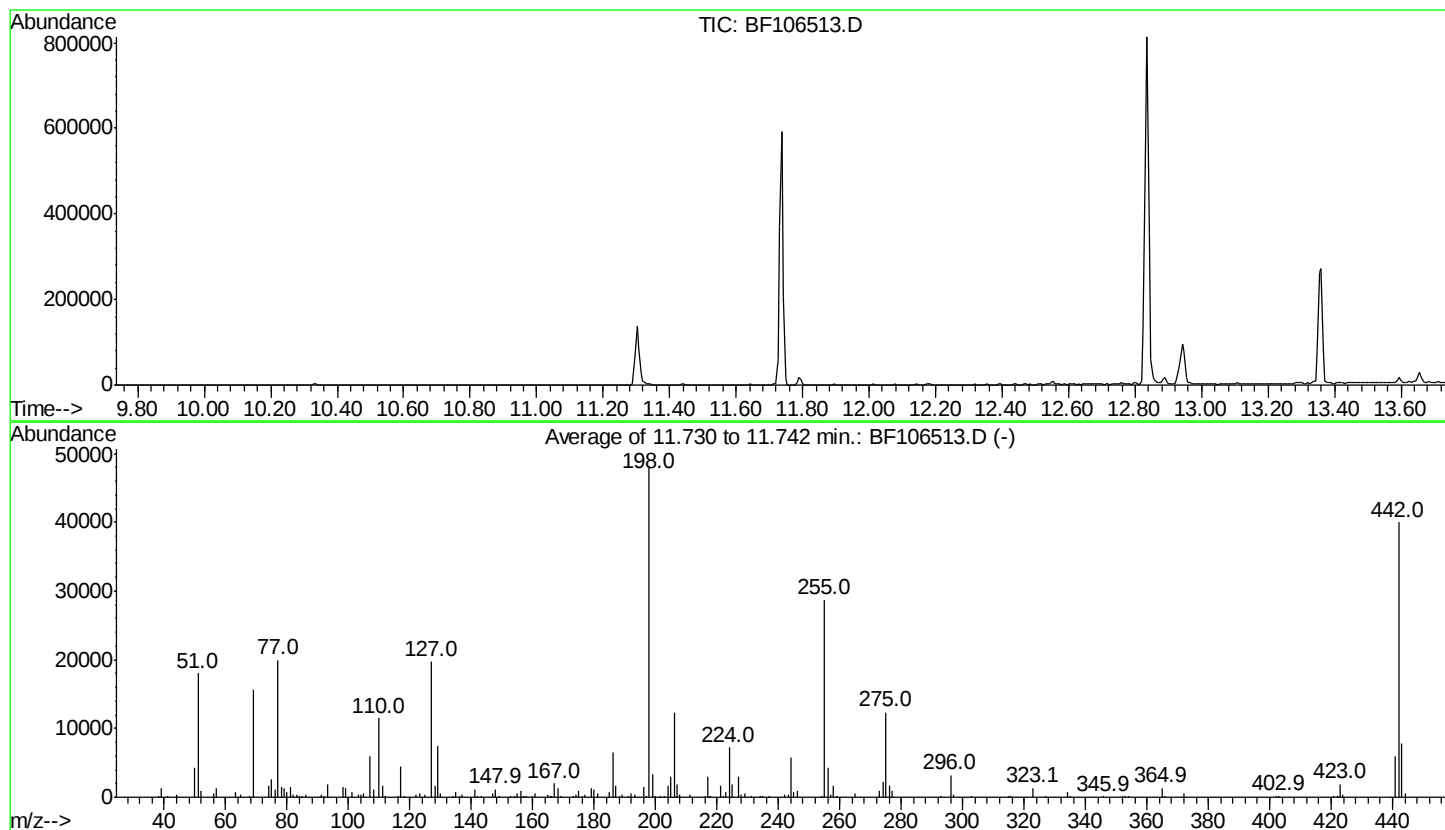

AutoFind: Scans 1597, 1598, 1599; Background Corrected with Scan 1592

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.3	17999	PASS
68	69	0.00	2	0.7	114	PASS
69	198	0.00	100	32.5	15690	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.8	19705	PASS
197	198	0.00	2	0.3	151	PASS
198	198	100	100	100.0	48245	PASS
199	198	5	9	6.9	3344	PASS
275	198	10	60	25.5	12314	PASS
365	198	1	100	2.9	1393	PASS
441	443	0.01	100	76.7	6044	PASS
442	198	50	100	82.8	39970	PASS
443	442	15	24	19.7	7881	PASS