
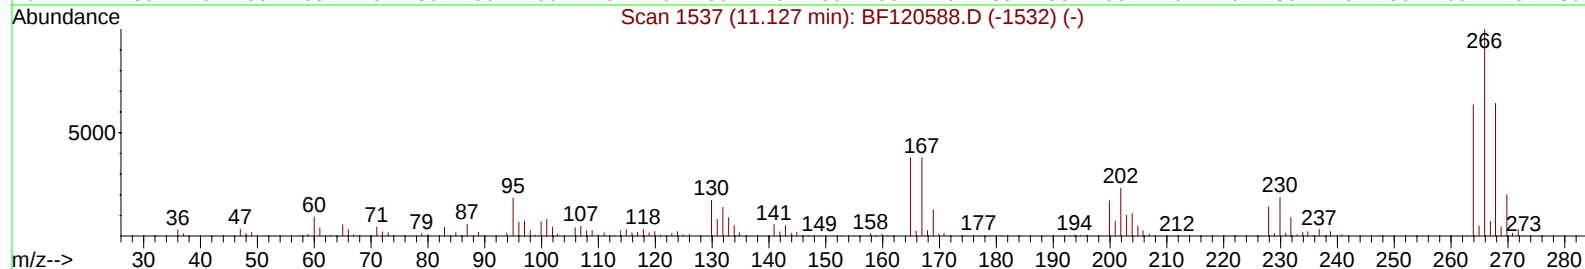
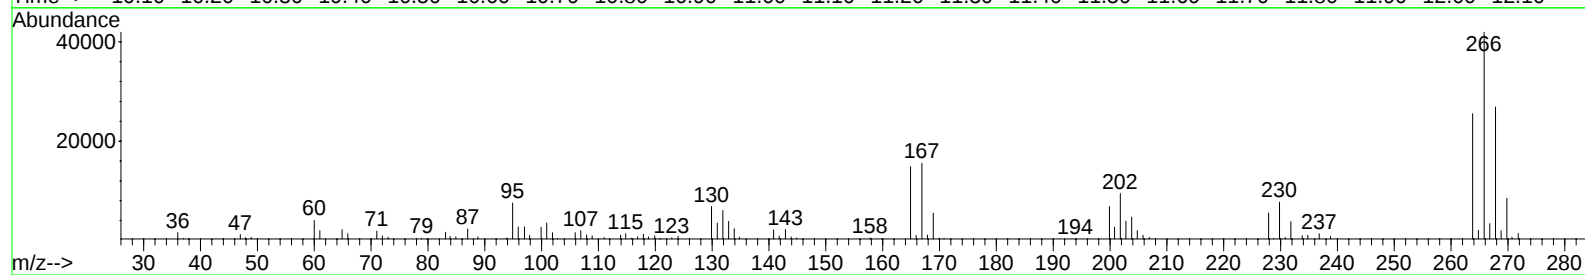


```
Data Path   : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061520\  
Data File   : BF120617.D  
Acq On      : 15 Jun 2020   11:39  
Operator    : JU/CG  
Sample      : DFTPP  
Misc        :  
ALS Vial    : 1      Sample Multiplier: 1
```

Quant Time: Jun 15 17:09:15 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 11 11:28:22 2020
Response via : Initial Calibration

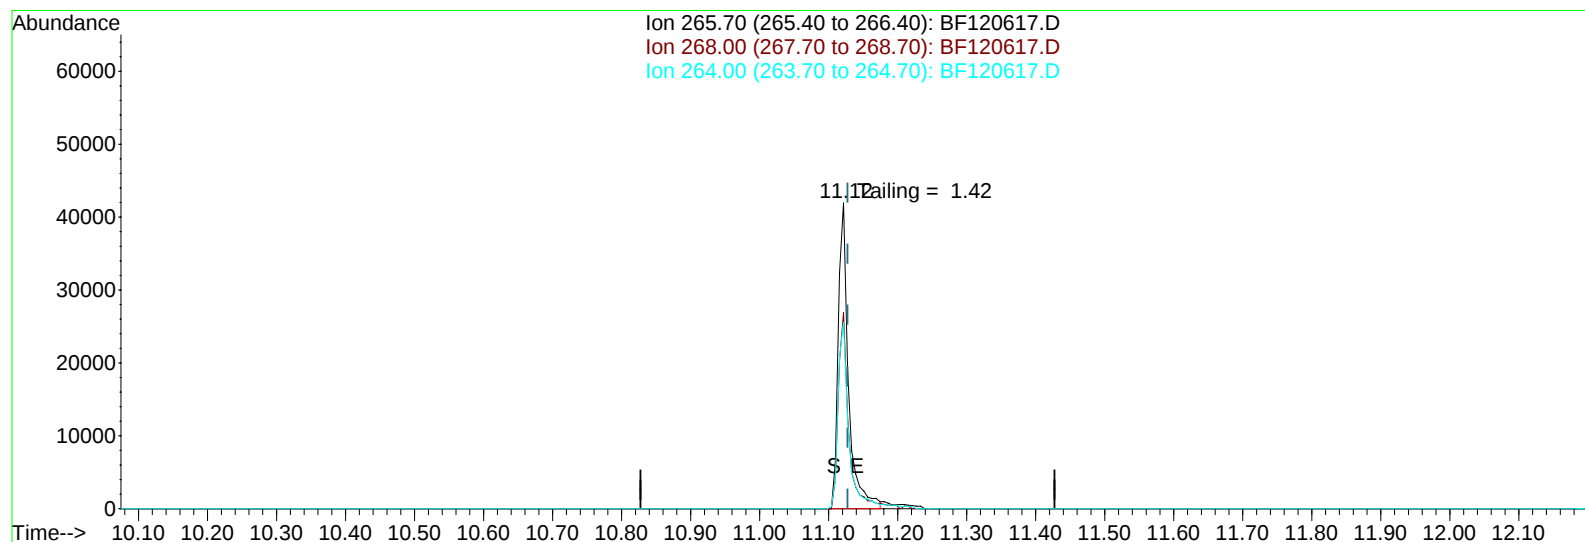

TIC: BF120617.D

(70) Pentachlorophenol (C)




11.121min (-0.006) 6756.09ng

response 44412

Ion	Exp%	Act%
265.70	100	100
268.00	64.20	64.14
264.00	63.50	60.89
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061520\
Data File : BF120617.D
Acq On : 15 Jun 2020 11:39
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 15 17:09:15 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 11 11:28:22 2020
Response via : Initial Calibration

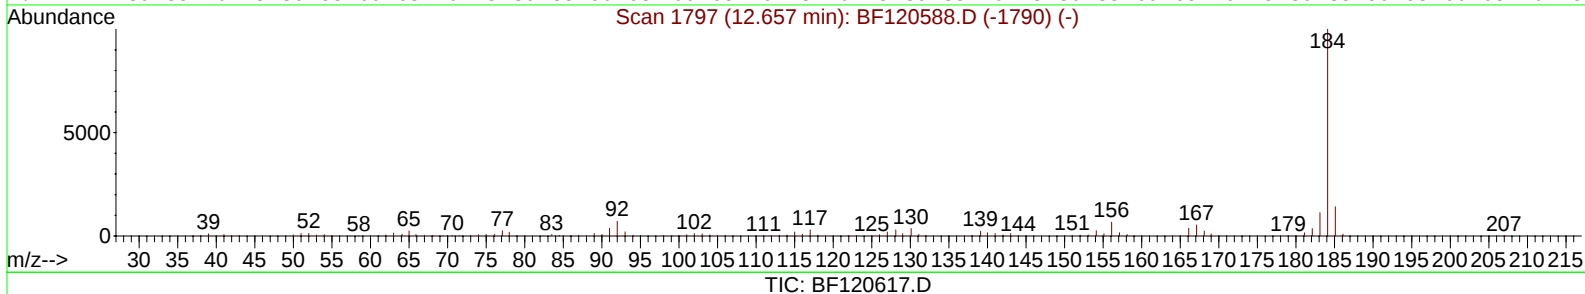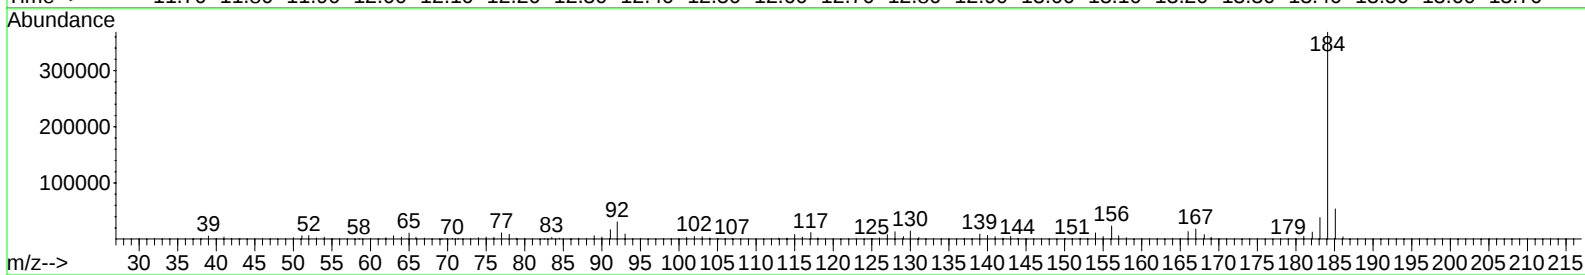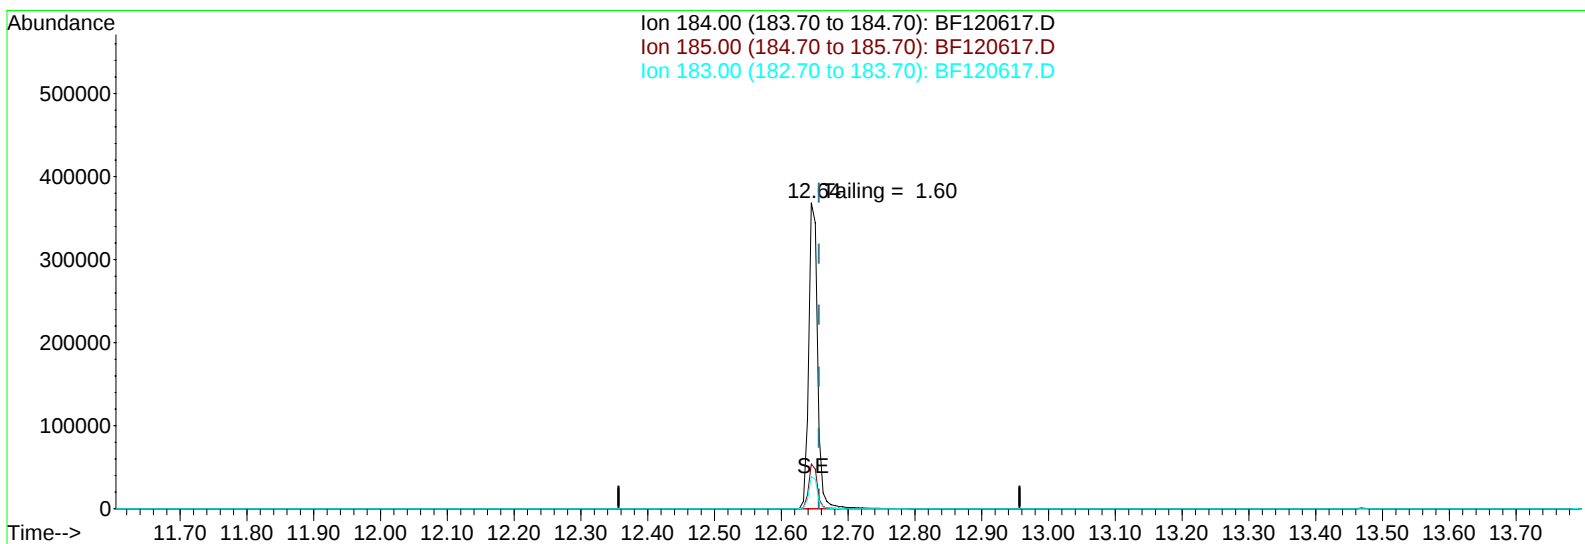

(77) Benzidine

12.645min (-0.012) 19360.37ng

response 342437

Ion	Exp%	Act%
184.00	100	100
185.00	14.20	14.64
183.00	11.30	10.48
0.00	0.00	0.00