
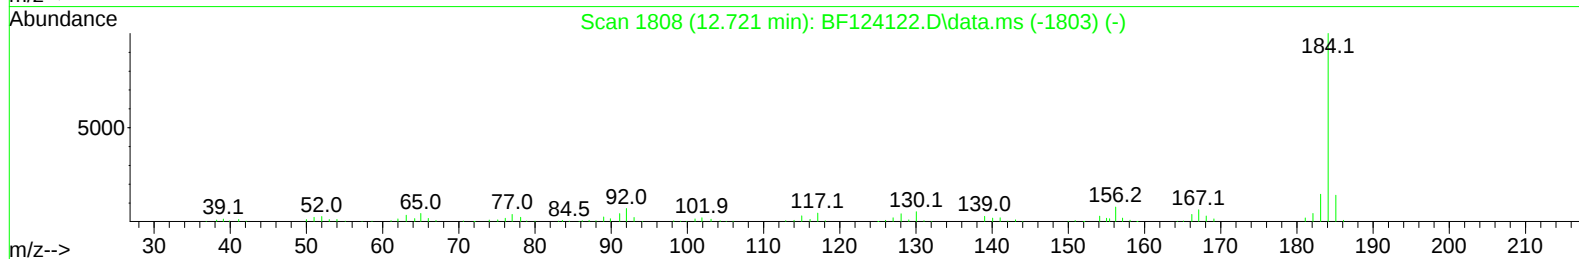
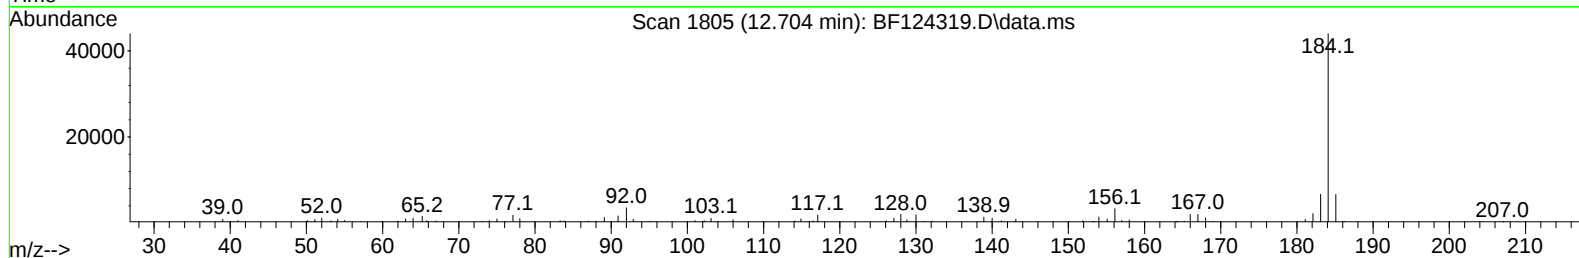


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061521\
Data File : BF124319.D
Acq On : 15 Jun 2021 11:18
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 15 12:59:10 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 14 12:10:02 2021
Response via : Initial Calibration

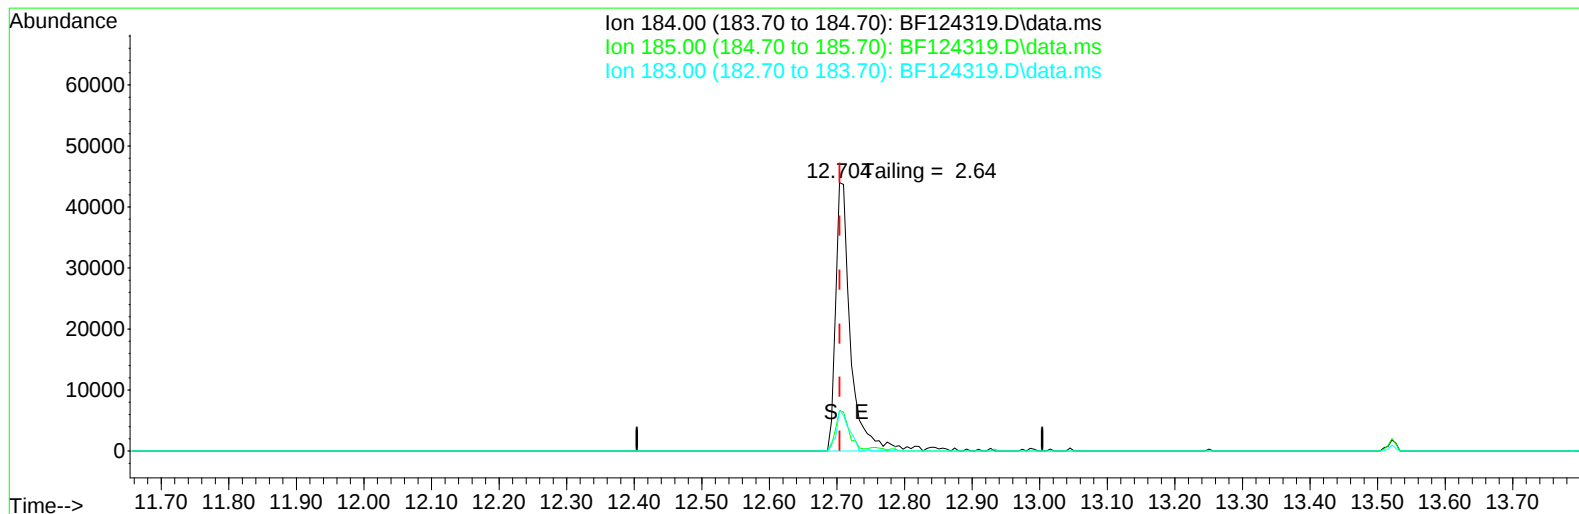

TIC: BF124319.D\data.ms

(77) Benzidine




12.704min (-0.000) 0.00 ng

response 66732

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	15.14
183.00	9.80	15.28#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061521\
Data File : BF124319.D
Acq On : 15 Jun 2021 11:18
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 15 12:59:10 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 14 12:10:02 2021
Response via : Initial Calibration

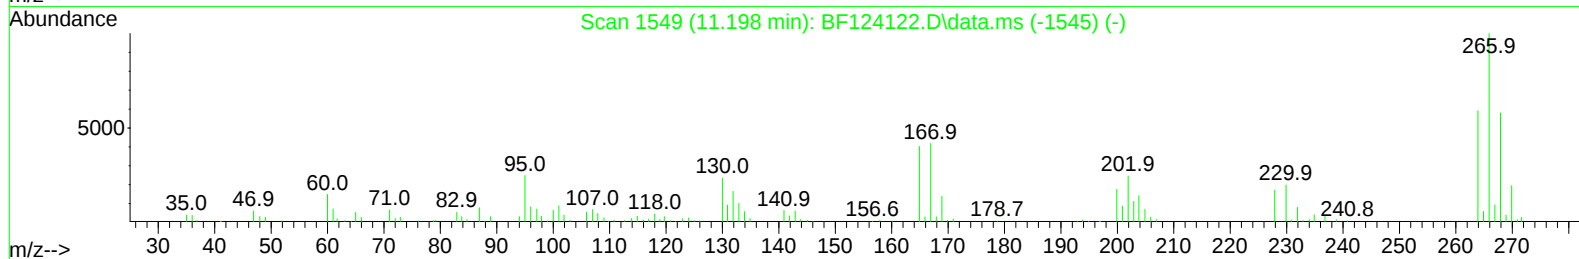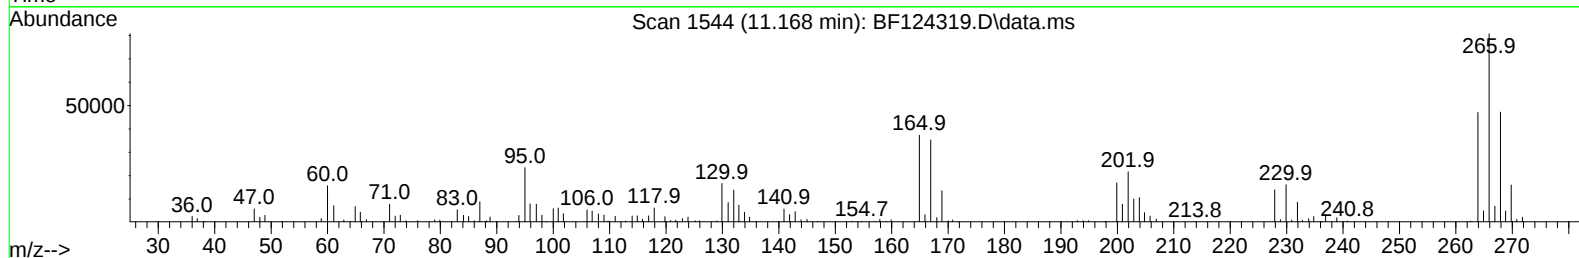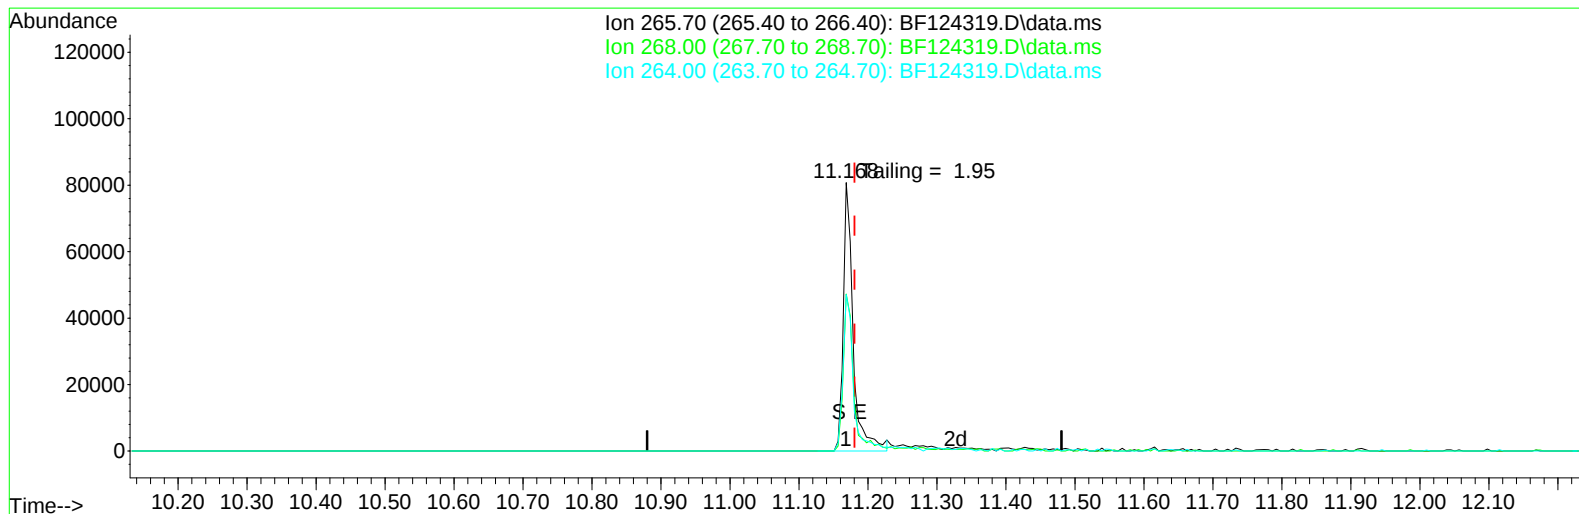

TIC: BF124319.D\data.ms

(70) Pentachlorophenol (C)

11.168min (-0.012) 8884.37 ng

response 79104

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	58.49
264.00	65.70	58.28
0.00	0.00	0.00