

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061521\
 Data File : BF124329.D
 Acq On : 15 Jun 2021 18:38
 Operator : JU/CG
 Sample : M2658-11
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 G-FLOOR-2

Quant Time: Jun 15 19:04:22 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 15 18:30:57 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.787	152	34534	20.00	ng	0.00
21) Naphthalene-d8	8.069	136	124404	20.00	ng	0.00
39) Acenaphthene-d10	9.822	164	75132	20.00	ng	0.00
64) Phenanthrene-d10	11.310	188	130999	20.00	ng	0.00
76) Chrysene-d12	13.957	240	75657	20.00	ng	# 0.00
86) Perylene-d12	15.415	264	62551	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.428	112	273247	119.11	ng	0.01
7) Phenol-d6	6.445	99	308890	100.17	ng	0.00
23) Nitrobenzene-d5	7.351	82	279253	89.03	ng	0.00
42) 2,4,6-Tribromophenol	10.622	330	127750	120.02	ng	0.00
45) 2-Fluorobiphenyl	9.145	172	527531	88.35	ng	0.00
79) Terphenyl-d14	12.904	244	458035	83.12	ng	0.00
Target Compounds						
84) Bis(2-ethylhexyl)phtha...	13.933	149	20183	5.76	ng	# 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061521\
Data File : BF124329.D
Acq On : 15 Jun 2021 18:38
Operator : JU/CG
Sample : M2658-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-FLOOR-2

Quant Time: Jun 15 19:04:22 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 15 18:30:57 2021
Response via : Initial Calibration




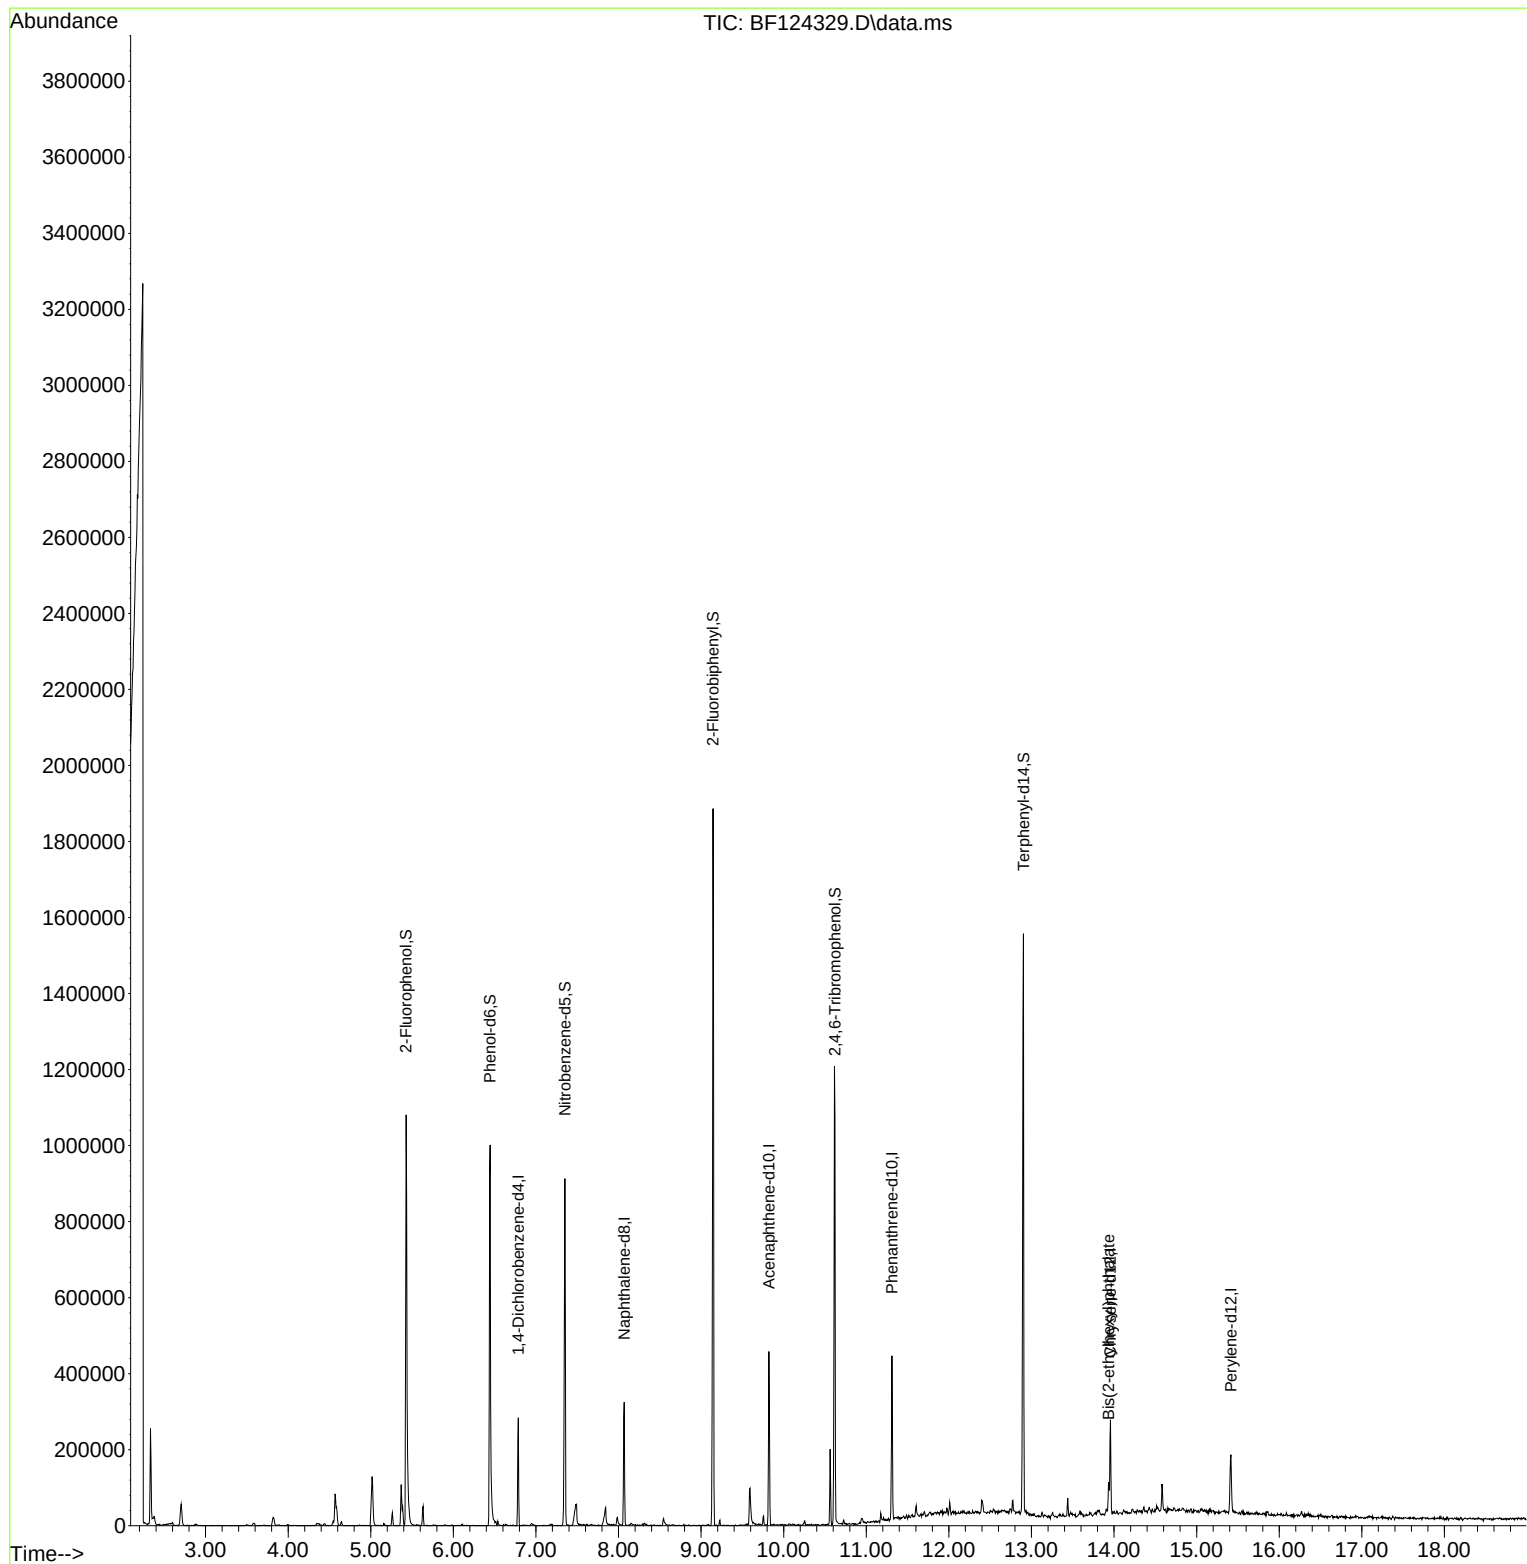


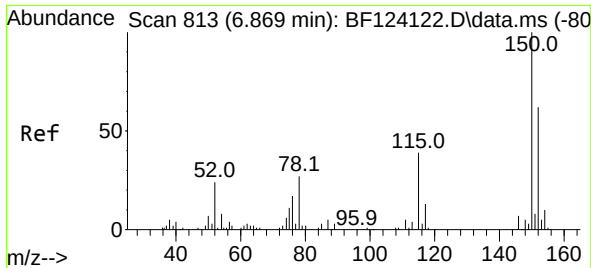

#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.787 min Scan# 799
Delta R.T. 0.001 min
Lab File: BF124329.D
Acq: 15 Jun 2021 18:38




Instrument :
BNA_F
ClientSampled :
G-FLOOR-2


Tgt Ion:152 Resp: 34534
Ion Ratio Lower Upper
152 100
150 148.8 127.0 190.6
115 55.6 54.3 81.5

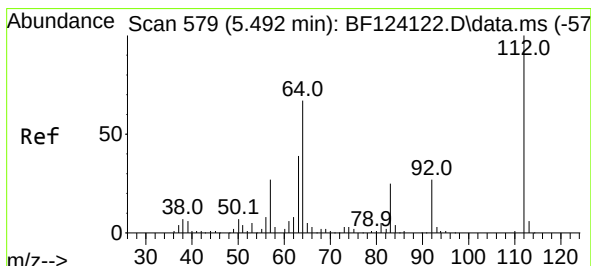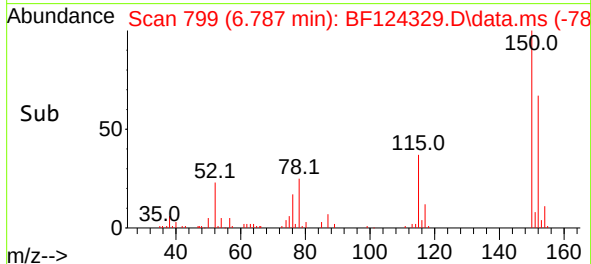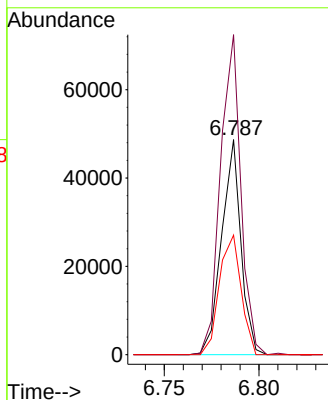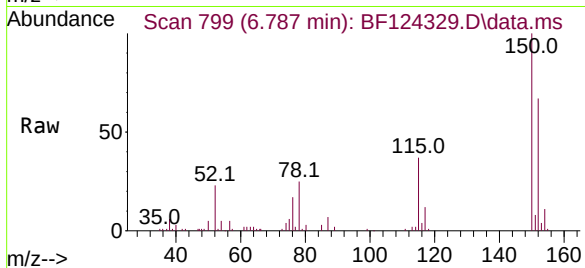

#5
2-Fluorophenol
Concen: 119.11 ng
RT: 5.428 min Scan# 568
Delta R.T. 0.012 min
Lab File: BF124329.D
Acq: 15 Jun 2021 18:38

Tgt Ion:112 Resp: 273247
Ion Ratio Lower Upper
112 100
64 74.5 61.4 92.0
63 41.2 33.0 49.4


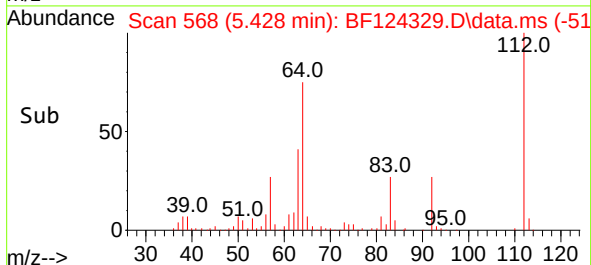
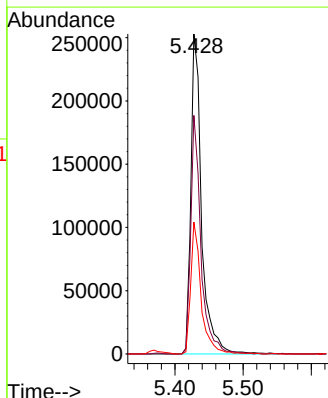
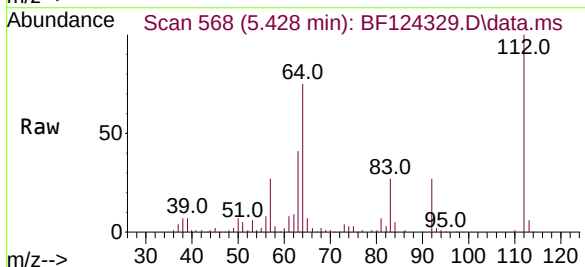


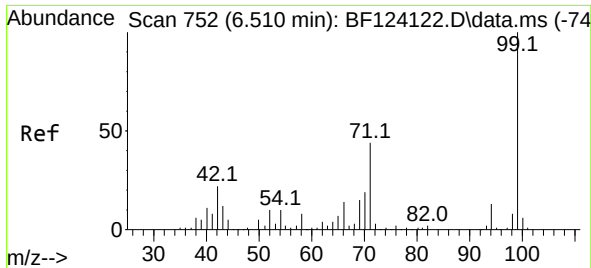

#7
Phenol-d6
Concen: 100.17 ng
RT: 6.445 min Scan# 741
Delta R.T. 0.000 min
Lab File: BF124329.D
Acq: 15 Jun 2021 18:38




Instrument :
BNA_F
ClientSampled :
G-FLOOR-2


Tgt Ion: 99 Resp: 308890
Ion Ratio Lower Upper
99 100
42 20.8 19.8 29.8
71 43.4 31.1 46.7

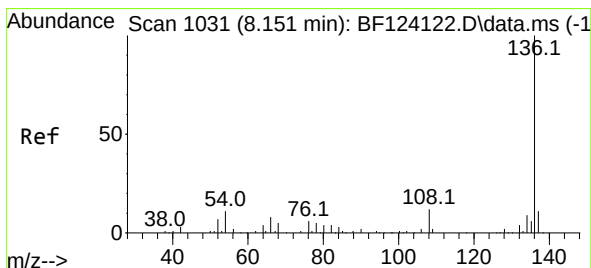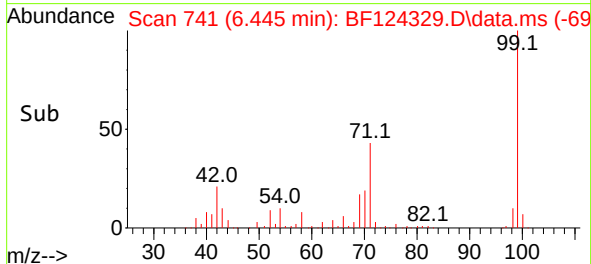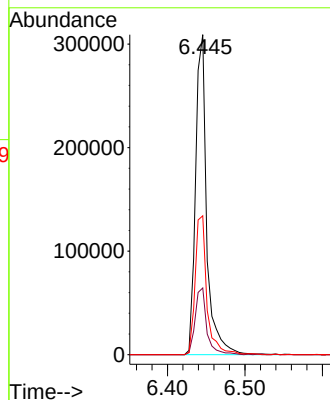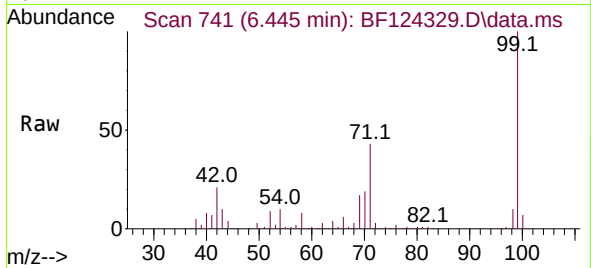

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.069 min Scan# 1017
Delta R.T. -0.006 min
Lab File: BF124329.D
Acq: 15 Jun 2021 18:38

Tgt Ion: 136 Resp: 124404
Ion Ratio Lower Upper
136 100
137 9.8 8.7 13.1
54 11.1 9.8 14.6
68 4.6 4.1 6.1

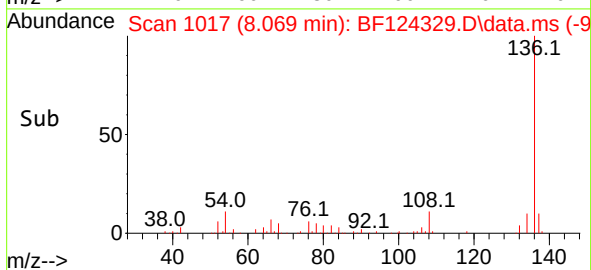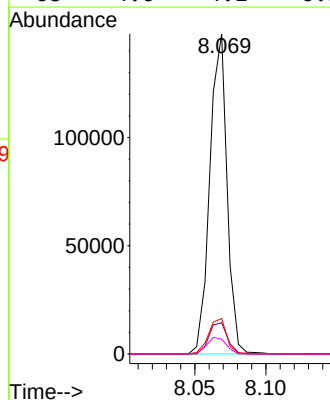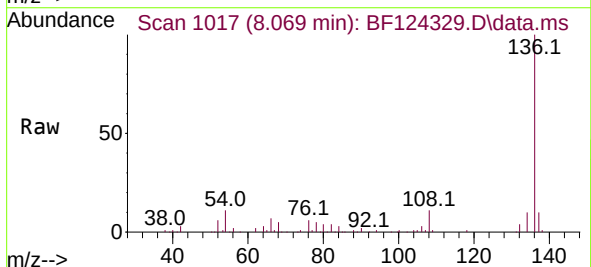

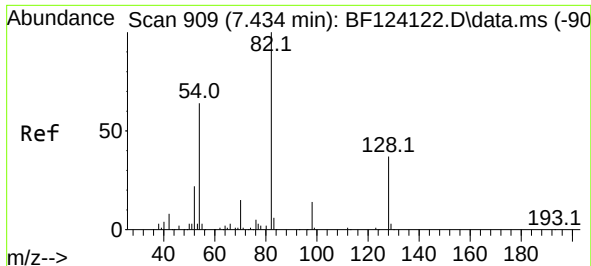

#23

Nitrobenzene-d5

Concen: 89.03 ng

RT: 7.351 min Scan# 895

Delta R.T. -0.006 min

Lab File: BF124329.D

Acq: 15 Jun 2021 18:38

Instrument :

BNA_F

ClientSampleId :

G-FLOOR-2





Tgt Ion: 82 Resp: 279253

Ion Ratio Lower Upper

82 100

128 35.2 29.4 44.2

54 57.3 54.1 81.1

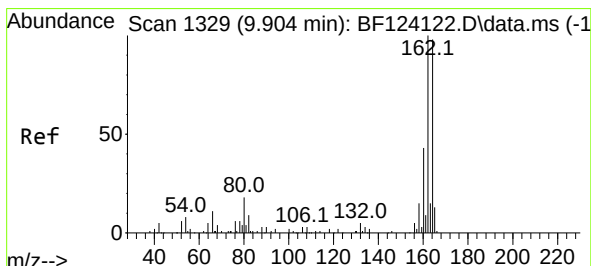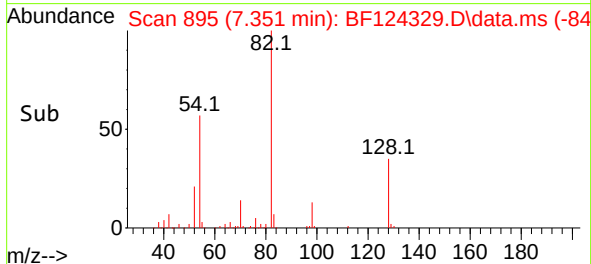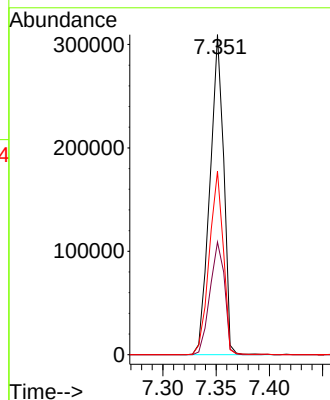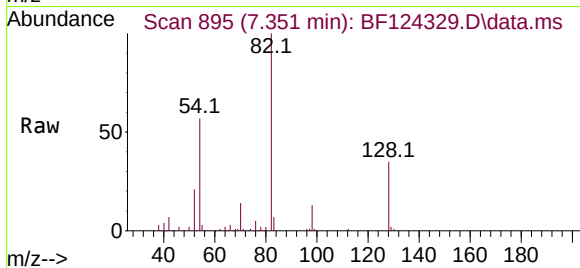

#39

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.822 min Scan# 1315

Delta R.T. -0.006 min

Lab File: BF124329.D

Acq: 15 Jun 2021 18:38




Tgt Ion: 164 Resp: 75132


Ion Ratio Lower Upper

164 100

162 108.1 80.7 121.1

160 44.6 37.3 55.9


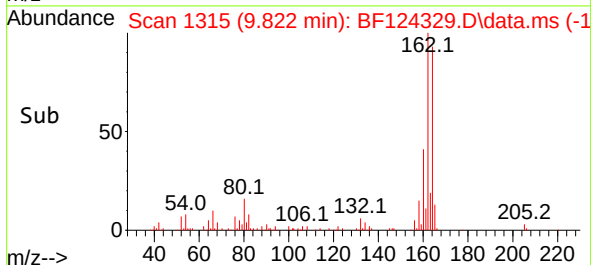
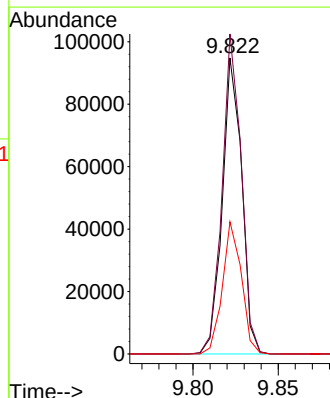
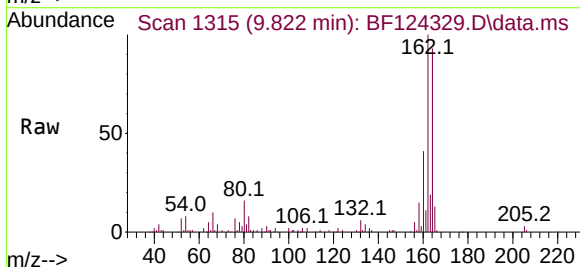


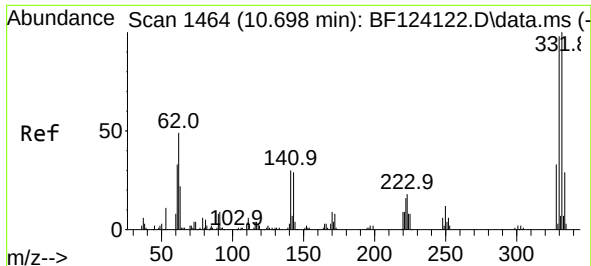

#42
2,4,6-Tribromophenol
Concen: 120.02 ng
RT: 10.622 min Scan# 1451
Delta R.T. 0.000 min
Lab File: BF124329.D
Acq: 15 Jun 2021 18:38




Instrument :
BNA_F
ClientSampled :
G-FLOOR-2


Tgt Ion: 330 Resp: 127750
Ion Ratio Lower Upper
330 100
332 98.3 77.1 115.7
141 39.8 27.9 41.9

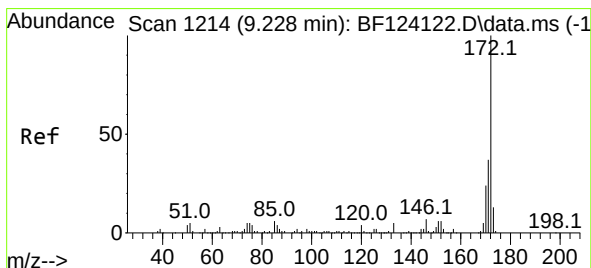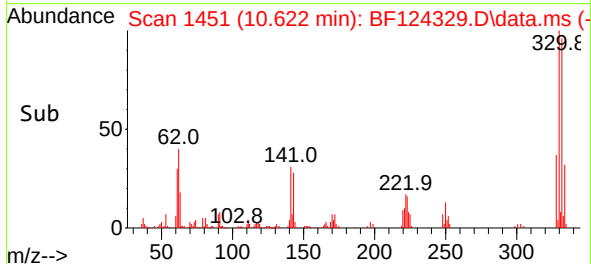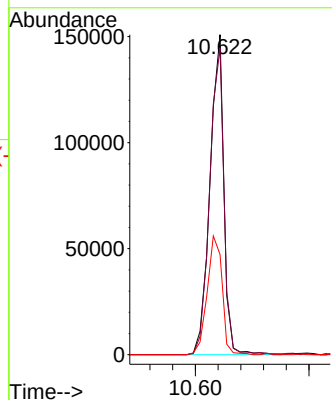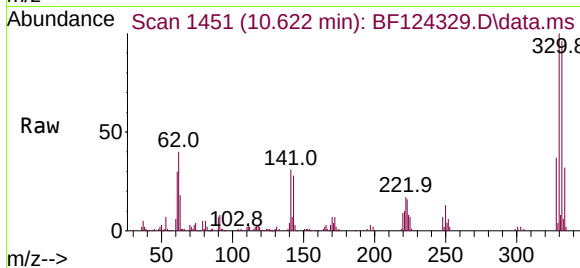

#45
2-Fluorobiphenyl
Concen: 88.35 ng
RT: 9.145 min Scan# 1200
Delta R.T. -0.006 min
Lab File: BF124329.D
Acq: 15 Jun 2021 18:38

Tgt Ion: 172 Resp: 527531
Ion Ratio Lower Upper
172 100
171 37.5 28.1 42.1
170 23.4 19.2 28.8


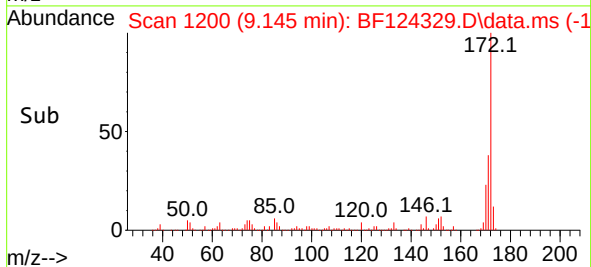
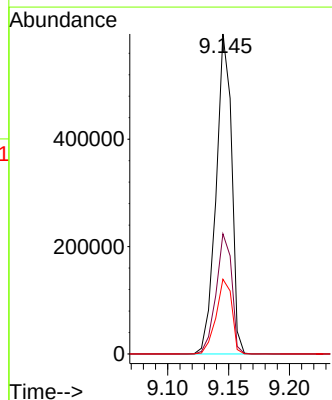
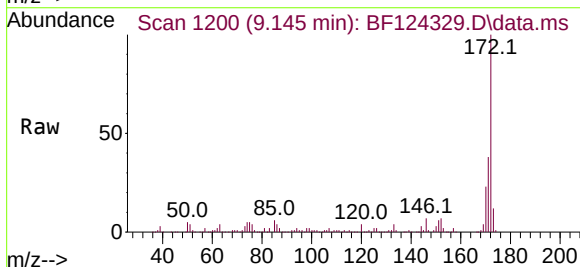


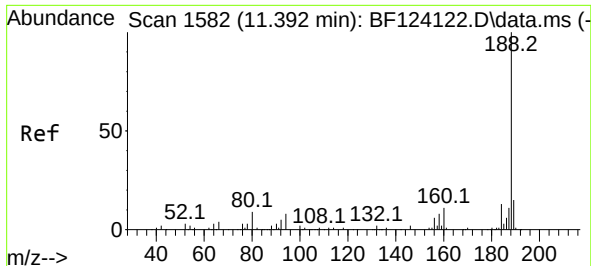

#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.310 min Scan# 1568
Delta R.T. -0.006 min
Lab File: BF124329.D
Acq: 15 Jun 2021 18:38




Instrument :
BNA_F
ClientSampleId :
G-FLOOR-2


Tgt Ion:188 Resp: 130999
Ion Ratio Lower Upper
188 100
94 7.0 6.9 10.3
80 10.5 8.2 12.2

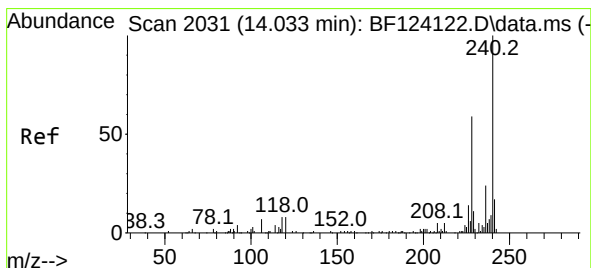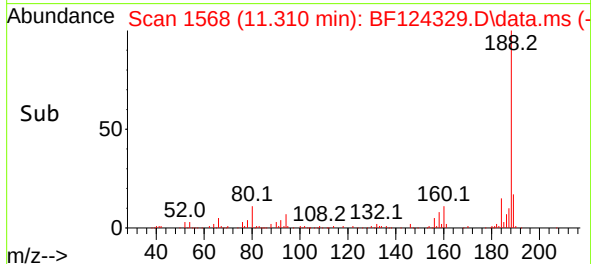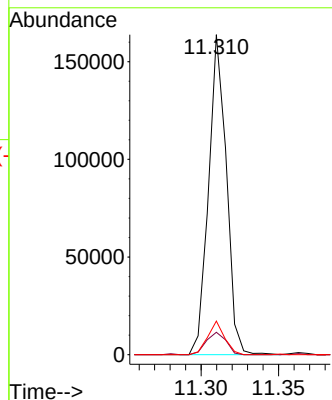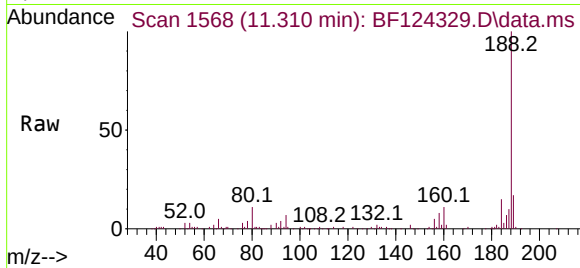

#76
Chrysene-d12
Concen: 20.00 ng
RT: 13.957 min Scan# 2018
Delta R.T. -0.006 min
Lab File: BF124329.D
Acq: 15 Jun 2021 18:38

Tgt Ion:240 Resp: 75657
Ion Ratio Lower Upper
240 100
120 6.9 7.2 10.8#
236 24.3 19.0 28.4


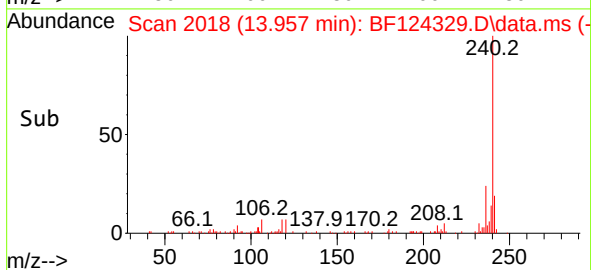
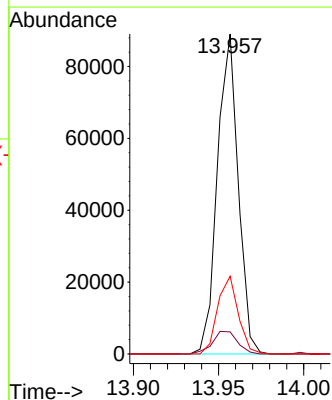
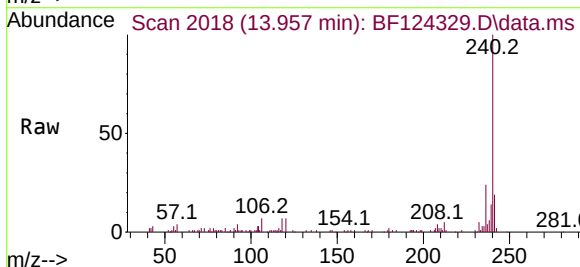


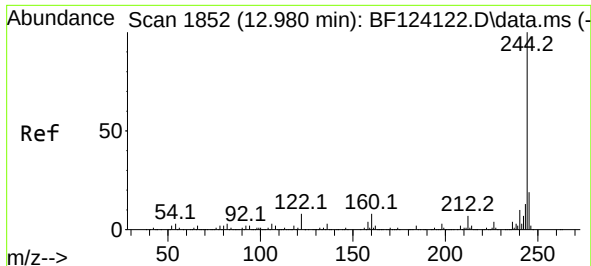

#79
 Terphenyl-d14
 Concen: 83.12 ng
 RT: 12.904 min Scan# 1839
 Delta R.T. 0.000 min
 Lab File: BF124329.D
 Acq: 15 Jun 2021 18:38




Instrument :
 BNA_F
 ClientSampleId :
 G-FLOOR-2


Tgt Ion:244 Resp: 458035
 Ion Ratio Lower Upper
 244 100
 212 7.6 5.7 8.5
 122 8.4 9.7 14.5#

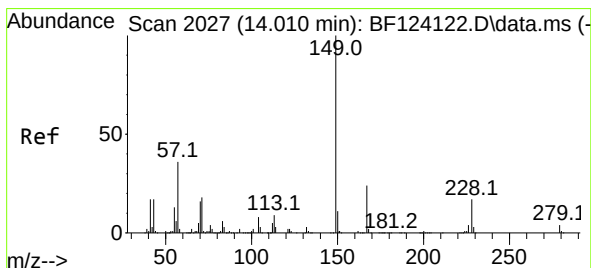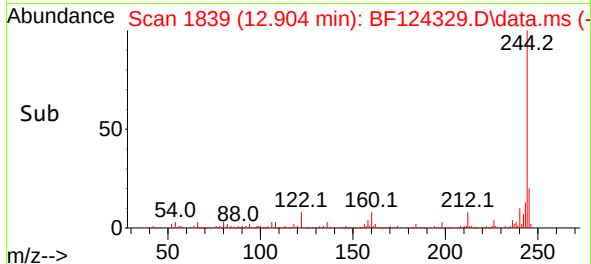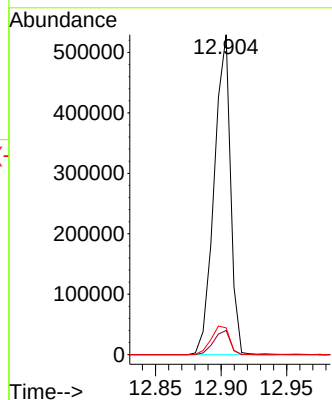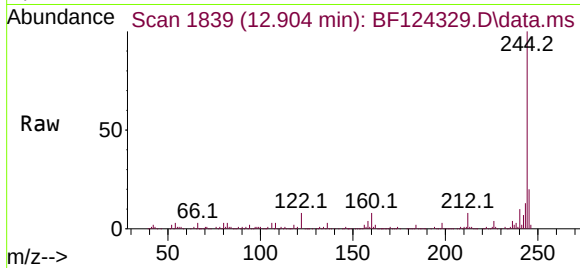

#84
 Bis(2-ethylhexyl)phthalate
 Concen: 5.76 ng
 RT: 13.933 min Scan# 2014
 Delta R.T. -0.006 min
 Lab File: BF124329.D
 Acq: 15 Jun 2021 18:38

Tgt Ion:149 Resp: 20183
 Ion Ratio Lower Upper
 149 100
 167 22.7 21.8 32.6
 279 6.3 3.3 4.9#

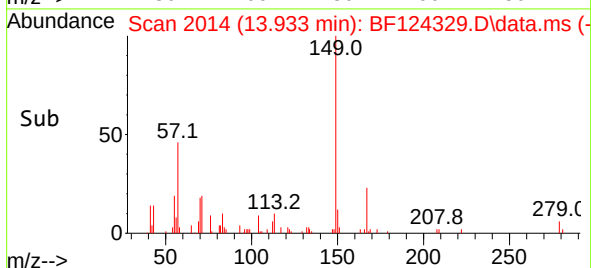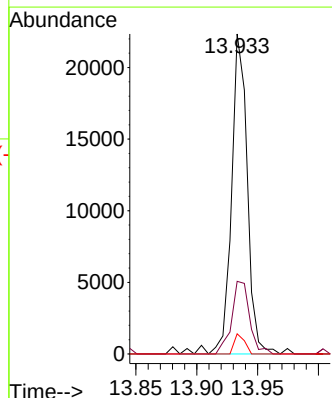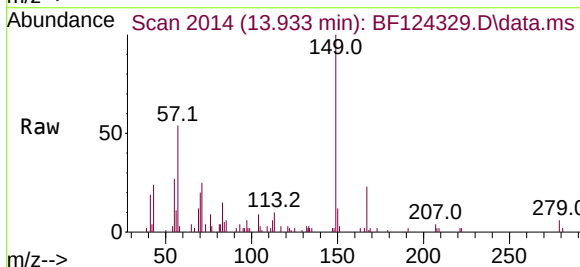

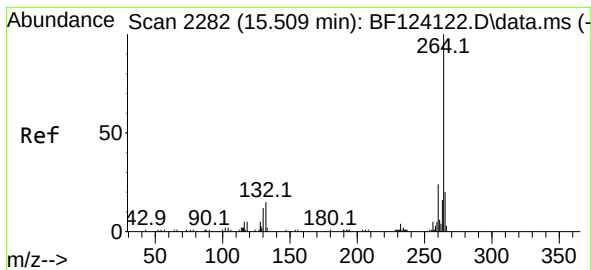

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.415 min Scan# 2266
 Delta R.T. 0.000 min
 Lab File: BF124329.D
 Acq: 15 Jun 2021 18:38

Instrument :
 BNA_F
 ClientSampleId :
 G-FLOOR-2

Tgt Ion:264 Resp: 62551
 Ion Ratio Lower Upper
 264 100
 260 19.2 18.7 28.1
 265 20.3 17.8 26.8

