
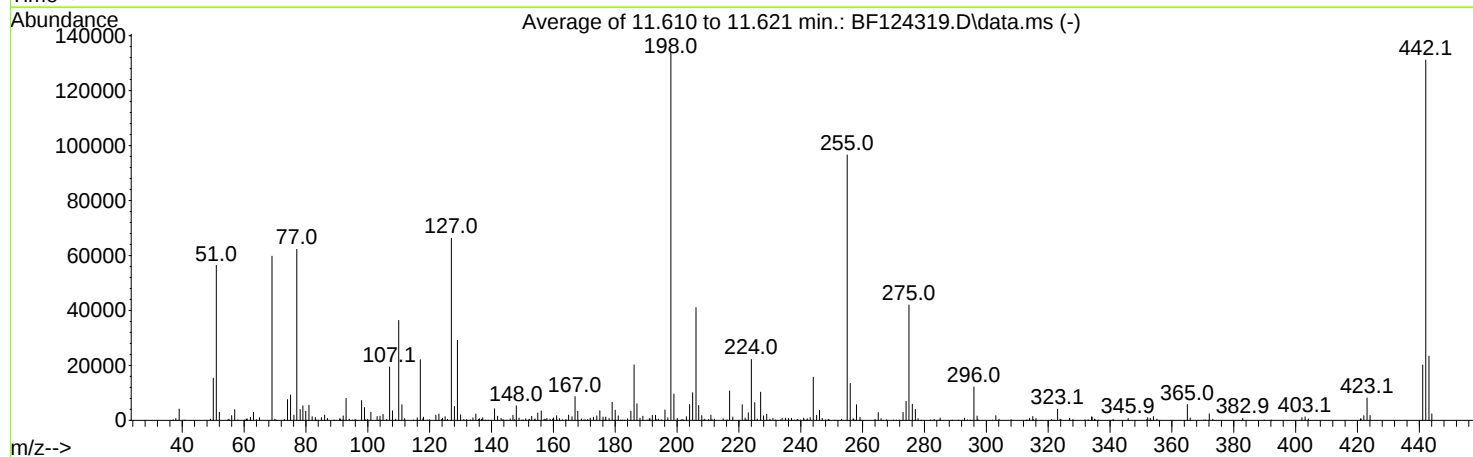


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061521\
 Data File : BF124319.D
 Acq On : 15 Jun 2021 11:18
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 15 20:09:26 2021

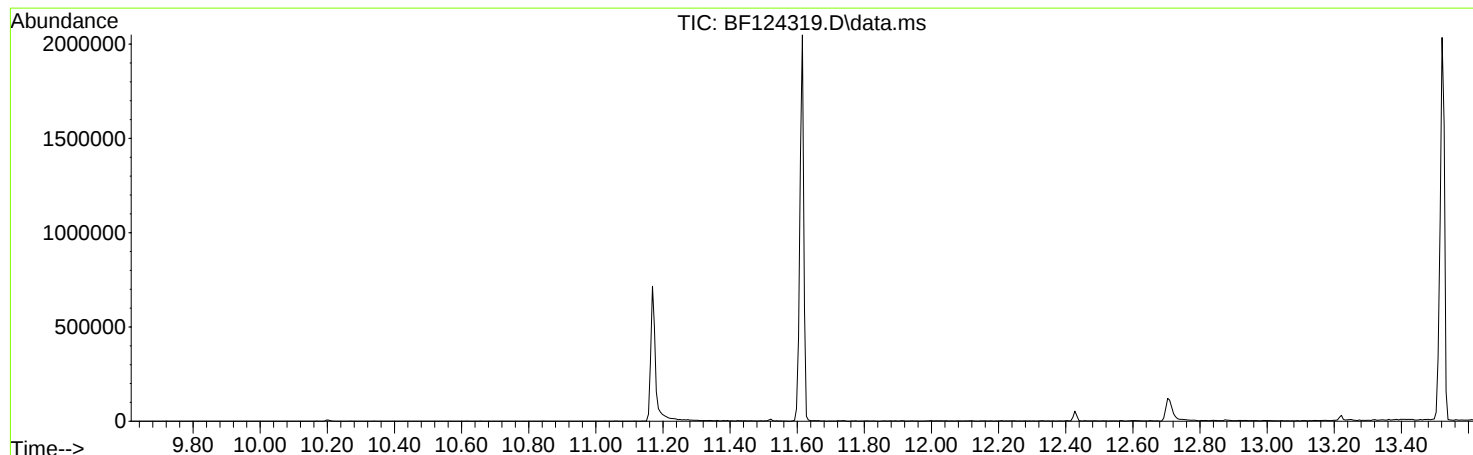

AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1613

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.1	56402	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	44.6	59720	PASS
70	69	0.00	2	0.6	386	PASS
127	198	10	80	49.5	66271	PASS
197	198	0.00	2	0.7	937	PASS
198	198	100	100	100.0	133861	PASS
199	198	5	9	7.2	9611	PASS
275	198	10	60	31.4	42000	PASS
365	198	1	100	4.3	5767	PASS
441	198	0.01	100	15.1	20153	PASS
442	442	50	100	100.0	131125	PASS
443	442	15	24	17.8	23329	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/15/2021	BNA_F	<u>BF124319.D</u>
Compound Name	Response	Retention Time
DDT	331110	13.52
DDD	3810	13.22
DDE	320	12.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4130	335240	1.23

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061521\
Data File : BF124319.D
Acq On : 15 Jun 2021 11:18
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 15 12:59:10 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 14 12:10:02 2021
Response via : Initial Calibration

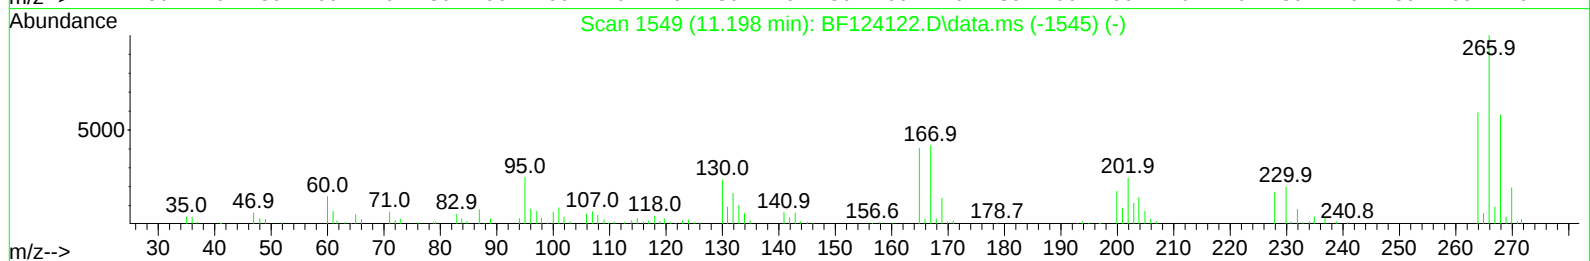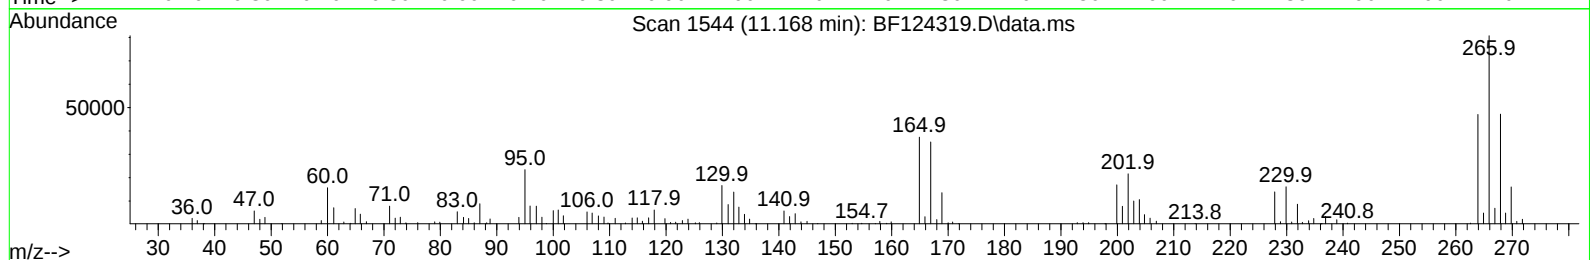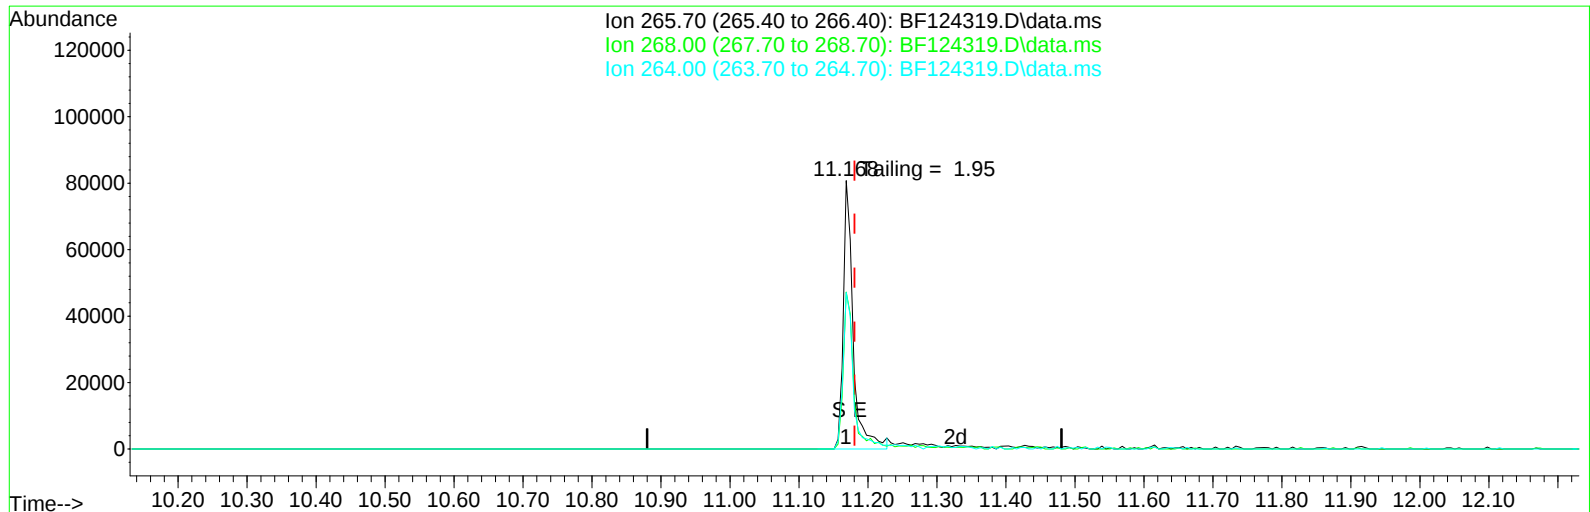

TIC: BF124319.D\data.ms

(70) Pentachlorophenol (C)

11.168min (-0.012) 8884.37 ng




response 79104

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	58.49
264.00	65.70	58.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061521\
Data File : BF124319.D
Acq On : 15 Jun 2021 11:18
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 15 12:59:10 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 14 12:10:02 2021
Response via : Initial Calibration

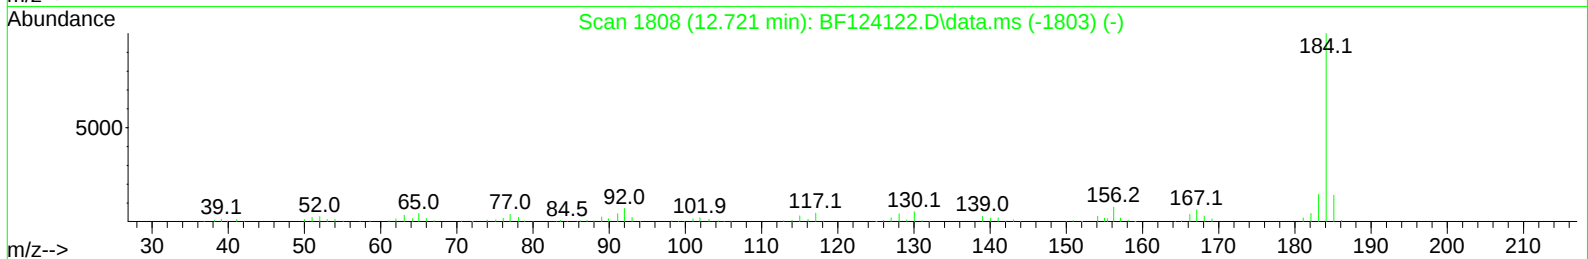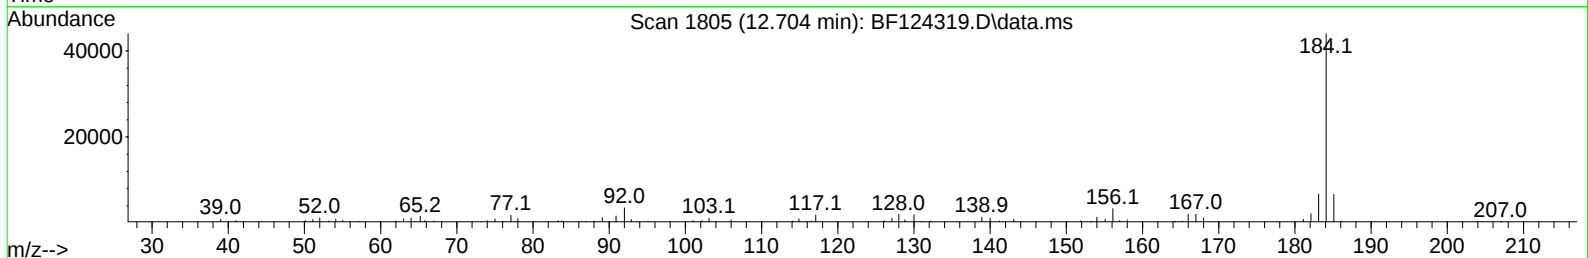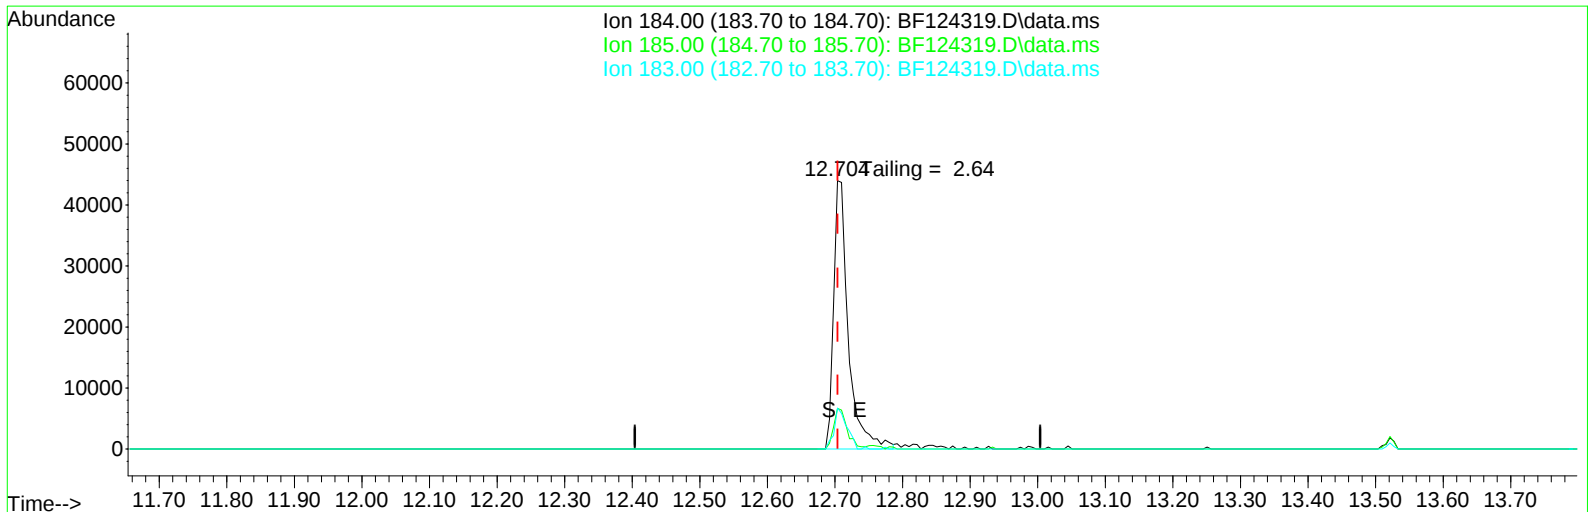

TIC: BF124319.D\data.ms

(77) Benzidine

12.704min (-0.000) 0.00 ng

response 66732

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	15.14
183.00	9.80	15.28#
0.00	0.00	0.00