

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061522\
 Data File : BF128820.D
 Acq On : 15 Jun 2022 11:51
 Operator : CG\JU
 Sample : PB145493TB
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB145493TB

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128820.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.022	461	465	474	rVB2	50607	74634	1.75%	0.324%
2	5.428	530	534	551	rBV	3170655	2850644	66.90%	12.380%
3	6.439	701	706	709	rBV	2927433	2835652	66.55%	12.315%
4	6.781	760	764	767	rBV	737682	583700	13.70%	2.535%
5	7.351	855	861	864	rBV	1802869	1987139	46.64%	8.630%
6	8.063	977	982	985	rBV	867266	753630	17.69%	3.273%
7	9.145	1159	1166	1169	rBV	4101148	3792959	89.02%	16.472%
8	9.822	1275	1281	1284	rBV	1036587	890933	20.91%	3.869%
9	10.616	1411	1416	1419	rBV	2405991	2176067	51.07%	9.450%
10	11.310	1530	1534	1537	rVB	1180865	949041	22.27%	4.122%
11	12.904	1799	1805	1808	rBV	4437167	4260952	100.00%	18.505%
12	13.957	1980	1984	1987	rBV	1013759	888524	20.85%	3.859%
13	14.045	1993	1999	2003	rBV	200877	229565	5.39%	0.997%
14	15.409	2226	2231	2236	rBV	638230	752711	17.67%	3.269%




Sum of corrected areas: 23026151

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061522\
Data File : BF128820.D
Acq On : 15 Jun 2022 11:51
Operator : CG\JU
Sample : PB145493TB
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145493TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

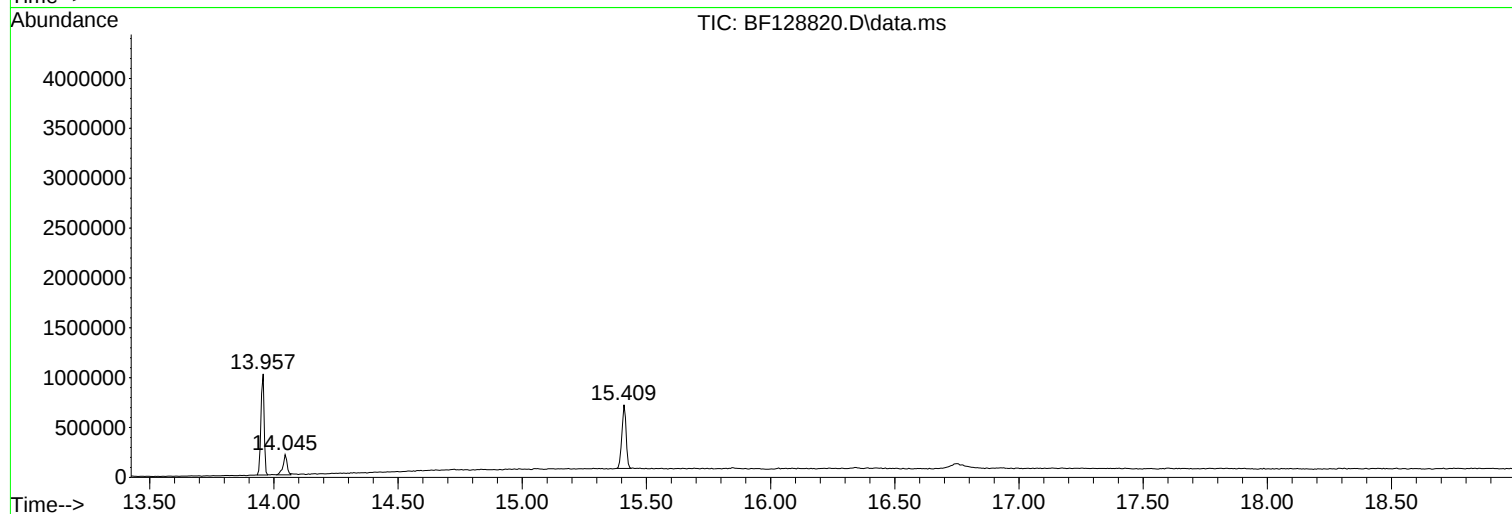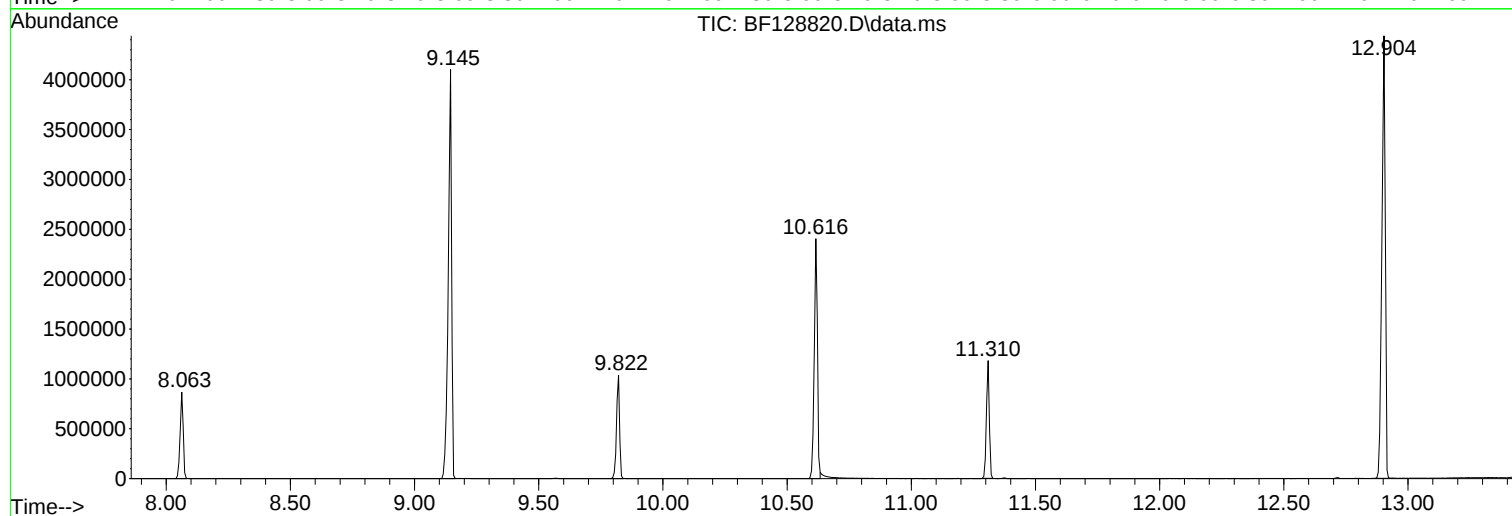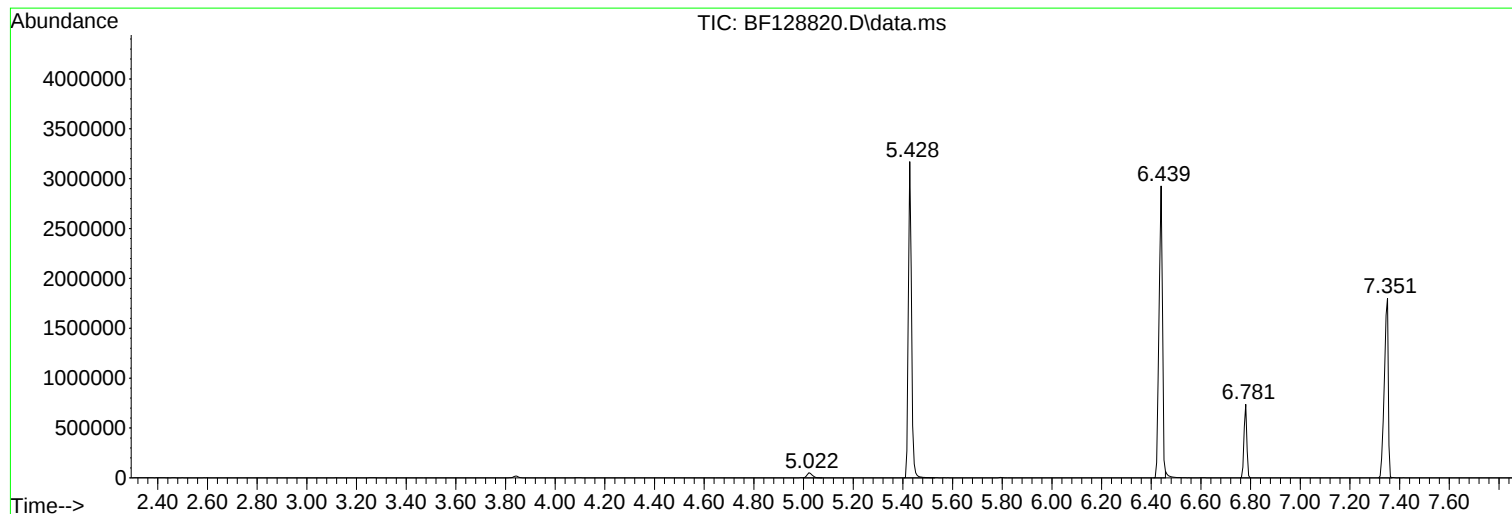

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061522\
Data File : BF128820.D
Acq On : 15 Jun 2022 11:51
Operator : CG\JU
Sample : PB145493TB
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145493TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061522\
Data File : BF128820.D
Acq On : 15 Jun 2022 11:51
Operator : CG\JU
Sample : PB145493TB
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145493TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------