

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061522\
 Data File : BF128825.D
 Acq On : 15 Jun 2022 14:34
 Operator : CG\JU
 Sample : N3340-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CS-3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128825.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.422	529	533	548	rBV	2455036	2199930	94.52%	14.092%
2	6.439	702	706	717	rVB	2552396	2249558	96.65%	14.410%
3	6.781	760	764	767	rBV	663504	497878	21.39%	3.189%
4	7.351	855	861	864	rBV	1458433	1471811	63.23%	9.428%
5	8.063	978	982	986	rBV	734432	607129	26.08%	3.889%
6	9.145	1161	1166	1169	rBV	2788730	2327582	100.00%	14.910%
7	9.822	1277	1281	1284	rVB	744688	567555	24.38%	3.636%
8	10.616	1412	1416	1419	rBV	1432697	1189921	51.12%	7.622%
9	11.310	1530	1534	1536	rBV	696419	549213	23.60%	3.518%
10	11.333	1536	1538	1541	rVB	134756	95500	4.10%	0.612%
11	11.810	1616	1619	1622	rBV	54172	49306	2.12%	0.316%
12	11.839	1622	1624	1628	rVB	69686	61330	2.63%	0.393%
13	11.921	1635	1638	1640	rBV	61609	58053	2.49%	0.372%
14	11.945	1640	1642	1647	rVB	45988	39585	1.70%	0.254%
15	12.110	1666	1670	1672	rBV2	26140	26673	1.15%	0.171%
16	12.139	1672	1675	1681	rVB2	25764	28039	1.20%	0.180%
17	12.363	1709	1713	1716	rBV	52156	59050	2.54%	0.378%
18	12.451	1725	1728	1733	rBV2	24961	32544	1.40%	0.208%
19	12.521	1737	1740	1744	rBV	106856	97619	4.19%	0.625%
20	12.568	1745	1748	1750	rBV3	19878	26654	1.15%	0.171%
21	12.751	1775	1779	1785	rBV	136374	160408	6.89%	1.028%
22	12.898	1800	1804	1808	rBV	2136430	1988931	85.45%	12.741%
23	12.968	1814	1816	1824	rBV2	25323	48608	2.09%	0.311%
24	13.310	1872	1874	1878	rVB2	32270	29506	1.27%	0.189%
25	13.957	1980	1984	1986	rBV	463727	415579	17.85%	2.662%
26	13.980	1986	1988	1993	rVB	55814	54326	2.33%	0.348%
27	14.051	1996	2000	2003	rVV	252261	254787	10.95%	1.632%
28	15.409	2228	2231	2236	rBV	274795	423814	18.21%	2.715%




Sum of corrected areas: 15610889

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061522\
Data File : BF128825.D
Acq On : 15 Jun 2022 14:34
Operator : CG\JU
Sample : N3340-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CS-3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

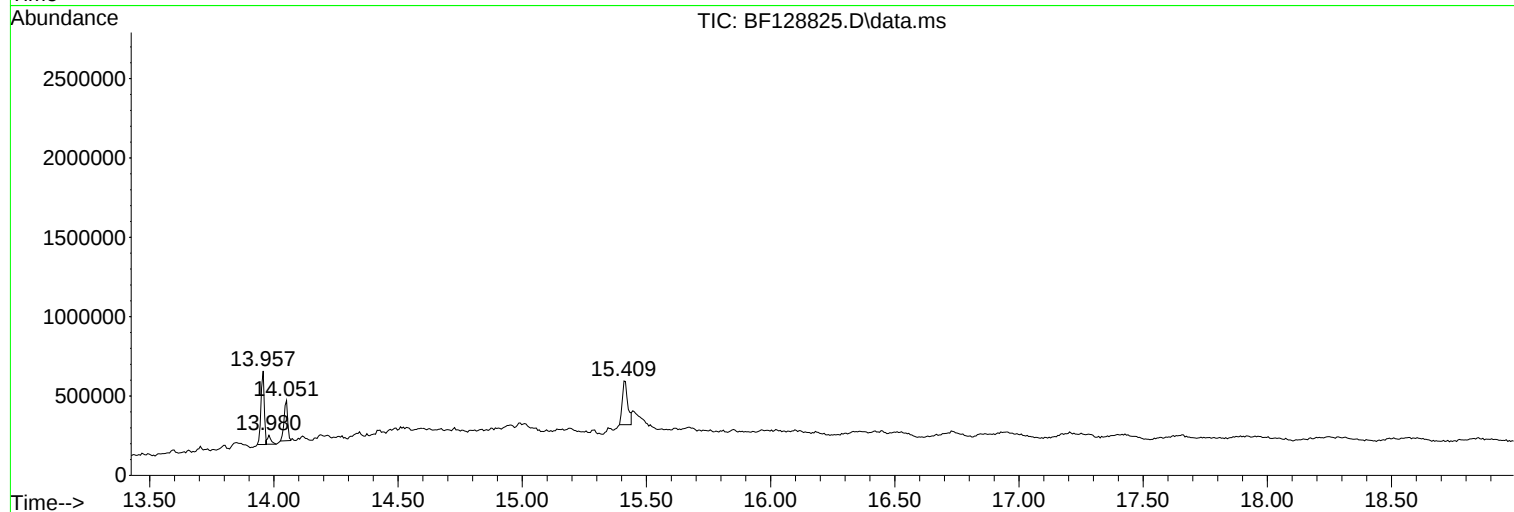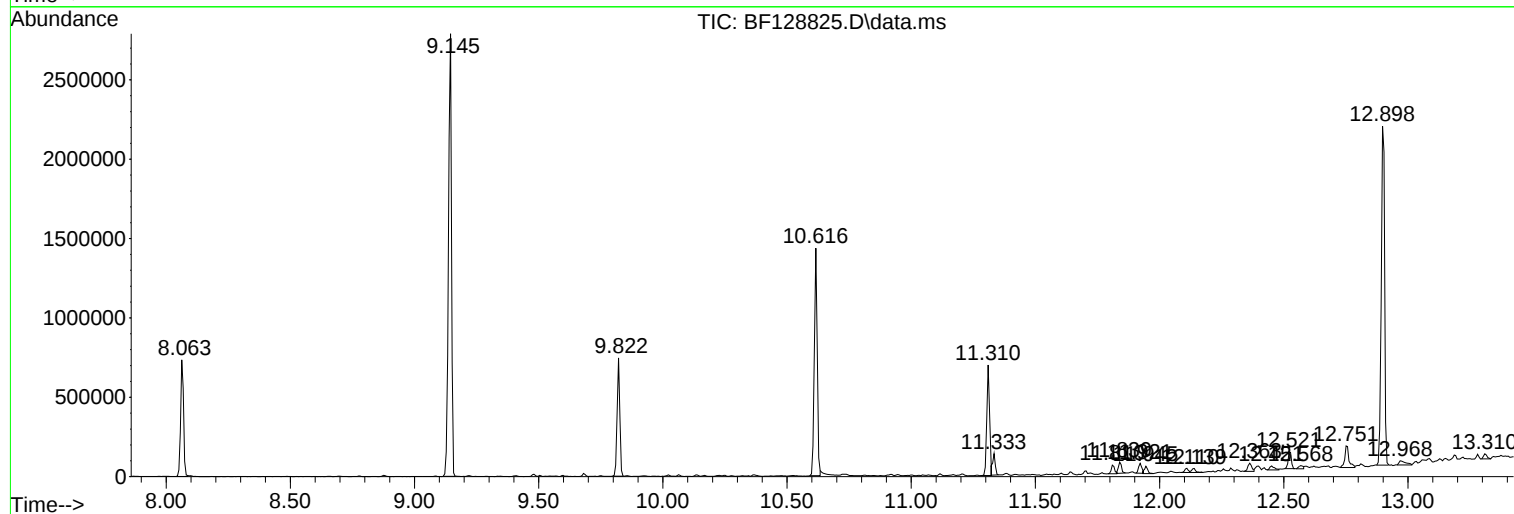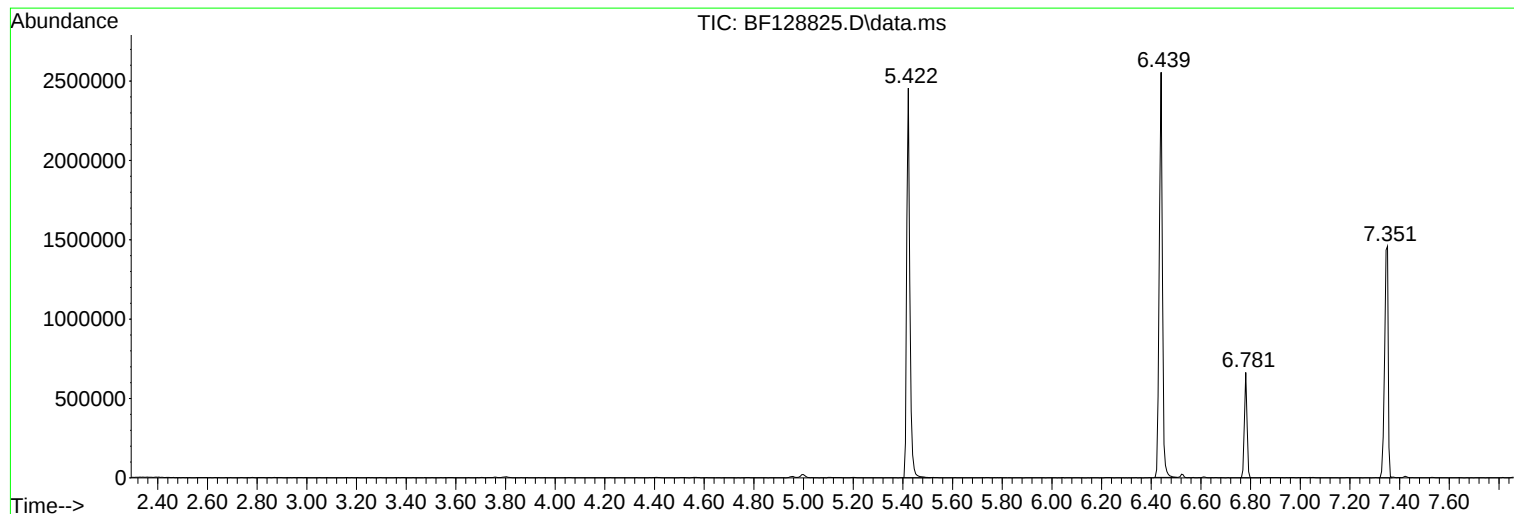

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061522\
Data File : BF128825.D
Acq On : 15 Jun 2022 14:34
Operator : CG\JU
Sample : N3340-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CS-3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061522\
Data File : BF128825.D
Acq On : 15 Jun 2022 14:34
Operator : CG\JU
Sample : N3340-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CS-3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------