
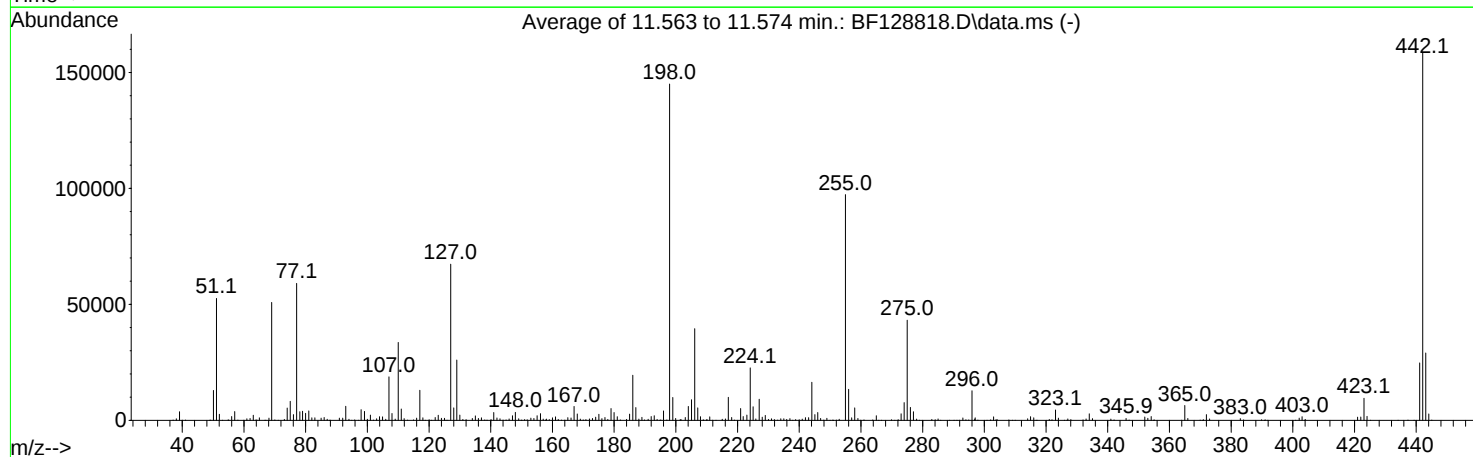


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061522\
 Data File : BF128818.D
 Acq On : 15 Jun 2022 10:24
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 14 14:53:53 2022

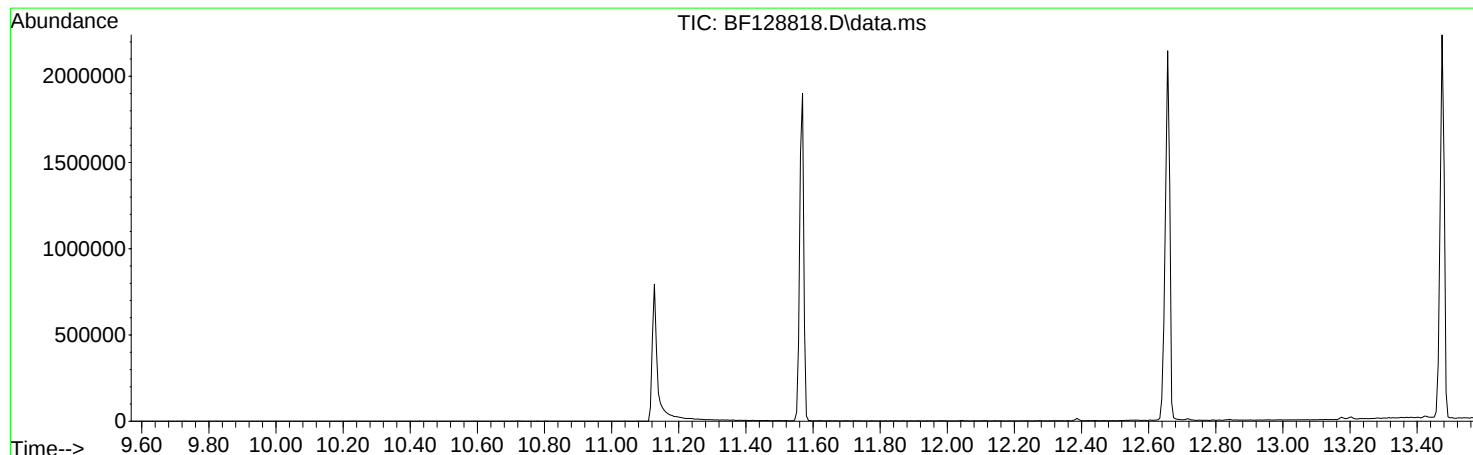




AutoFind: Scans 1577, 1578, 1579; Background Corrected with Scan 1571

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	52575	PASS
68	69	0.00	2	1.9	981	PASS
69	198	0.00	100	35.1	50824	PASS
70	69	0.00	2	0.5	247	PASS
127	198	10	80	46.4	67312	PASS
197	198	0.00	2	0.1	193	PASS
198	198	100	100	100.0	144987	PASS
199	198	5	9	6.8	9875	PASS
275	198	10	60	29.8	43152	PASS
365	198	1	100	4.4	6446	PASS
441	198	0.01	100	17.1	24747	PASS
442	442	50	100	100.0	158603	PASS
443	442	15	24	18.3	29029	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061522\
Data File : BF128818.D
Acq On : 15 Jun 2022 10:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 15 13:04:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 14 14:53:53 2022
Response via : Initial Calibration

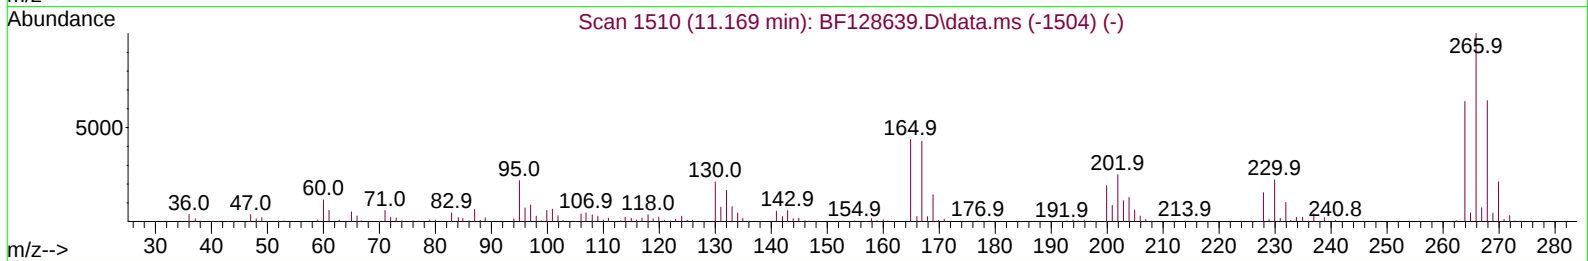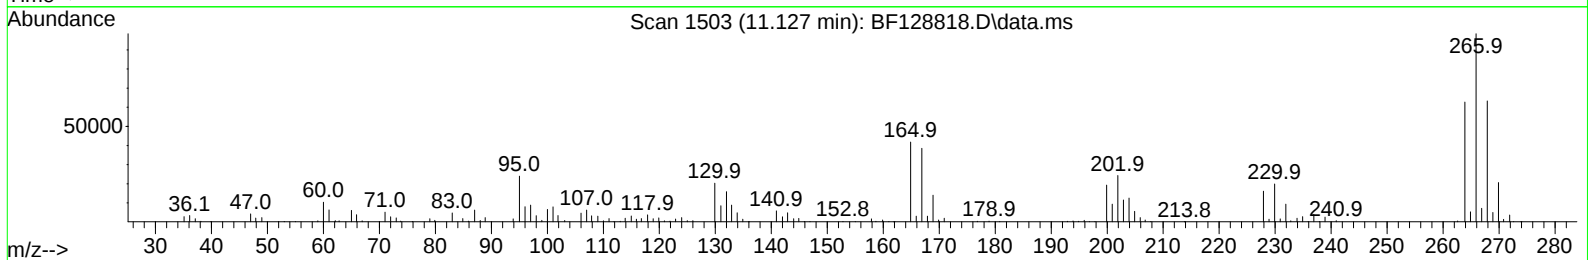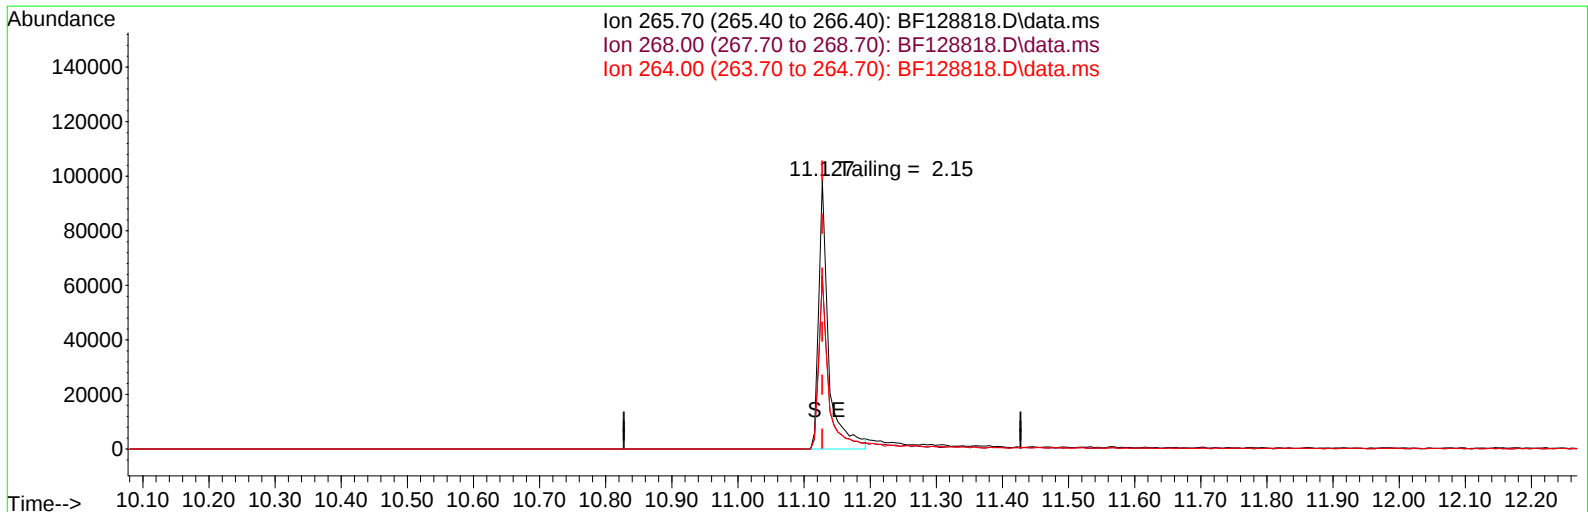

TIC: BF128818.D\data.ms

(70) Pentachlorophenol (C)

11.127min (-0.000) 29908.24 ng




response 114268

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	64.32
264.00	61.80	63.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061522\
 Data File : BF128818.D
 Acq On : 15 Jun 2022 10:24
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jun 15 13:04:08 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 14 14:53:53 2022
 Response via : Initial Calibration

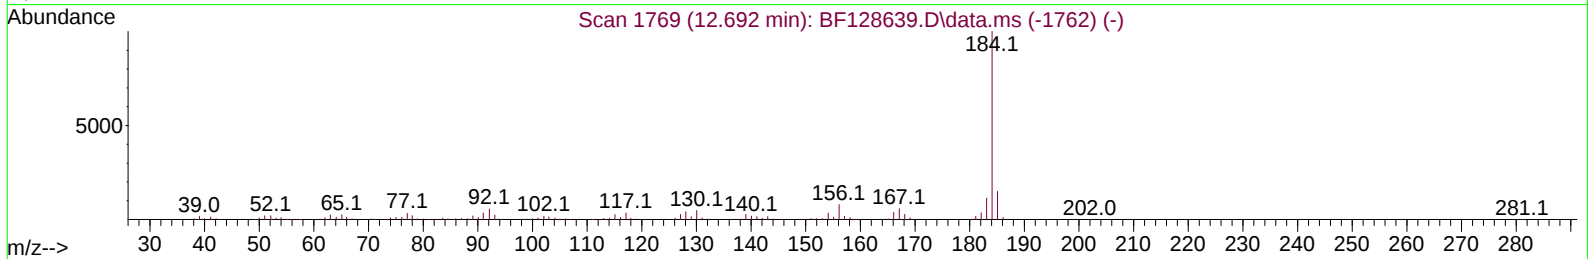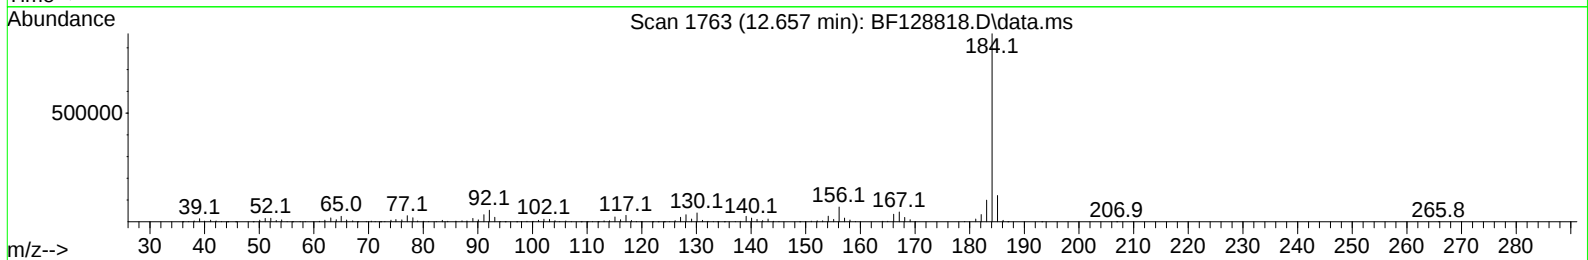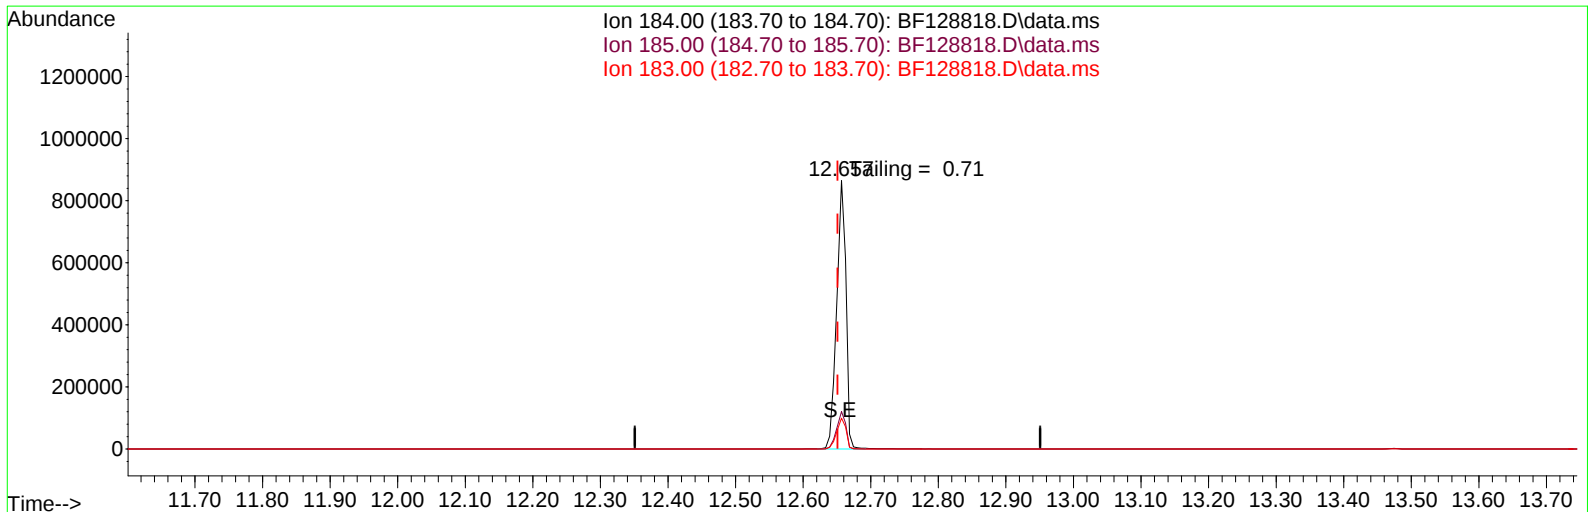

TIC: BF128818.D\data.ms

(77) Benzidine

12.657min (+ 0.006) 720978.41 ng

response 804850

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	13.97
183.00	11.60	11.55
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/15/2022	BNA_F	<u>BF128818.D</u>
Compound Name	Response	Retention Time
DDT	374949	13.47
DDD	2525	13.17
DDE	1143	12.84
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3668	378617	0.97

Instrument :
BNA_F
ClientSampleId :
DFTPP