
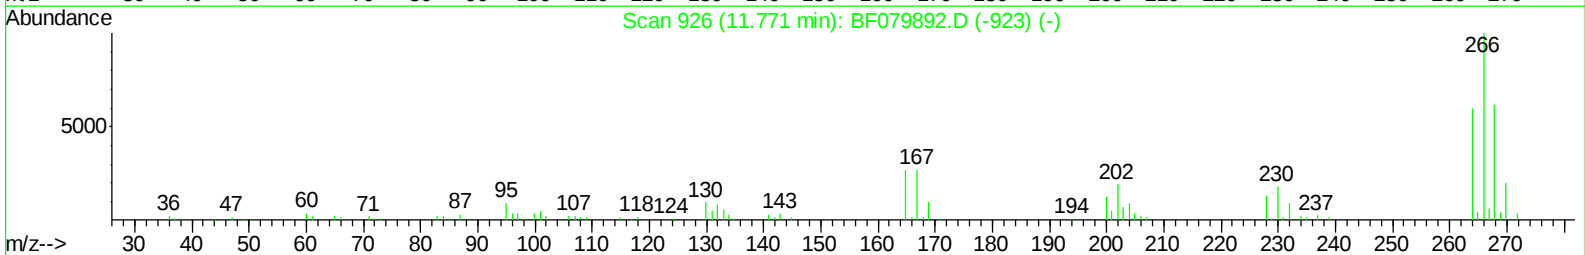
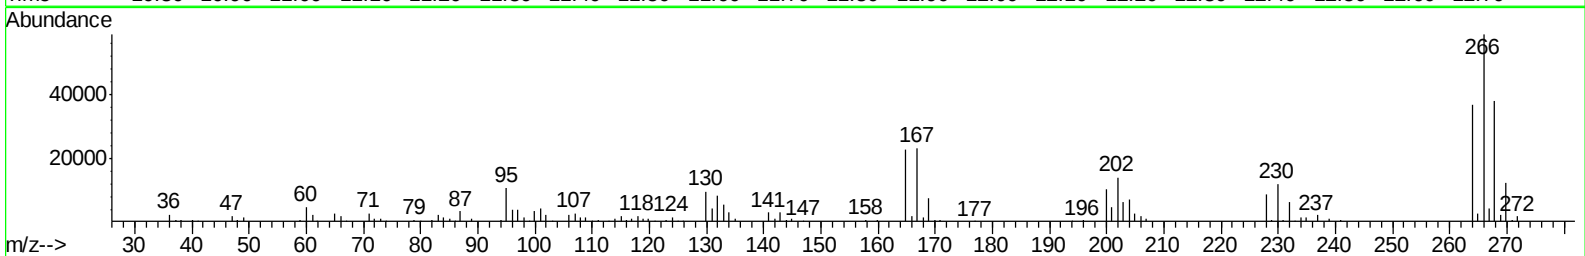


Data Path : Z:\HPCHEM1\BNA_F\Data\BF061615\
Data File : BF079988.D
Acq On : 16 Jun 2015 13:45
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 17 09:09:25 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 15 15:44:31 2015
Response via : Initial Calibration

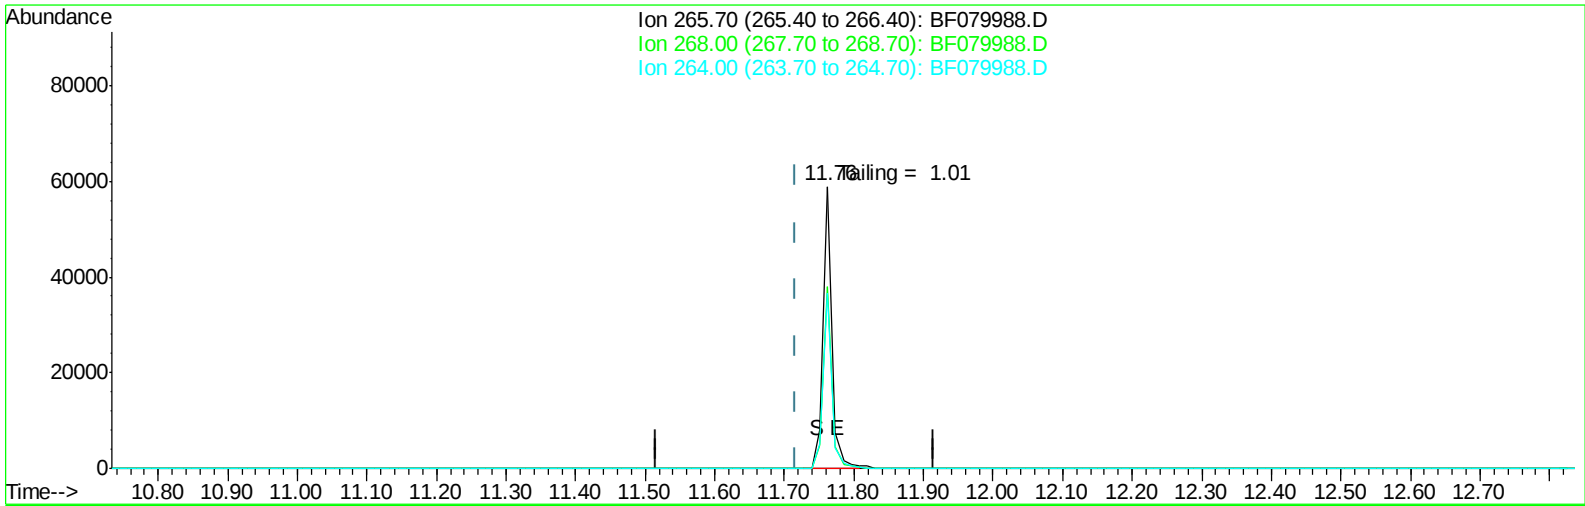

TIC: BF079988.D

(69) Pentachlorophenol (C)




11.762min (+0.046) 0.00ng

response 53370

Ion	Exp%	Act%
265.70	100	100
268.00	61.80	64.75
264.00	59.60	62.44
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF061615\
Data File : BF079988.D
Acq On : 16 Jun 2015 13:45
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 17 09:09:25 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 15 15:44:31 2015
Response via : Initial Calibration

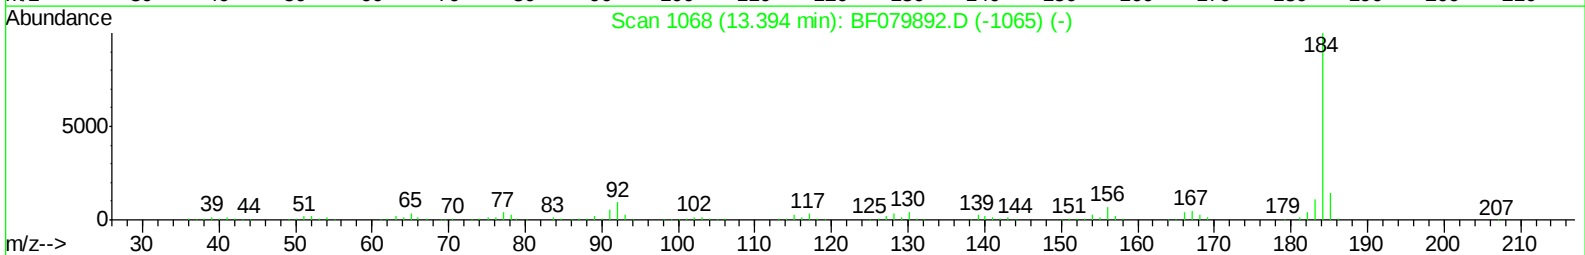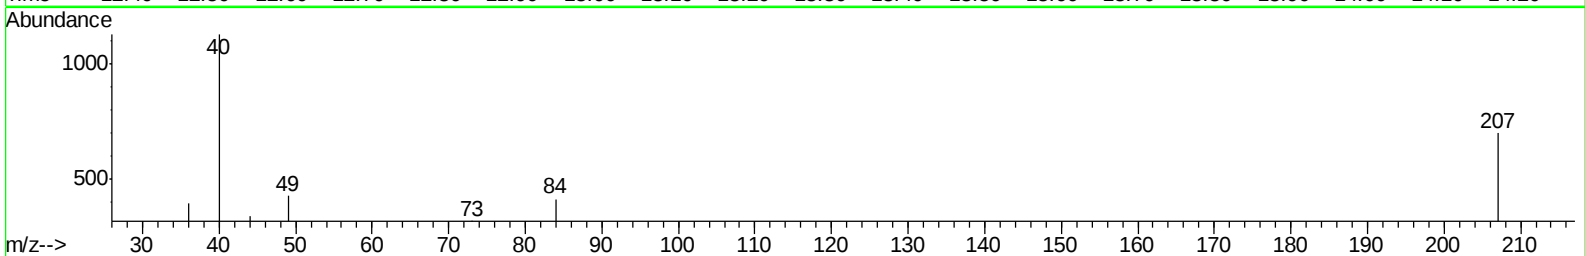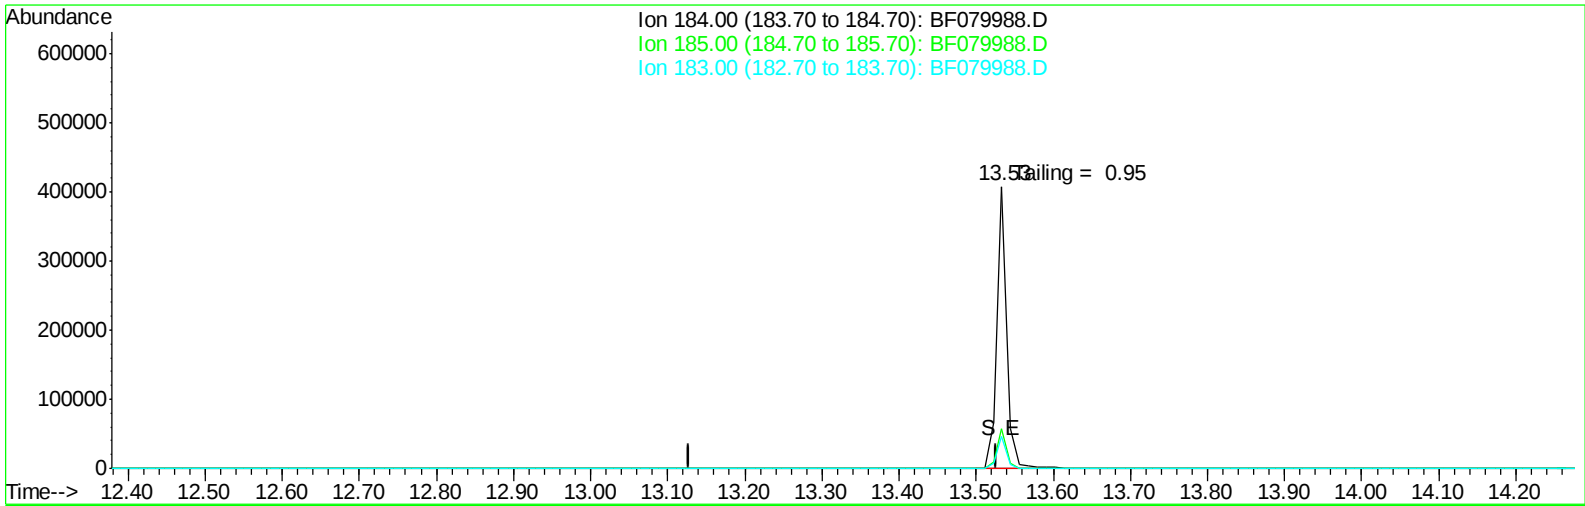

TIC: BF079988.D

(76) Benzidine

13.328min (-13.328) 0.00ng

response 0

Ion	Exp%	Act%
184.00	100	0.00
185.00	14.70	0.00#
183.00	11.30	0.00#
0.00	0.00	0.00