
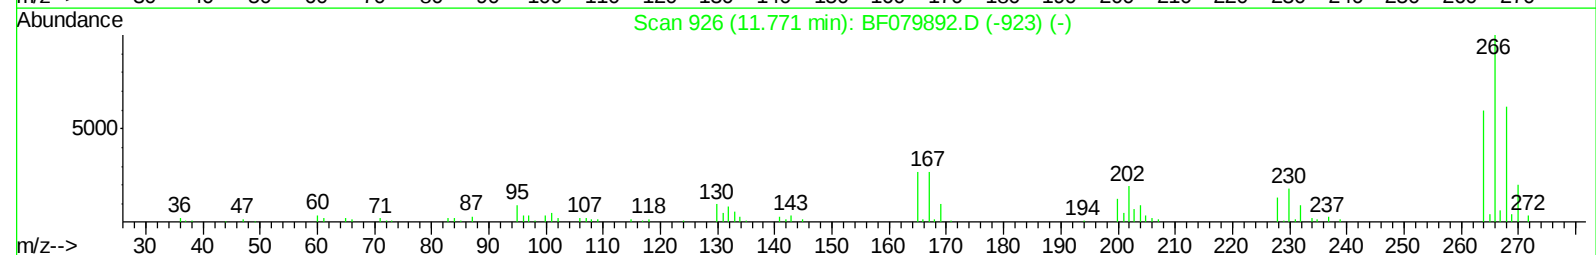
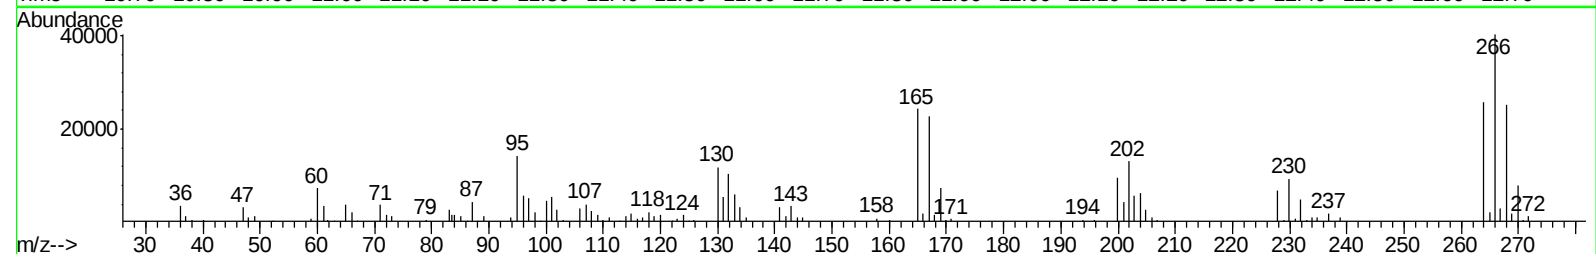


```
Data Path : Z:\HPCHEM1\BNA_F\Data\BF061615\  
Data File : BF080002.D  
Acq On    : 16 Jun 2015   23:12  
Operator  : TP/IZ  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Quant Time: Jun 17 09:12:07 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 15 15:44:31 2015
Response via : Initial Calibration

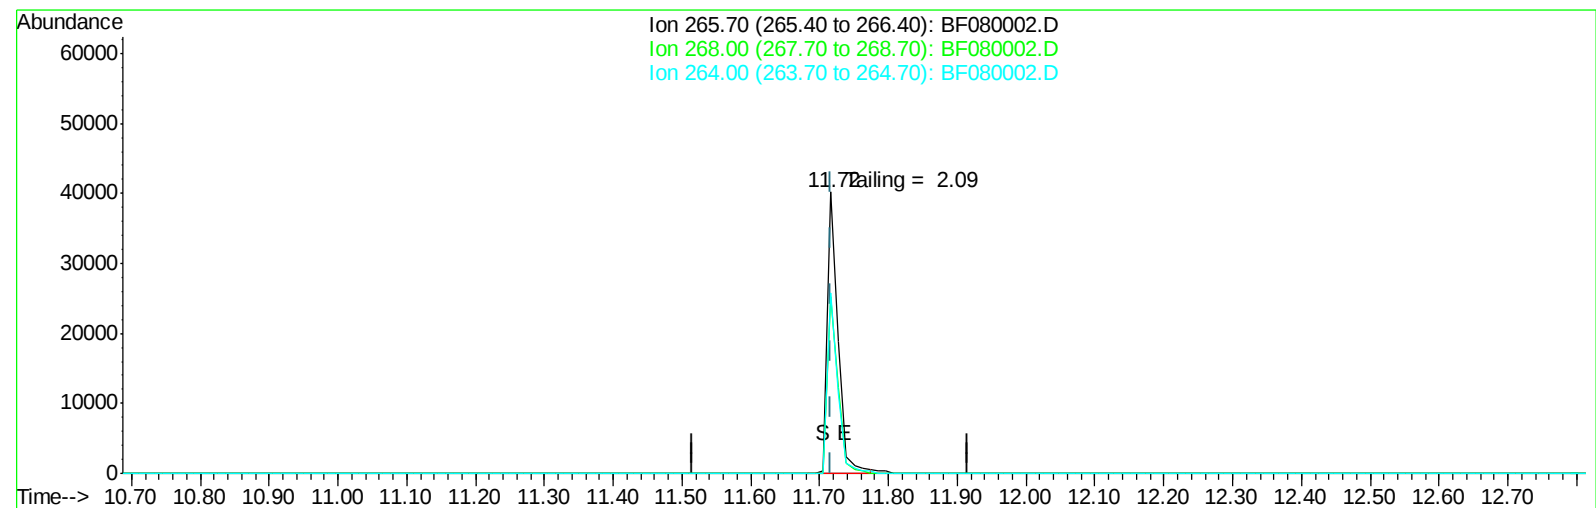

TIC: BF080002.D

(69) Pentachlorophenol (C)




11.716min (-0.000) 0.00ng

response 44484

Ion	Exp%	Act%
265.70	100	100
268.00	61.80	62.96
264.00	59.60	64.19
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF061615\
Data File : BF080002.D
Acq On : 16 Jun 2015 23:12
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 17 09:12:07 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 15 15:44:31 2015
Response via : Initial Calibration

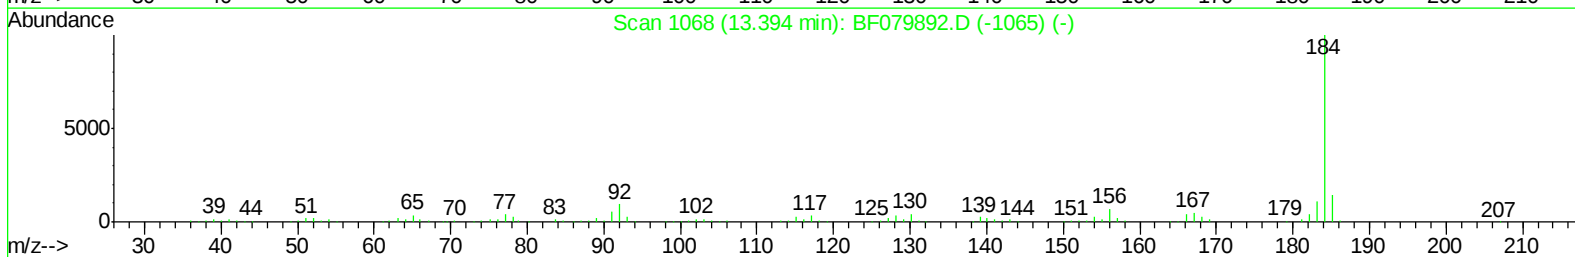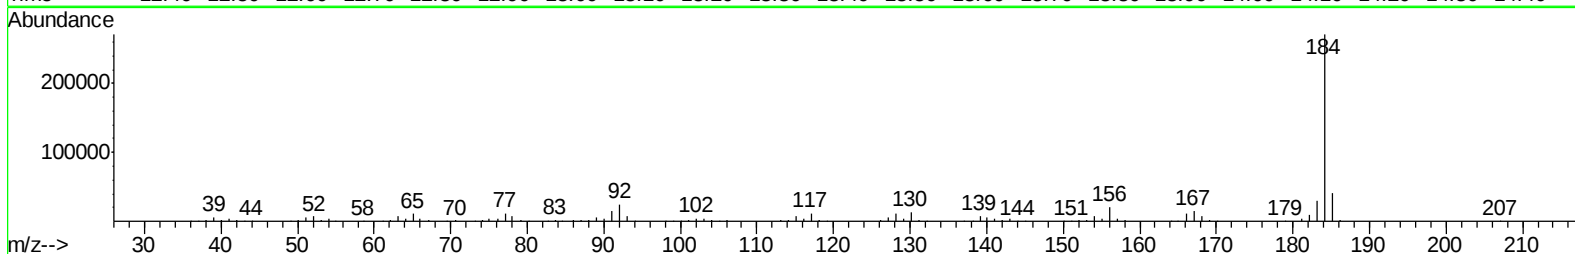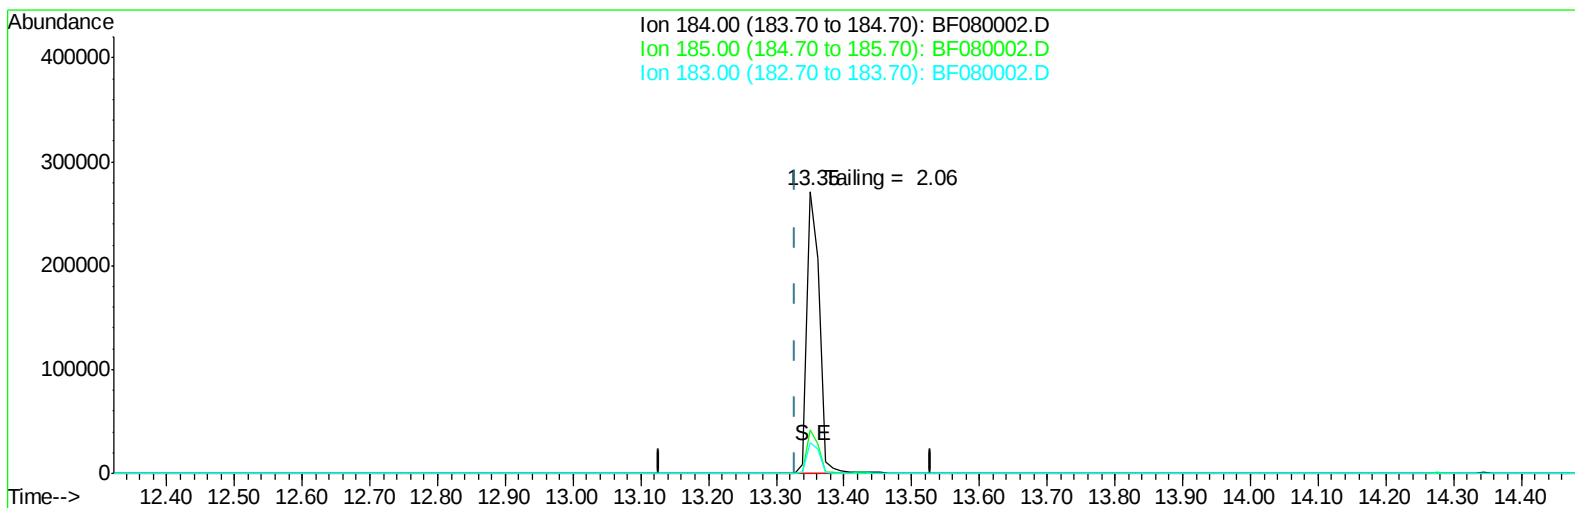

TIC: BF080002.D

(76) Benzidine

13.351min (+0.023) 0.00ng

response 351776

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	15.32
183.00	11.30	11.10
0.00	0.00	0.00