

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061615\
 Data File : BF080009.D
 Acq On : 17 Jun 2015 3:04
 Operator : TP/IZ
 Sample : G2474-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 C-3

Quant Time: Jun 17 05:40:05 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 15 15:44:31 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.35	152	48071	20.00	ng	0.00
21) Naphthalene-d8	8.64	136	200079	20.00	ng	0.00
38) Acenaphthene-d10	10.41	164	100354	20.00	ng	0.00
63) Phenanthrene-d10	11.92	188	206426	20.00	ng	0.00
75) Chrysene-d12	14.86	240	218940	20.00	ng	-0.05
86) Perylene-d12	16.73	264	205508	20.00	ng	-0.07
System Monitoring Compounds						
5) 2-Fluorophenol	5.96	112	88143	33.62	ng	0.00
7) Phenol-d6	6.95	99	81235	22.74	ng	0.00
23) Nitrobenzene-d5	7.91	82	205655	67.82	ng	0.00
41) 2,4,6-Tribromophenol	11.21	330	58089	59.13	ng	0.00
44) 2-Fluorobiphenyl	9.72	172	471528	65.79	ng	0.00
78) Terphenyl-d14	13.60	244	585896	61.70	ng	-0.02
Target Compounds						
49) Dimethylphthalate	10.10	163	37991	4.73	ng	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061615\
Data File : BF080009.D
Acq On : 17 Jun 2015 3:04
Operator : TP/IZ
Sample : G2474-03
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
C-3

Quant Time: Jun 17 05:40:05 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 15 15:44:31 2015
Response via : Initial Calibration

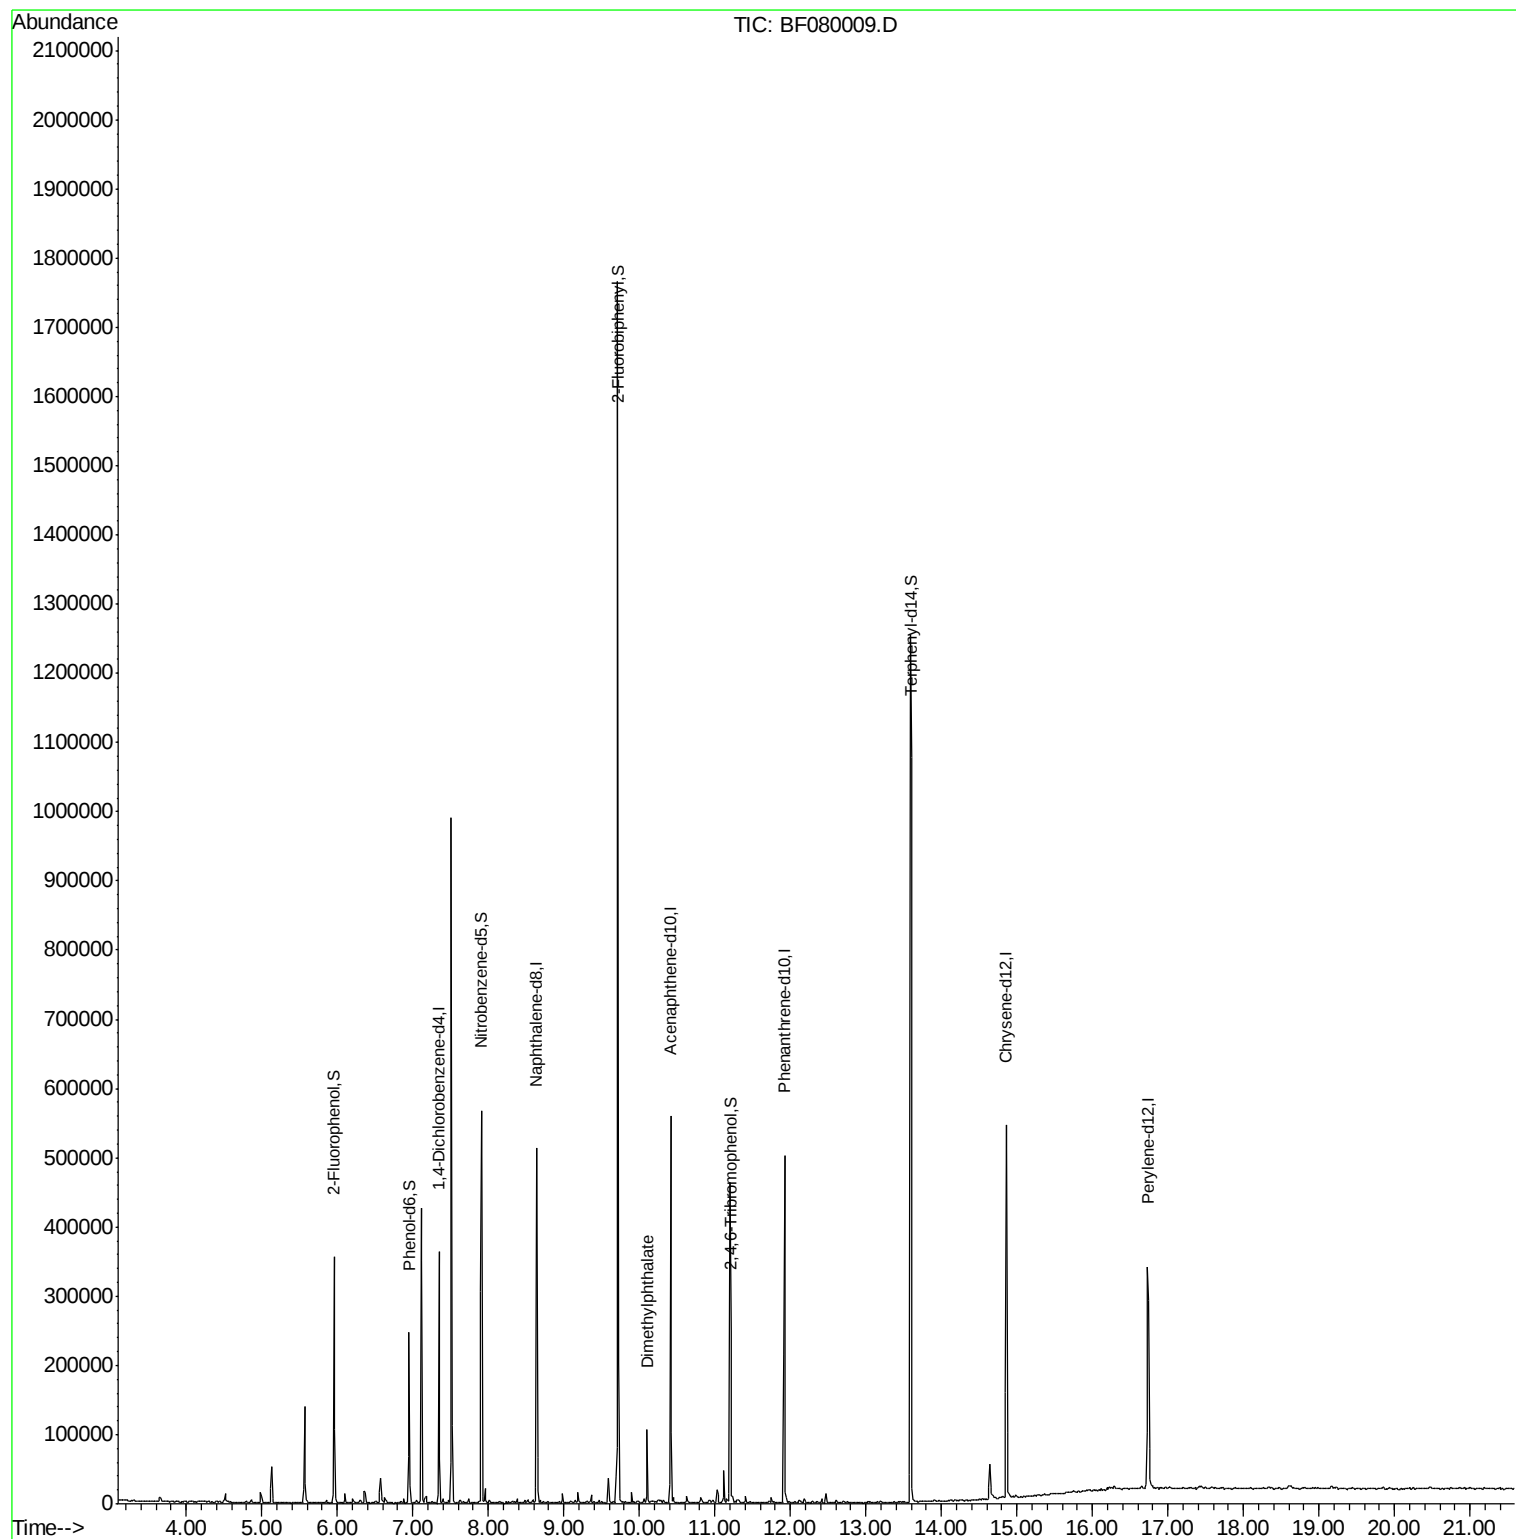

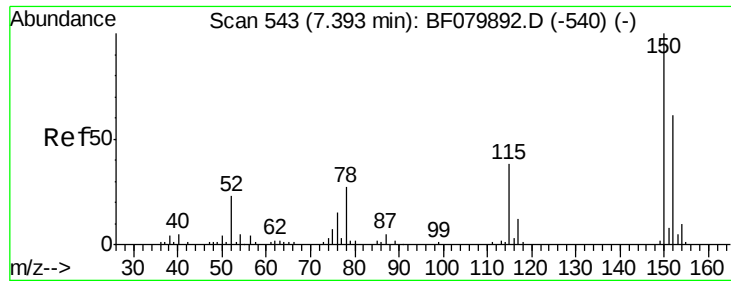


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.35 min Scan# 373
Delta R.T. 0.00 min
Lab File: BF080009.D
Acq: 17 Jun 2015 3:04

Instrument :
BNA_F
ClientSampleId :
C-3

Tgt Ion:152 Resp: 48071
Ion Ratio Lower Upper
152 100
150 160.0 131.0 196.4
115 65.4 49.8 74.6

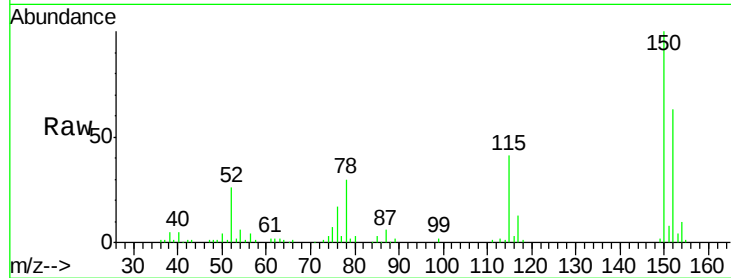


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

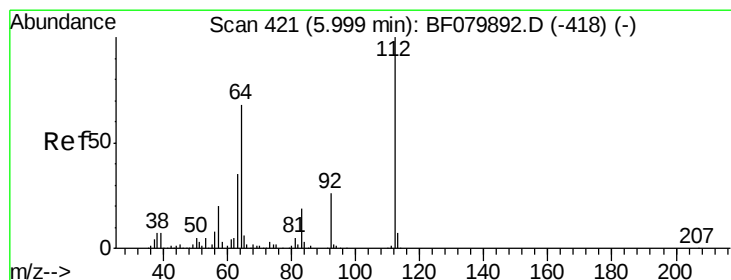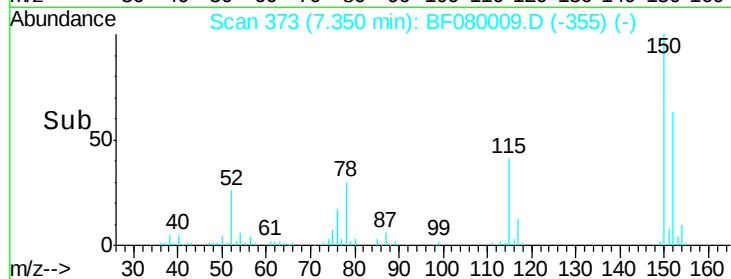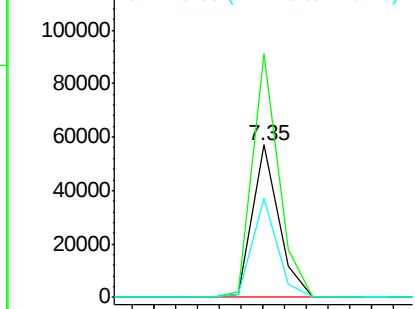



#5


2-Fluorophenol
Concen: 33.62 ng
RT: 5.96 min Scan# 251
Delta R.T. 0.00 min
Lab File: BF080009.D
Acq: 17 Jun 2015 3:04

Tgt Ion:112 Resp: 88143
Ion Ratio Lower Upper
112 100
64 67.7 54.5 81.7
63 34.6 27.9 41.9

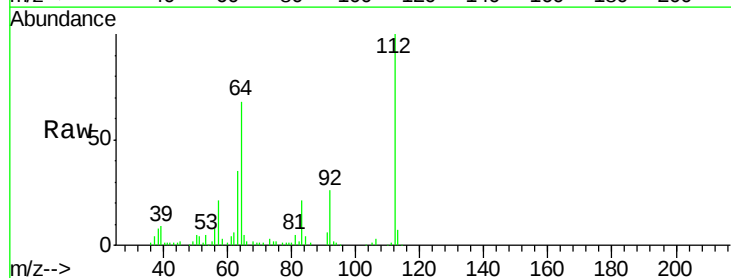

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

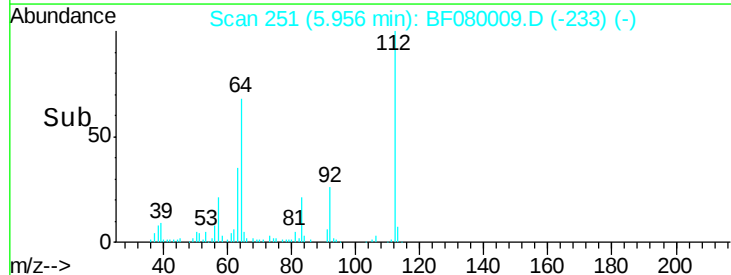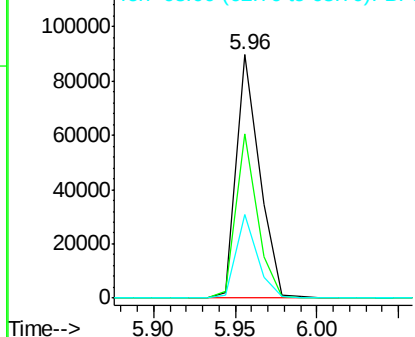

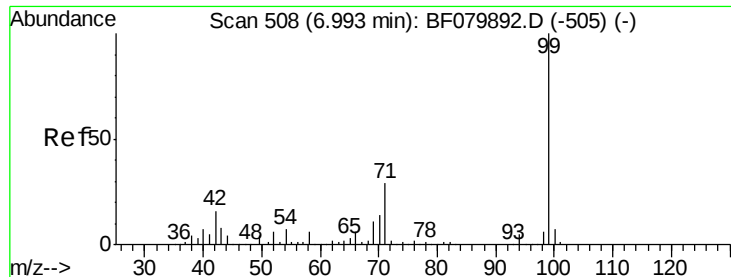

#7

Phenol-d6

Concen: 22.74 ng

RT: 6.95 min Scan# 338

Delta R.T. 0.00 min

Lab File: BF080009.D

Acq: 17 Jun 2015 3:04

Instrument :

BNA_F

ClientSampleId :

C-3


Tgt Ion: 99 Resp: 81235

Ion Ratio Lower Upper




99 100

42 17.2 12.9 19.3

71 29.6 23.4 35.2

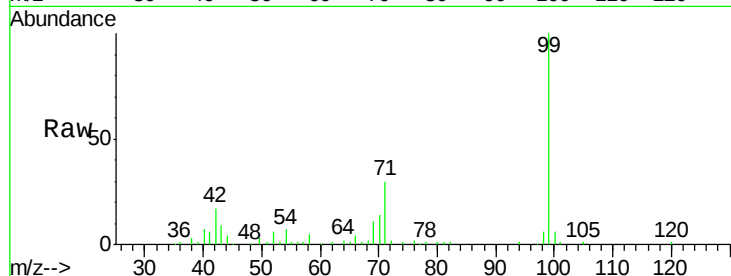

Abundance Ion 99.00 (98.70 to 99.70): BF0
Ion 42.00 (41.70 to 42.70): BF0
Ion 71.00 (70.70 to 71.70): BF0

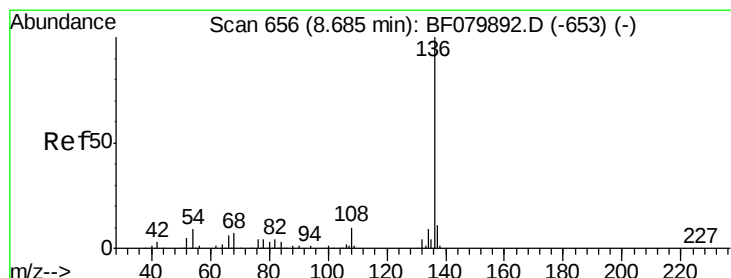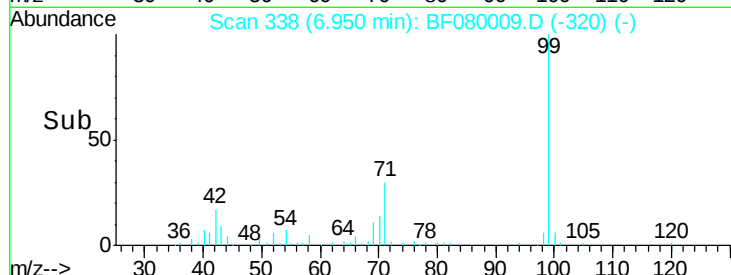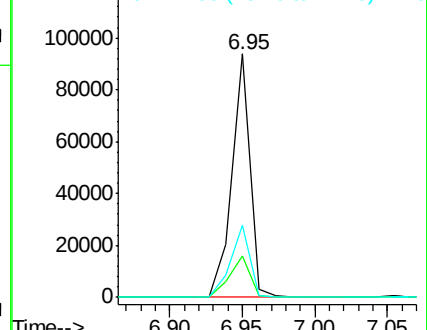

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.64 min Scan# 486

Delta R.T. 0.00 min

Lab File: BF080009.D

Acq: 17 Jun 2015 3:04

Tgt Ion: 136 Resp: 200079


Ion Ratio Lower Upper

136 100



137 10.6 8.7 13.1


54 8.4 7.3 10.9

68 6.3 5.9 8.9

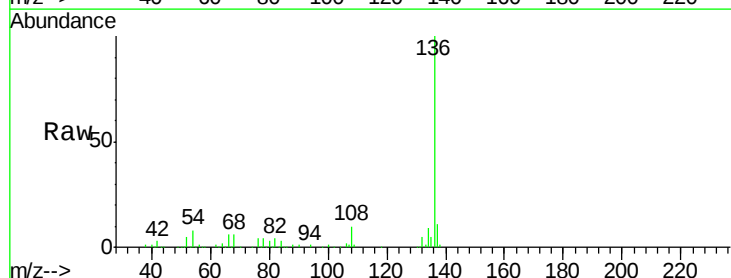

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

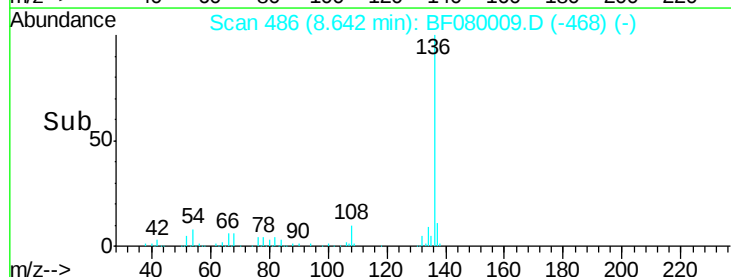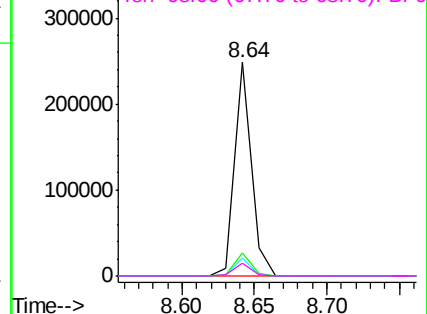

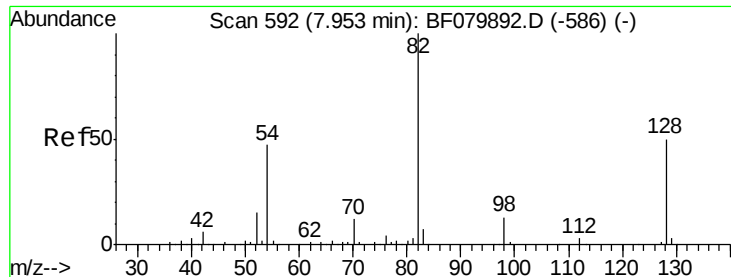

#23

Nitrobenzene-d5

Concen: 67.82 ng

RT: 7.91 min Scan# 422

Delta R.T. 0.00 min

Lab File: BF080009.D

Acq: 17 Jun 2015 3:04

Instrument :

BNA_F

ClientSampled :

C-3


Tgt Ion: 82 Resp: 205655

Ion Ratio Lower Upper




82 100

128 49.4 40.3 60.5

54 46.9 38.0 57.0

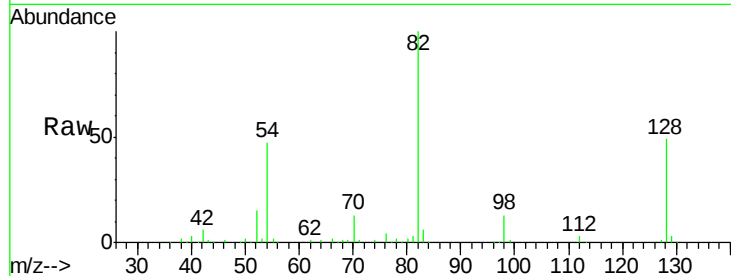

Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): B
Ion 54.00 (53.70 to 54.70): BF0

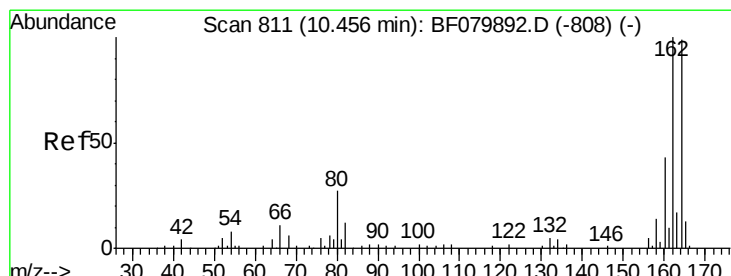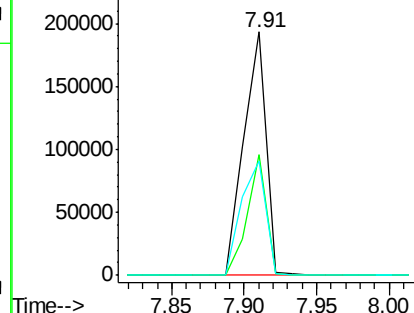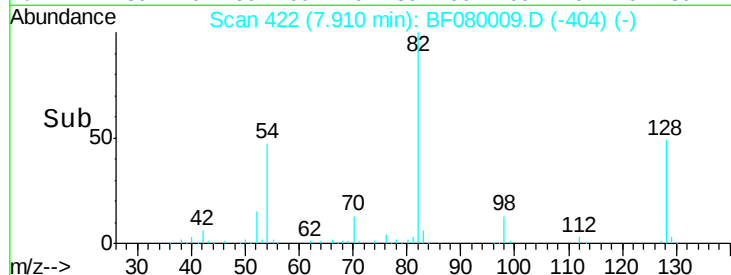

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 10.41 min Scan# 641

Delta R.T. 0.00 min

Lab File: BF080009.D

Acq: 17 Jun 2015 3:04


Tgt Ion: 164 Resp: 100354

Ion Ratio Lower Upper



164 100


162 105.3 80.7 121.1

160 45.4 34.6 51.8

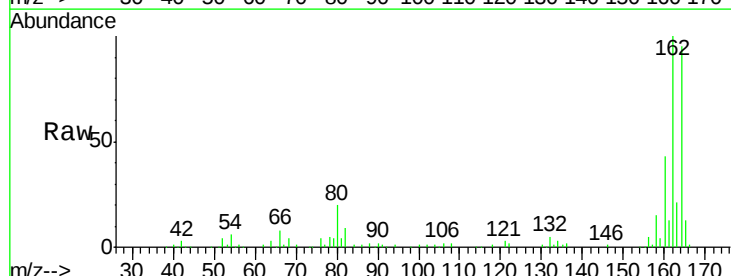

Abundance Ion 164.00 (163.70 to 164.70): B
Ion 162.00 (161.70 to 162.70): B
Ion 160.00 (159.70 to 160.70): B

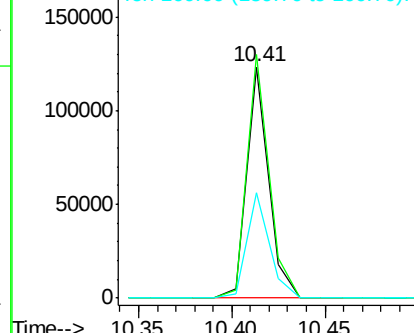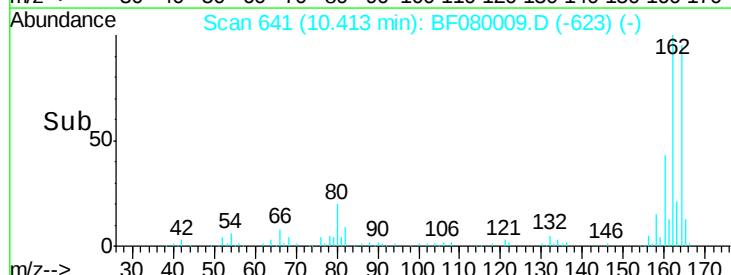


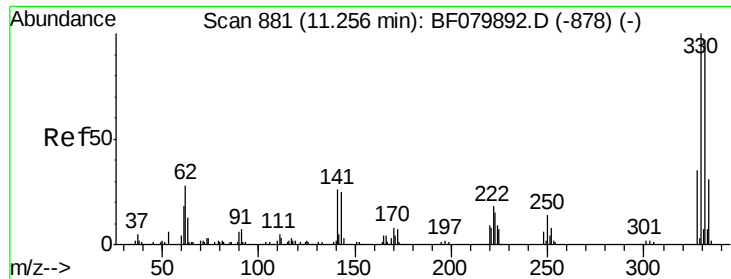




#41
 2,4,6-Tribromophenol
 Concen: 59.13 ng
 RT: 11.21 min Scan# 711
 Delta R.T. 0.00 min
 Lab File: BF080009.D
 Acq: 17 Jun 2015 3:04

Instrument :
 BNA_F
 ClientSampleId :
 C-3

Tgt Ion:330 Resp: 58089
 Ion Ratio Lower Upper
 330 100
 332 95.9 77.3 115.9
 141 39.5 26.8 40.2

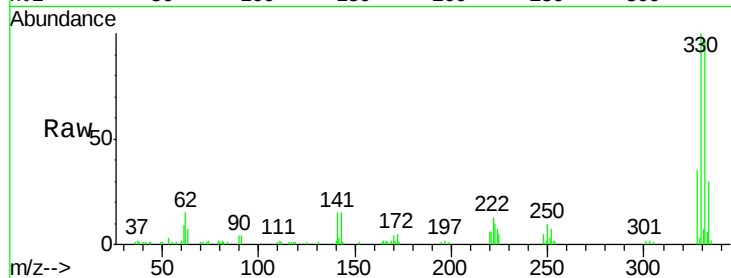


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

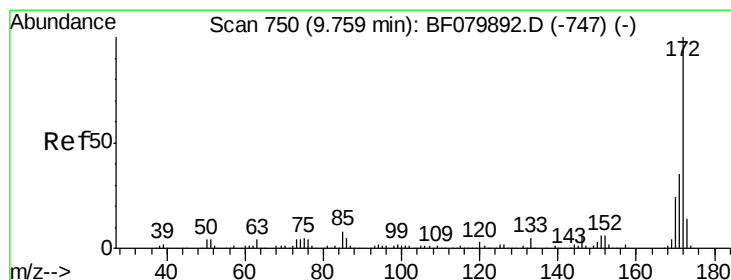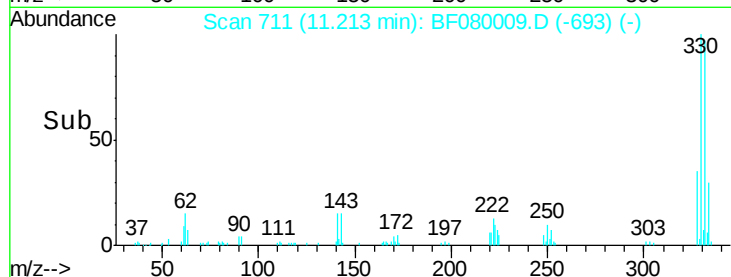
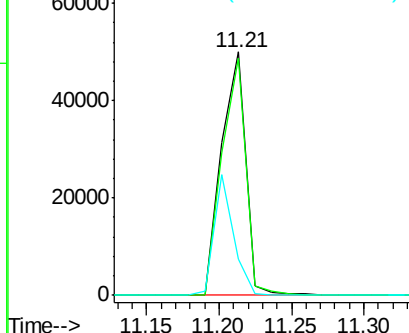



#44
 2-Fluorobiphenyl
 Concen: 65.79 ng
 RT: 9.72 min Scan# 580
 Delta R.T. 0.00 min
 Lab File: BF080009.D
 Acq: 17 Jun 2015 3:04

Tgt Ion:172 Resp: 471528
 Ion Ratio Lower Upper
 172 100
 171 35.2 28.3 42.5
 170 23.7 19.0 28.4

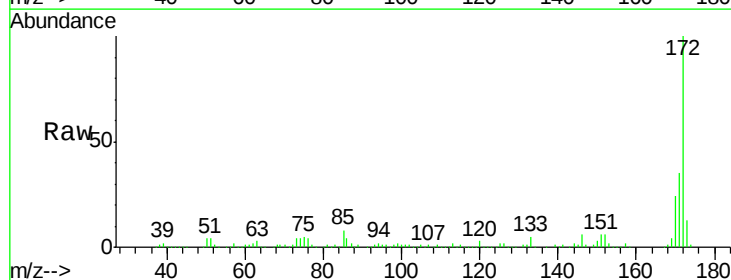

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

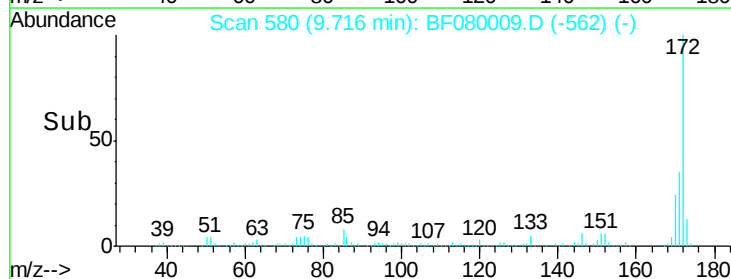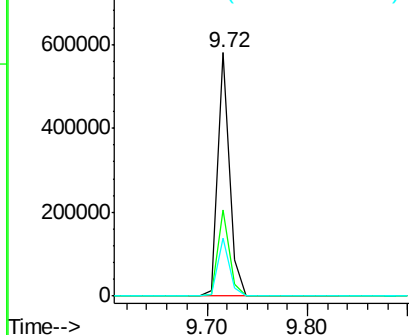

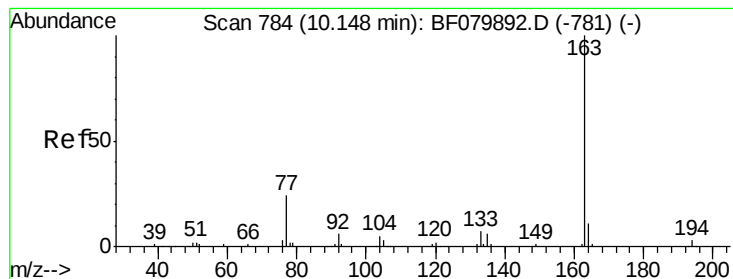

#49

Dimethylphthalate

Concen: 4.73 ng

RT: 10.10 min Scan# 614

Delta R.T. 0.00 min

Lab File: BF080009.D

Acq: 17 Jun 2015 3:04

Instrument :

BNA_F

ClientSampleId :

C-3


Tgt Ion:163 Resp: 37991

Ion Ratio Lower Upper

163 100

194 3.3 2.6 4.0




164 9.5 8.6 12.8

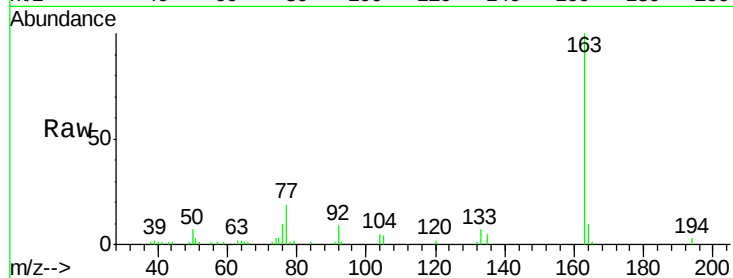

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

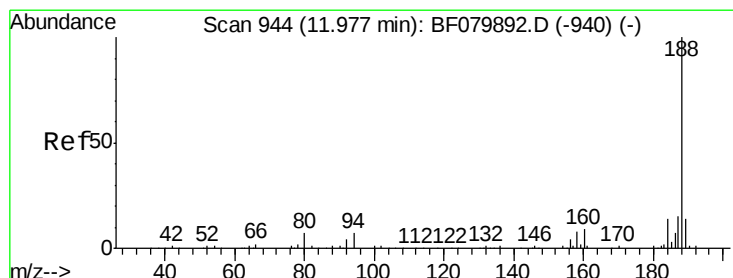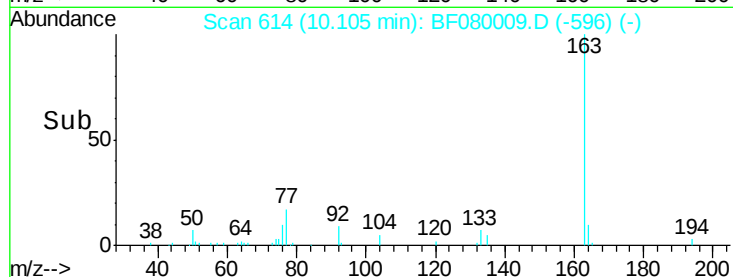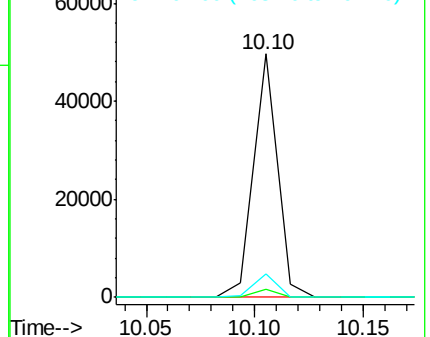

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.92 min Scan# 773

Delta R.T. 0.00 min

Lab File: BF080009.D

Acq: 17 Jun 2015 3:04


Tgt Ion:188 Resp: 206426

Ion Ratio Lower Upper

188 100

94 6.7 5.8 8.8



80 7.0 5.9 8.9

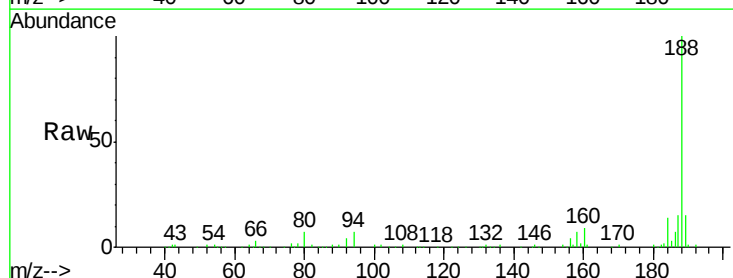


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

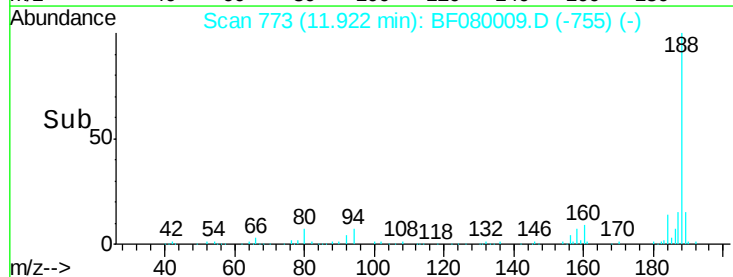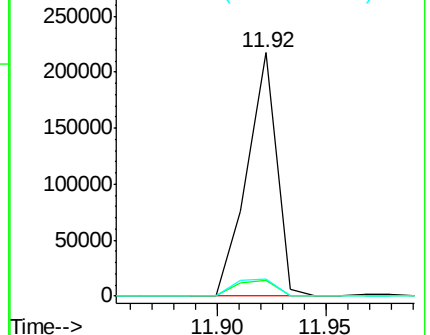

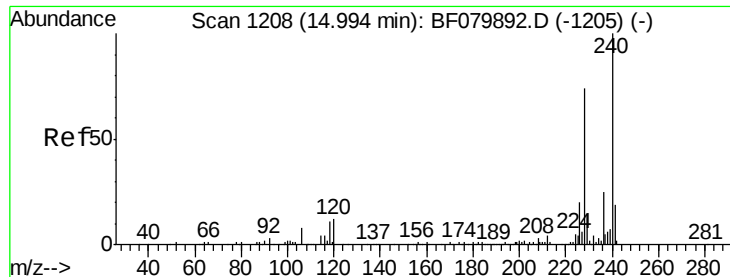

#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.86 min Scan# 1030

Delta R.T. -0.05 min

Lab File: BF080009.D

Acq: 17 Jun 2015 3:04

Instrument :

BNA_F

ClientSampleId :

C-3


Tgt Ion:240 Resp: 218940

Ion Ratio Lower Upper

240 100

120 9.4 9.4 14.2#




236 25.4 19.6 29.4

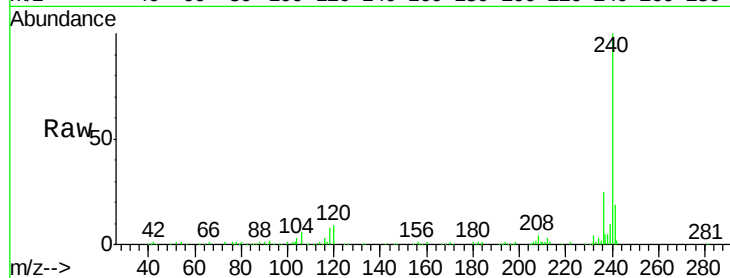

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

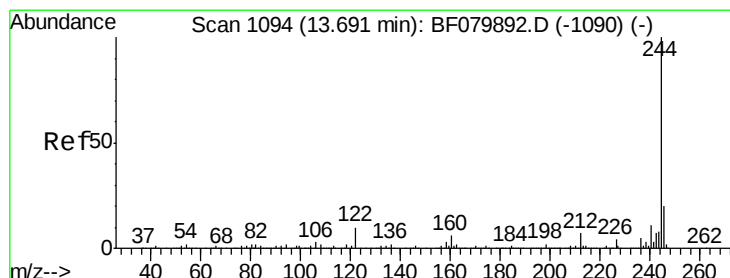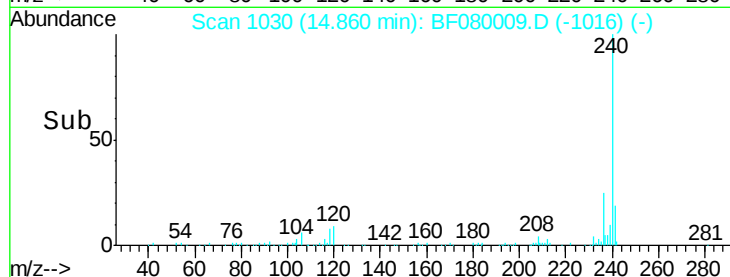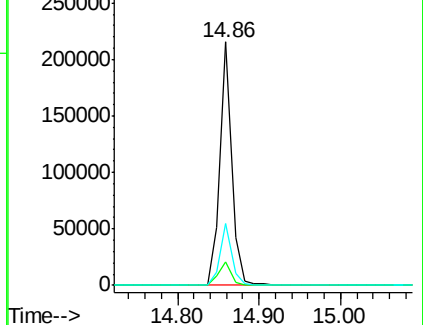

#78

Terphenyl-d14

Concen: 61.70 ng

RT: 13.60 min Scan# 920

Delta R.T. -0.02 min

Lab File: BF080009.D

Acq: 17 Jun 2015 3:04


Tgt Ion:244 Resp: 585896

Ion Ratio Lower Upper

244 100

212 6.3 5.4 8.2



122 5.7 7.8 11.8#

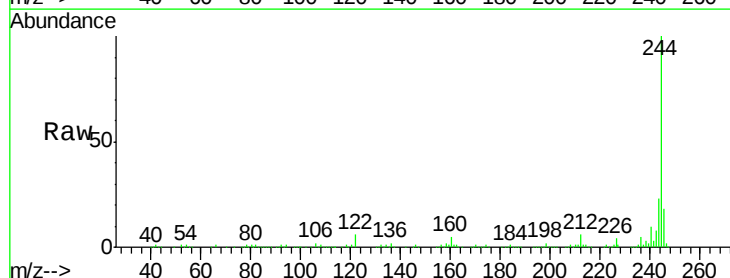


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

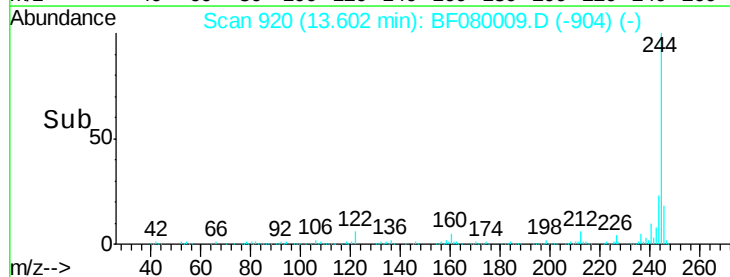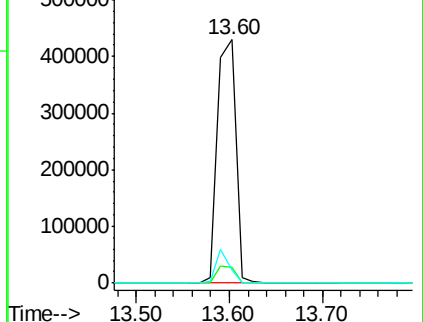


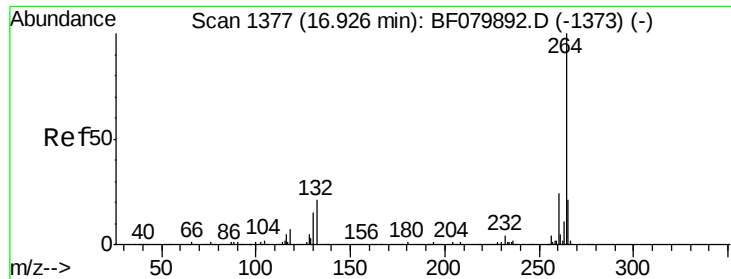

#86
Perylene-d12
Concen: 20.00 ng
RT: 16.73 min Scan# 1194
Delta R.T. -0.07 min
Lab File: BF080009.D
Acq: 17 Jun 2015 3:04

Instrument :
BNA_F
ClientSampleId :
C-3

Tgt Ion: 264 Resp: 205508
Ion Ratio Lower Upper
264 100
260 23.0 19.3 28.9
265 21.3 17.0 25.6

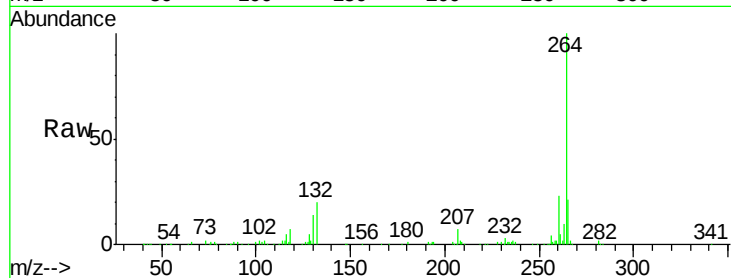

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

