

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061615\
Data File : BF080000.D
Acq On : 16 Jun 2015 19:51
Operator : TP/IZ
Sample : G2647-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SVOC-GPC-BLANK

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061115.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	7.350	371	373	376	rVB	312669	253100	53.63%	10.415%
2	8.642	484	486	489	rBV	420826	337060	71.41%	13.870%
3	10.413	639	641	644	rVB	470104	391470	82.94%	16.109%
4	11.922	771	773	775	rBV	451068	418684	88.71%	17.229%
5	14.151	957	968	973	rBV2	24571	101983	21.61%	4.197%
6	14.837	1026	1028	1031	rBV	386375	471979	100.00%	19.422%
7	16.700	1188	1191	1198	rBV	257643	455851	96.58%	18.758%


Sum of corrected areas: 2430127

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061615\
Data File : BF080000.D
Acq On : 16 Jun 2015 19:51
Operator : TP/IZ
Sample : G2647-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

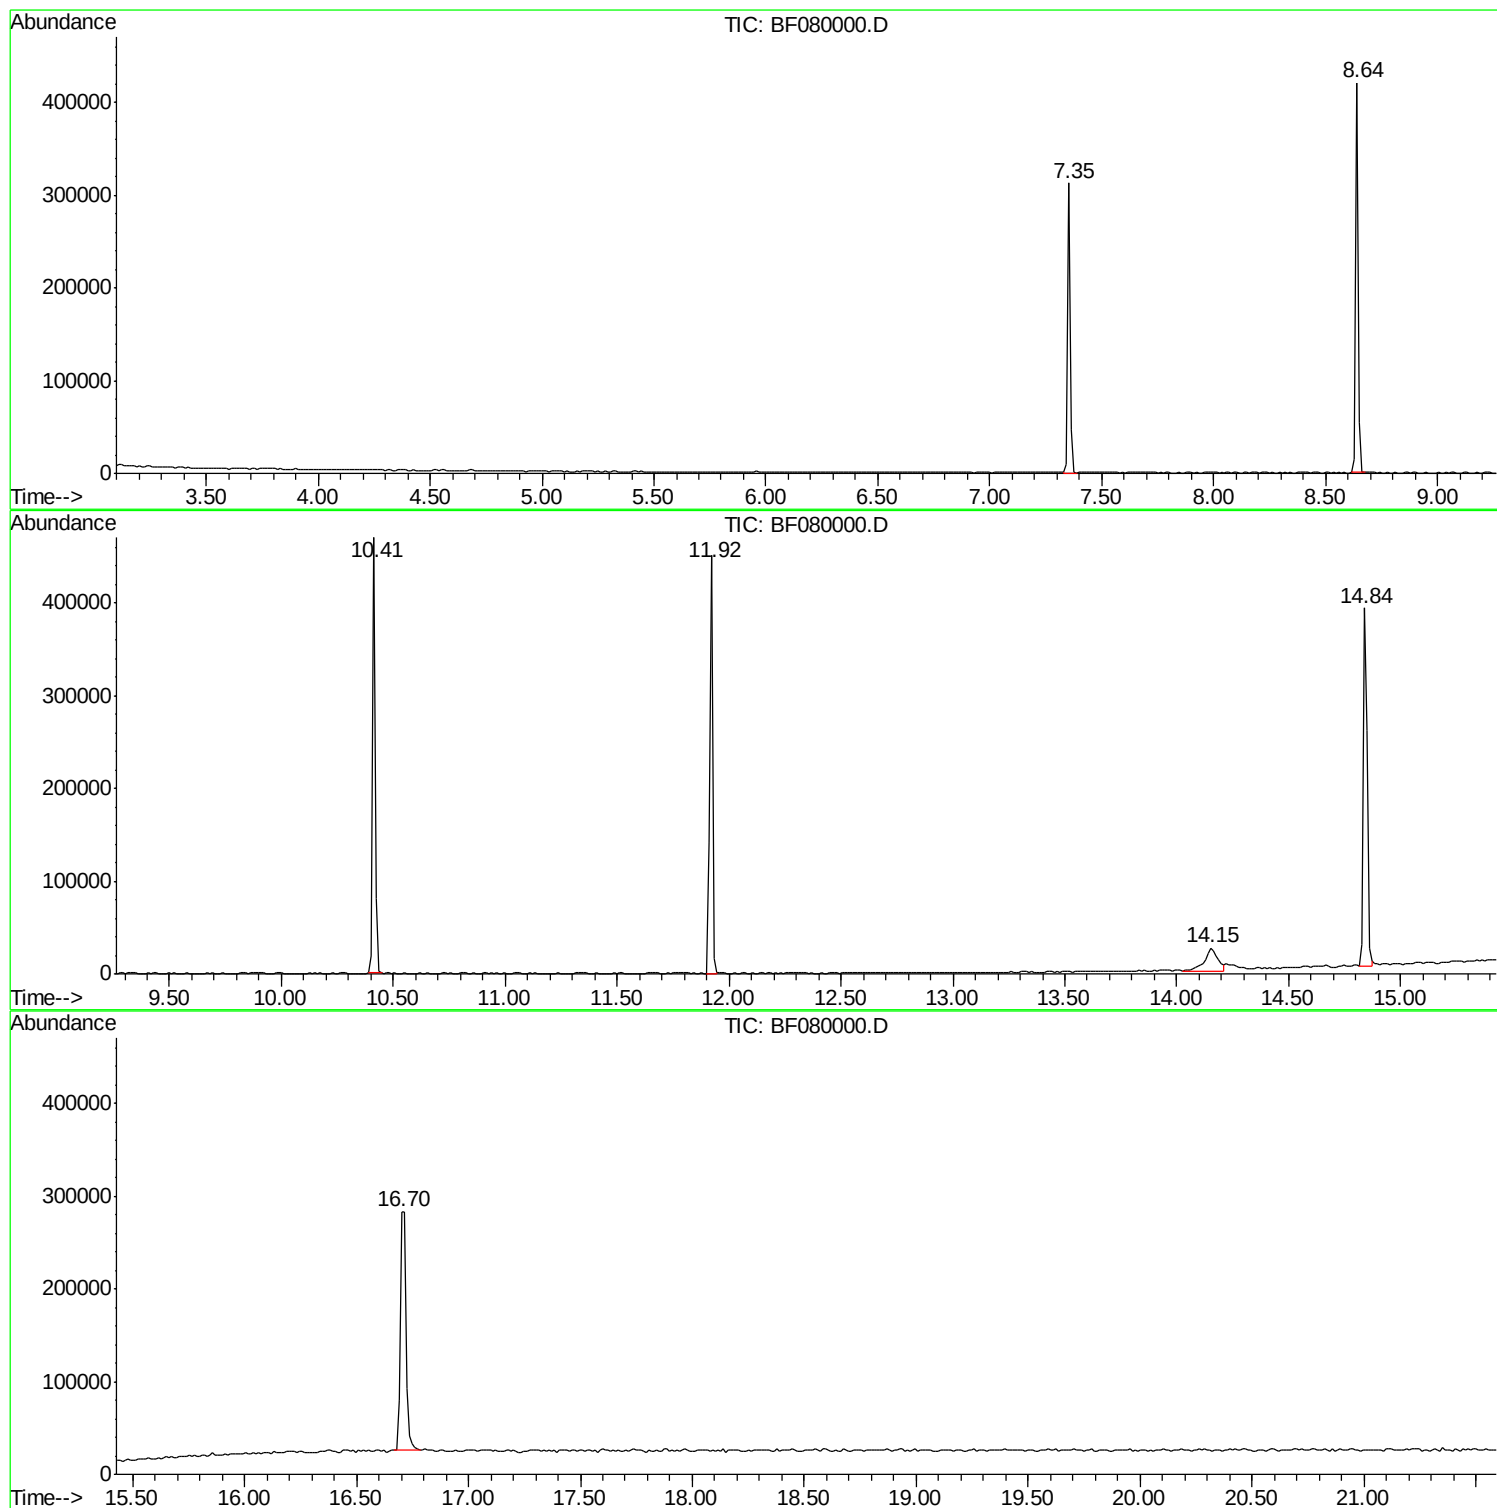

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061615\
Data File : BF080000.D
Acq On : 16 Jun 2015 19:51
Operator : TP/IZ
Sample : G2647-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061615\
Data File : BF080000.D
Acq On : 16 Jun 2015 19:51
Operator : TP/IZ
Sample : G2647-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc