


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061615\
 Data File : BF080002.D
 Acq On : 16 Jun 2015 23:12
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 15 15:44:31 2015

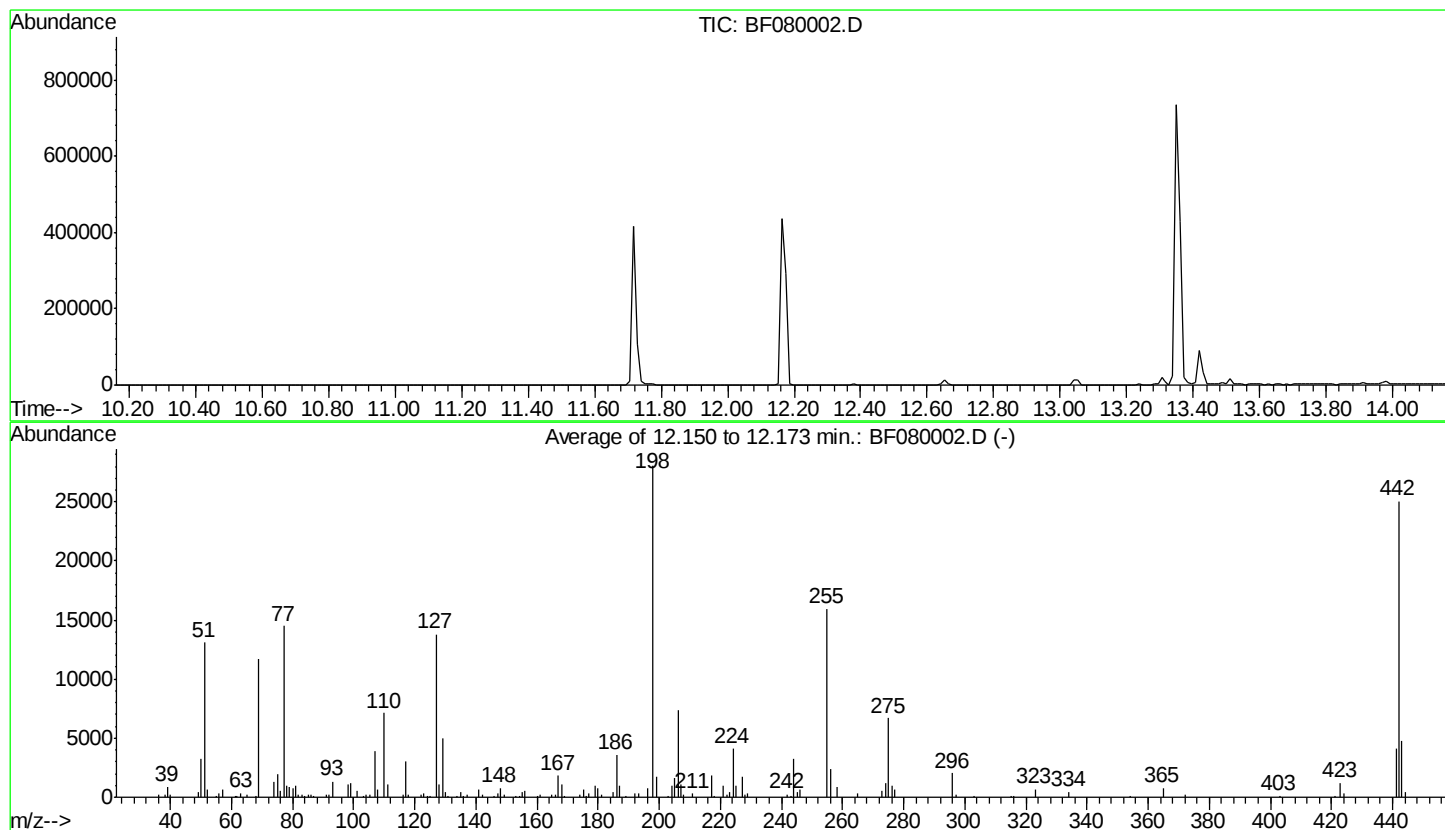

AutoFind: Scans 793, 794, 795; Background Corrected with Scan 791

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.5	13057	PASS
68	69	0.00	2	1.4	159	PASS
69	198	0.00	100	41.7	11710	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.1	13786	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	28058	PASS
199	198	5	9	6.0	1685	PASS
275	198	10	60	23.9	6708	PASS
365	198	1	100	2.9	806	PASS
441	442	0.01	24	16.6	4164	PASS
442	198	50	100	89.4	25075	PASS
443	442	15	24	18.8	4722	PASS