
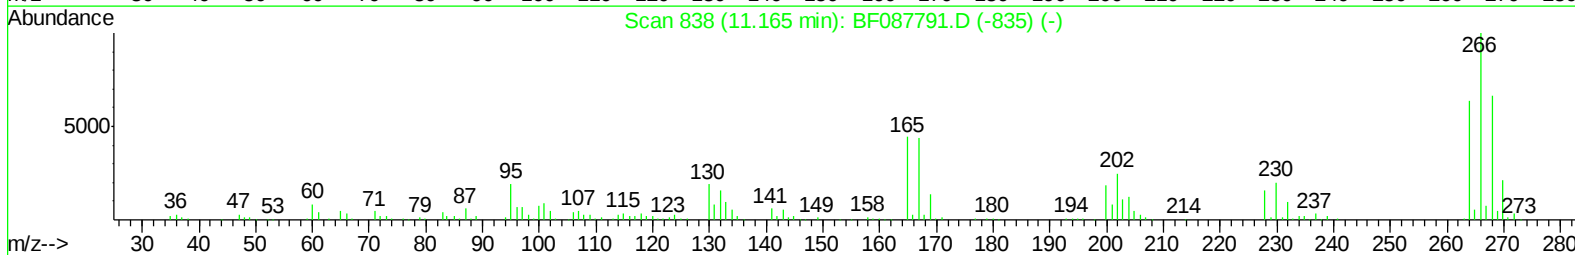
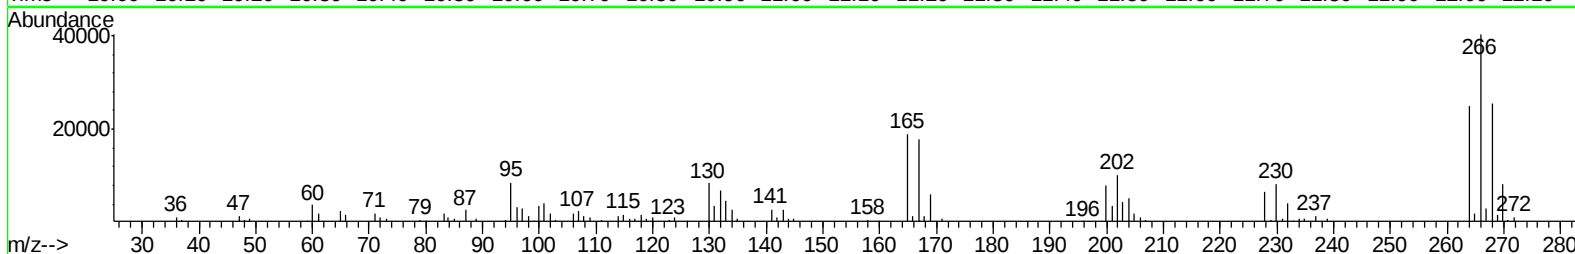


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061616\
Data File : BF088071.D
Acq On : 16 Jun 2016 11:41
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 17 04:42:35 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 16 14:54:54 2016
Response via : Initial Calibration

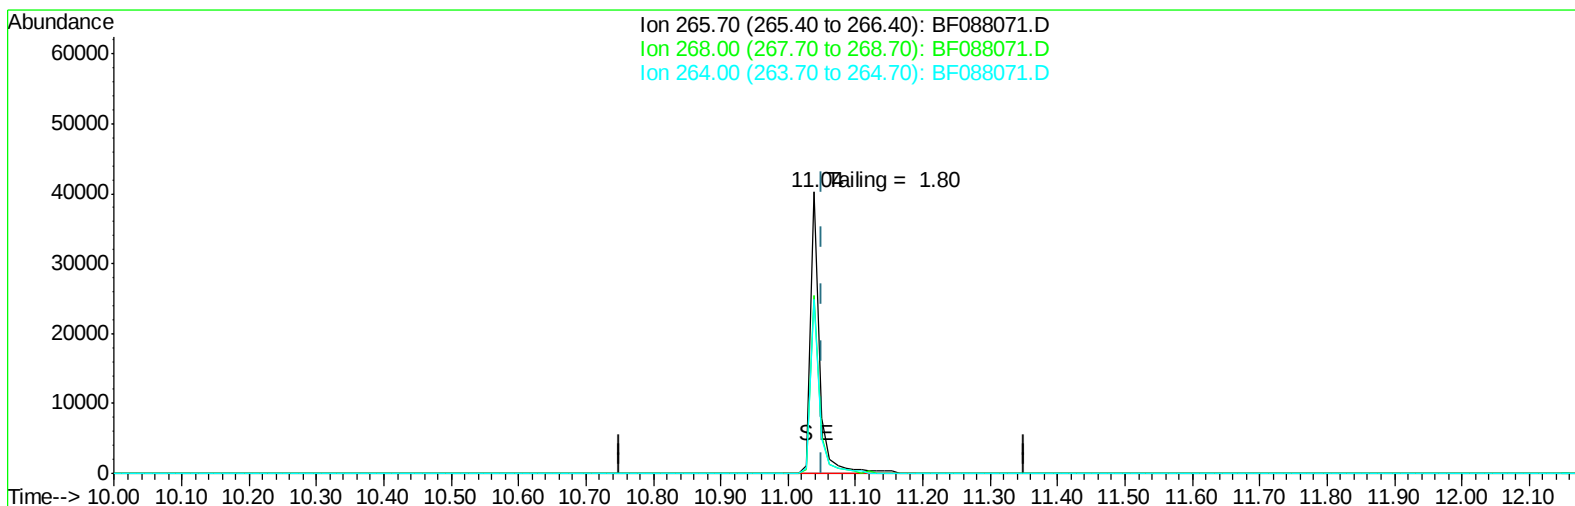

TIC: BF088071.D

(69) Pentachlorophenol (C)




11.039min (-0.011) 7724.31ng

response 38397

Ion	Exp%	Act%
265.70	100	100
268.00	66.00	63.19
264.00	62.00	61.86
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061616\
Data File : BF088071.D
Acq On : 16 Jun 2016 11:41
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 17 04:42:35 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 16 14:54:54 2016
Response via : Initial Calibration

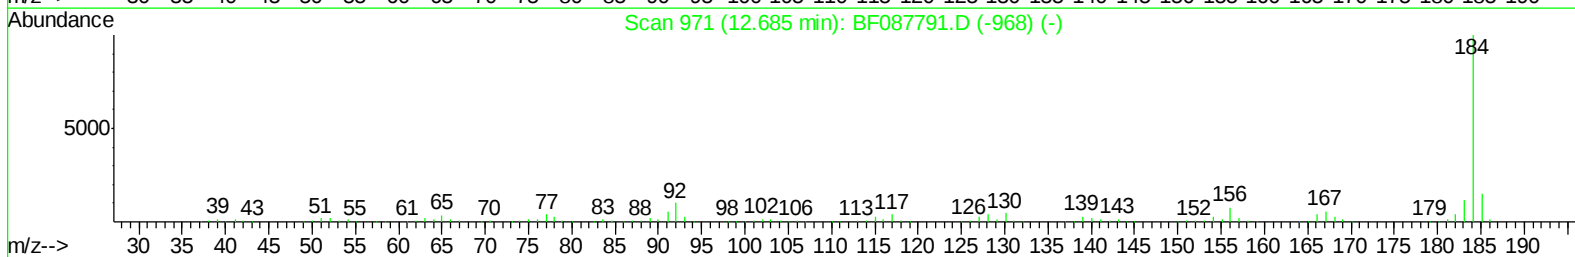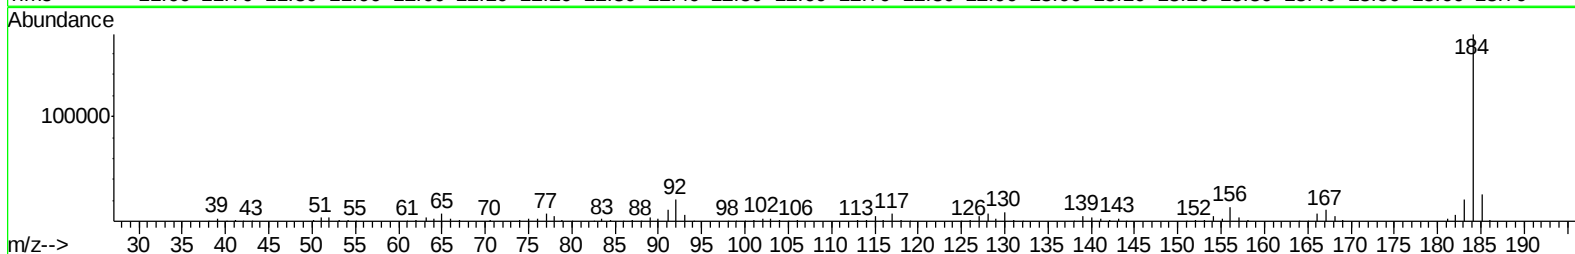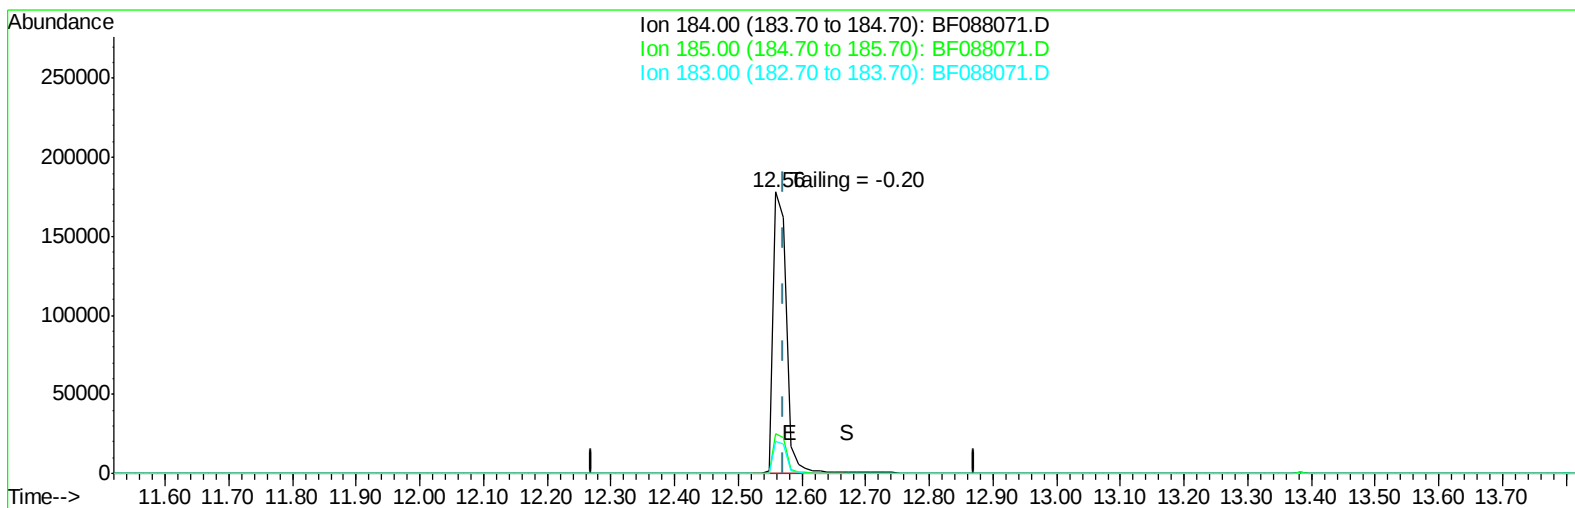

TIC: BF088071.D

(76) Benzidine

12.559min (-0.011) 3063.89ng m

response 256968

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	14.27
183.00	11.60	11.55
0.00	0.00	0.00