


Data Path : Z:\HPCHEM1\BNA F\DATA\BF061616\
Data File : BF088071.D
Acq On : 16 Jun 2016 11:41
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jun 17 16:09:13 2016

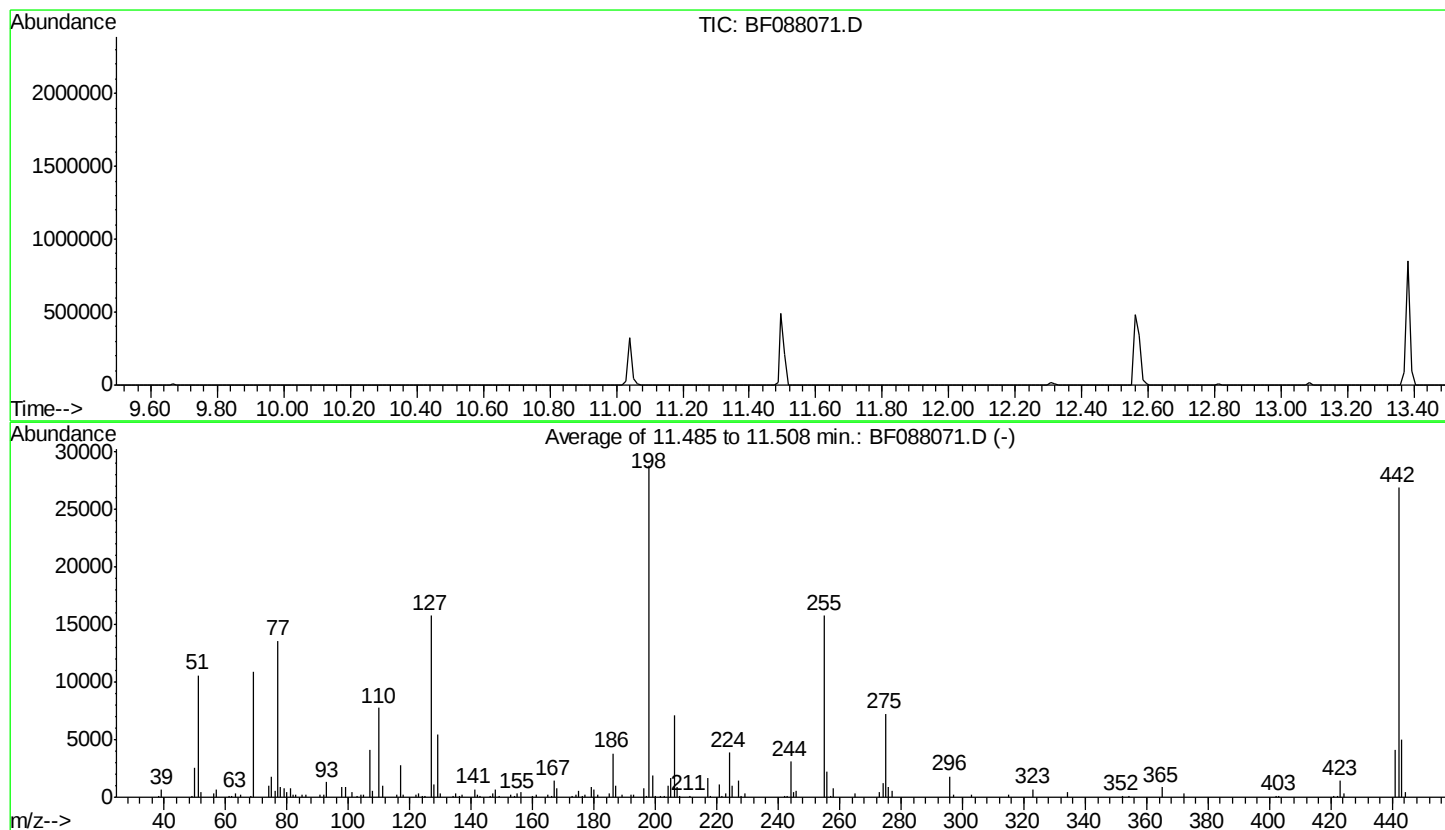

AutoFind: Scans 866, 867, 868; Background Corrected with Scan 863

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.8	10598	PASS
68	69	0.00	2	1.2	131	PASS
69	198	0.00	100	37.9	10897	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.7	15744	PASS
197	198	0.00	2	0.5	131	PASS
198	198	100	100	100.0	28785	PASS
199	198	5	9	6.6	1899	PASS
275	198	10	60	25.2	7253	PASS
365	198	1	100	3.1	887	PASS
441	442	0.01	24	15.2	4081	PASS
442	198	50	100	93.4	26888	PASS
443	442	15	24	18.7	5036	PASS