

Data Path : Z:\HPCHEM1\BNA F\DATA\BF061617\
 Data File : BF095975.D
 Acq On : 17 Jun 2017 2:47
 Operator : SJ/MA
 Sample : PB99832TB
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Jun 17 03:50:58 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 16 17:12:03 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.32	152	68284	20.00	ng	0.00
21) Naphthalene-d8	9.35	136	278382	20.00	ng	0.00
38) Acenaphthene-d10	12.17	164	123244	20.00	ng	-0.01
63) Phenanthrene-d10	14.57	188	195117	20.00	ng	0.00
75) Chrysene-d12	18.29	240	135699	20.00	ng	0.00
86) Perylene-d12	19.96	264	126563	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.22	112	577096	134.67	ng	0.00
7) Phenol-d6	6.89	99	708869	138.18	ng	-0.02
23) Nitrobenzene-d5	8.24	82	399917	89.22	ng	-0.01
41) 2,4,6-Tribromophenol	13.47	330	122983	112.78	ng	-0.01
44) 2-Fluorobiphenyl	11.13	172	794645	89.73	ng	0.00
78) Terphenyl-d14	16.94	244	496667	90.83	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	8.24	70	49873	15.34	ng	# 77
50) 2,6-Dinitrotoluene	12.17	165	15028	7.36	ng	# 31


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF061617\
Data File : BF095975.D
Acq On : 17 Jun 2017 2:47
Operator : SJ/MA
Sample : PB99832TB
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Jun 17 03:50:58 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 16 17:12:03 2017
Response via : Initial Calibration

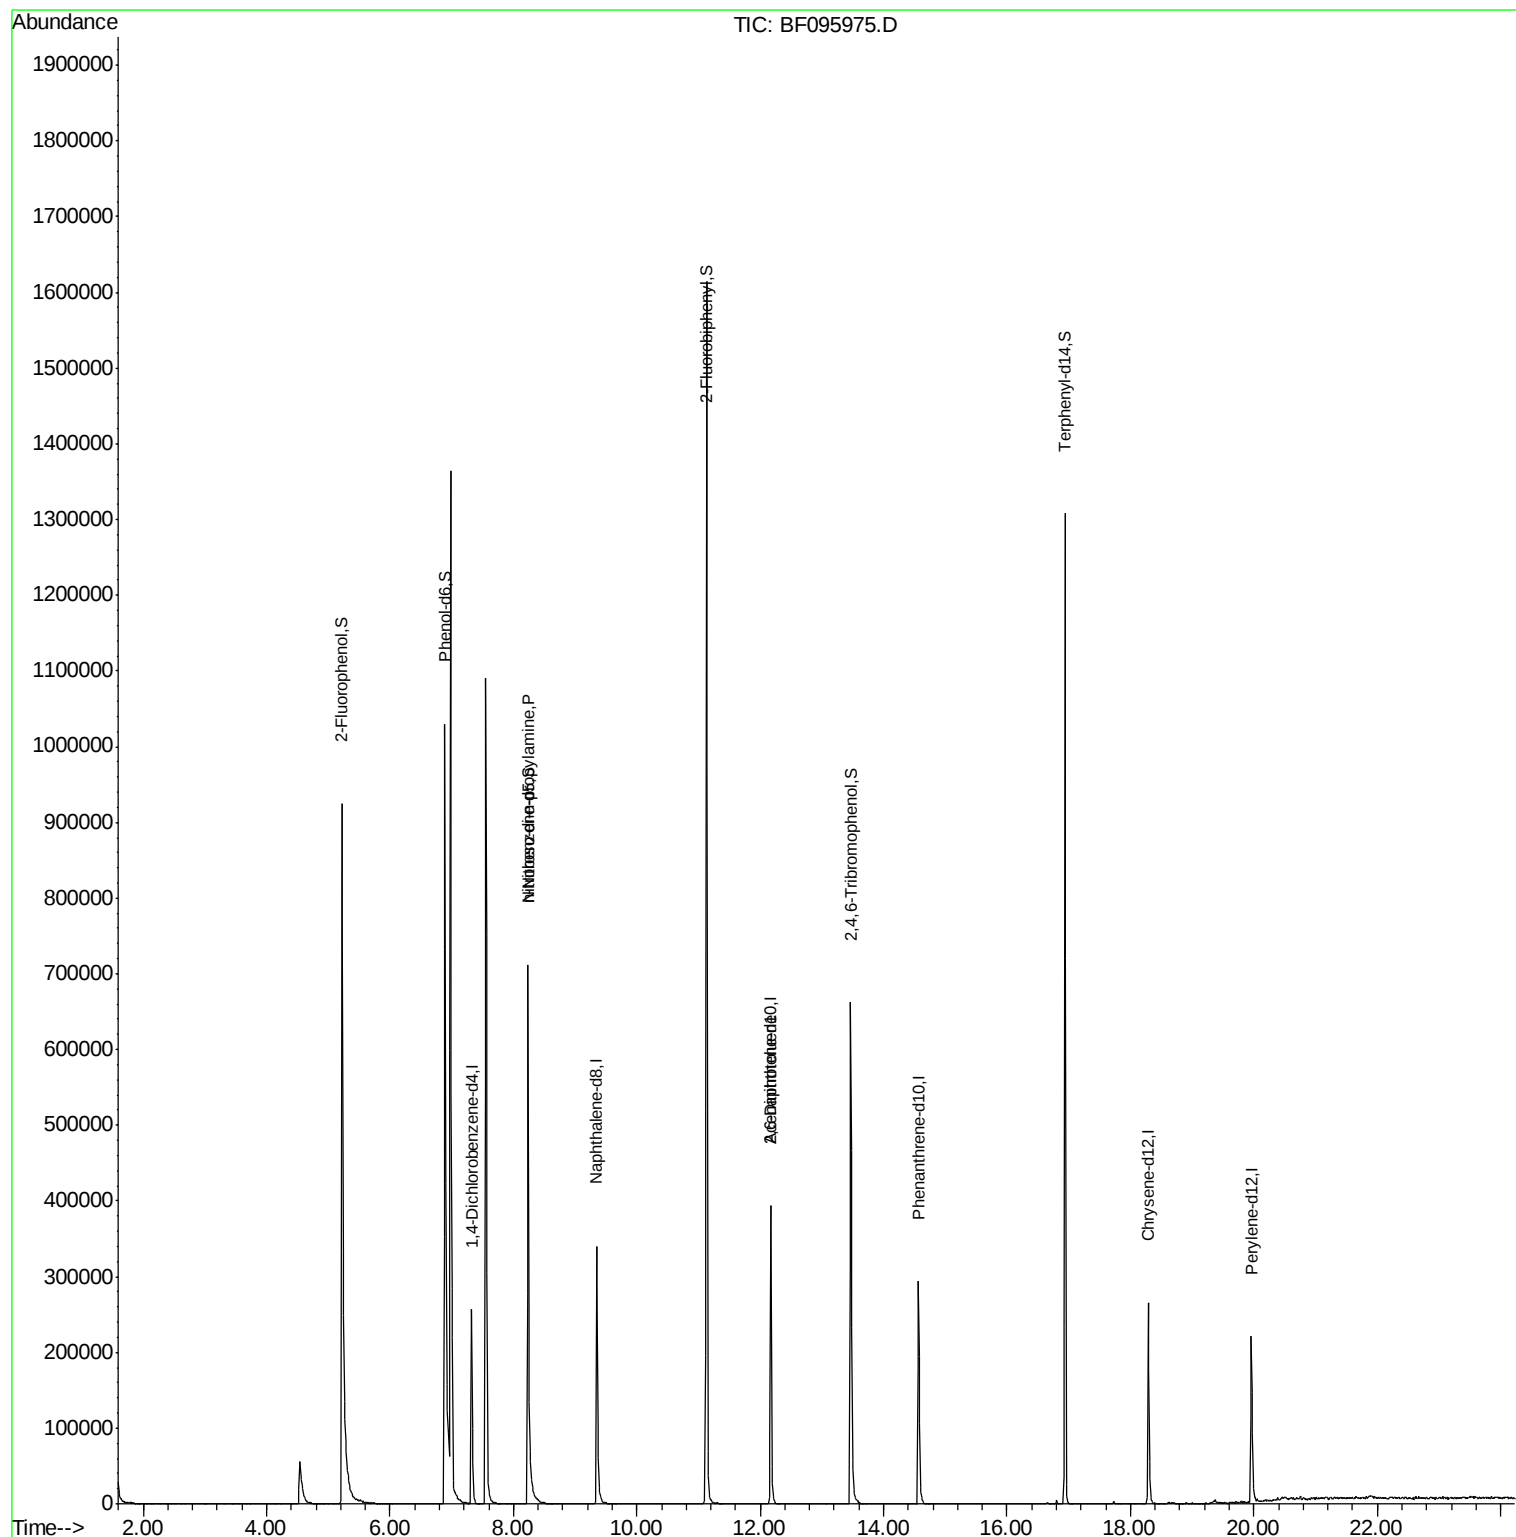

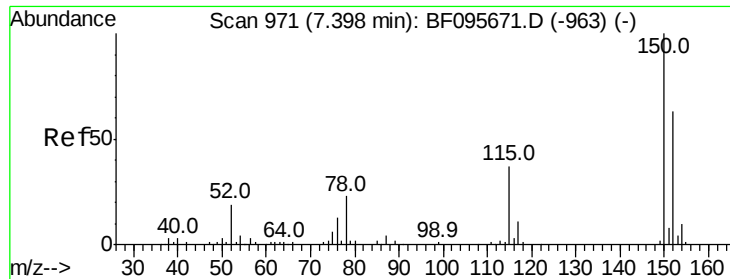


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.32 min Scan# 975
Delta R.T. 0.00 min
Lab File: BF095975.D
Acq: 17 Jun 2017 2:47

Instrument :
BNA_F
ClientSampled :

Tot Ion:152 Resp: 68284
Ion Ratio Lower Upper
152 100
150 156.5 126.2 189.2
115 57.2 52.2 78.2

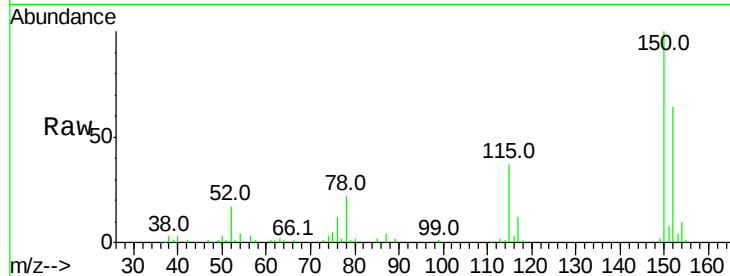


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

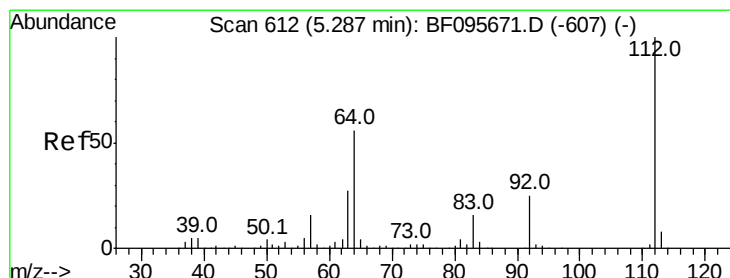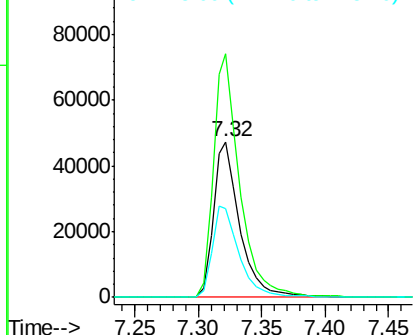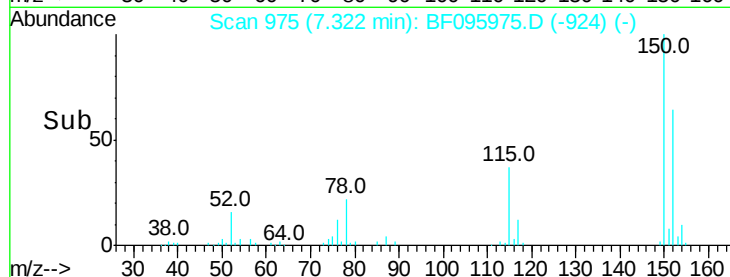



#5


2-Fluorophenol
Concen: 134.67 ng
RT: 5.22 min Scan# 618
Delta R.T. 0.01 min
Lab File: BF095975.D
Acq: 17 Jun 2017 2:47

Tgt Ion:112 Resp: 577096
Ion Ratio Lower Upper
112 100
64 56.0 46.0 69.0
63 26.7 23.4 35.0

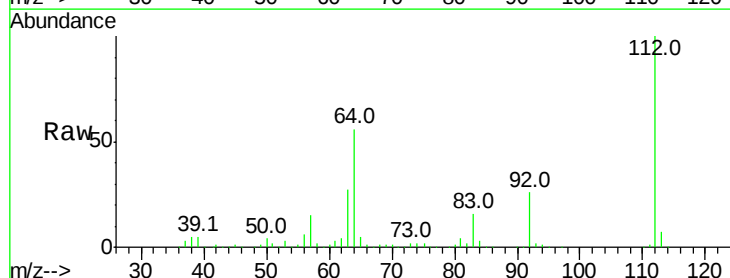

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

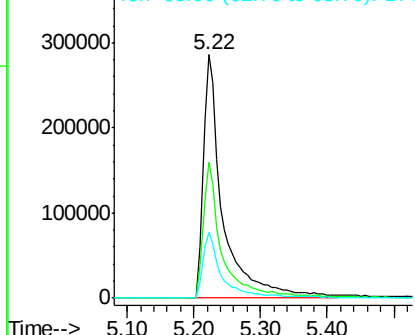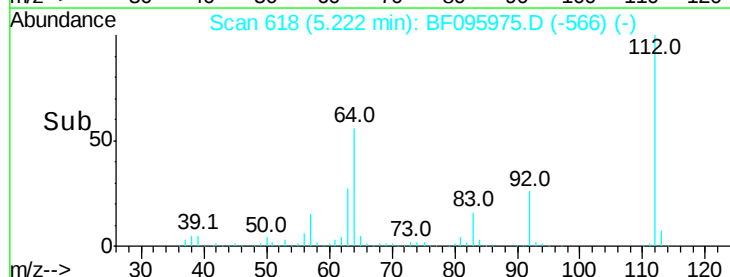

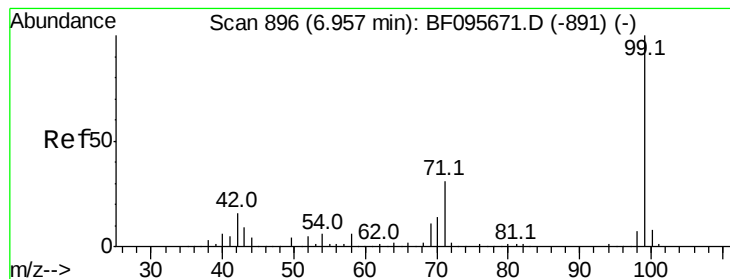

#7

Phenol-d6

Concen: 138.18 ng

RT: 6.89 min Scan# 902

Delta R.T. -0.02 min

Lab File: BF095975.D

Acq: 17 Jun 2017 2:47

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 99 Resp: 708869

Ion Ratio Lower Upper

99 100

42 16.6 13.5 20.3




71 32.5 24.5 36.7

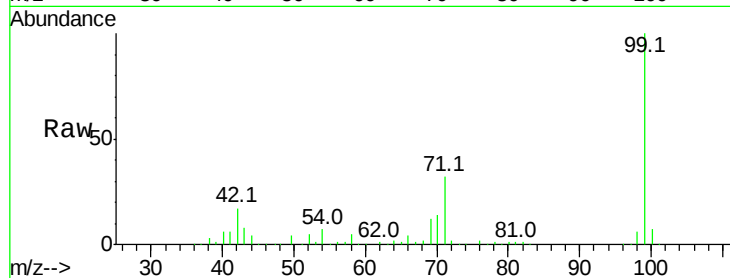

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

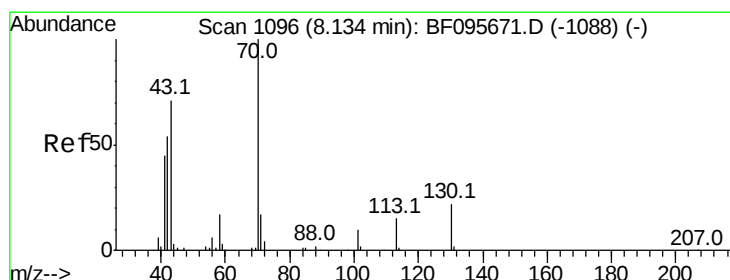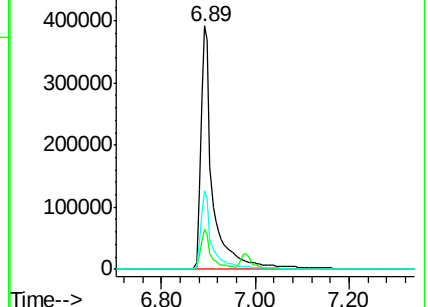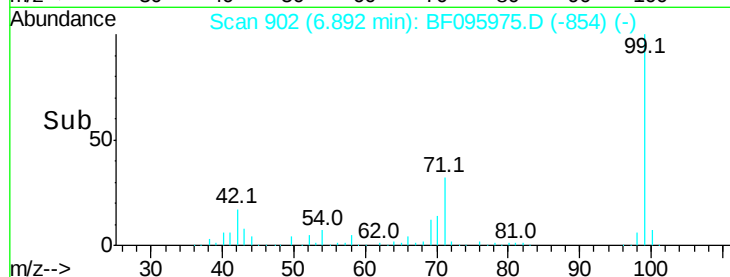

#19

n-Nitroso-di-n-propylamine

Concen: 15.34 ng

RT: 8.24 min Scan# 1131

Delta R.T. 0.17 min

Lab File: BF095975.D

Acq: 17 Jun 2017 2:47

Tgt Ion: 70 Resp: 49873


Ion Ratio Lower Upper

70 100

42 45.9 47.2 70.8#

101 0.0 7.2 10.8#

130 2.2 15.9 23.9#


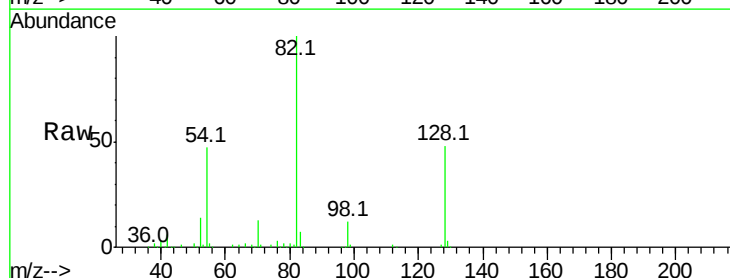



Abundance Ion 70.00 (69.70 to 70.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 101.00 (100.70 to 101.70): BF0

Ion 130.00 (129.70 to 130.70): BF0

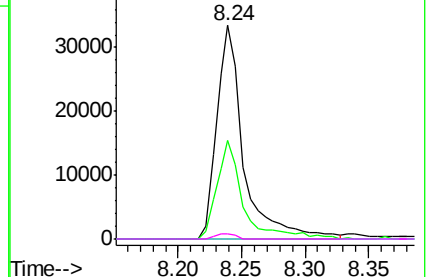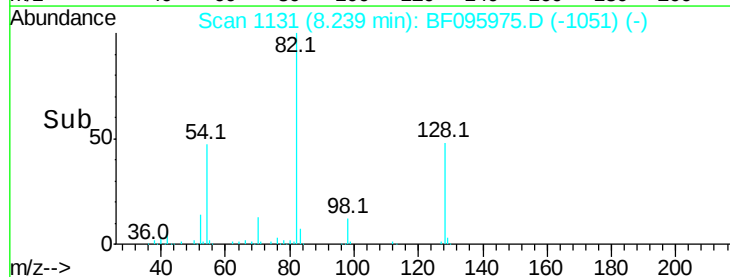


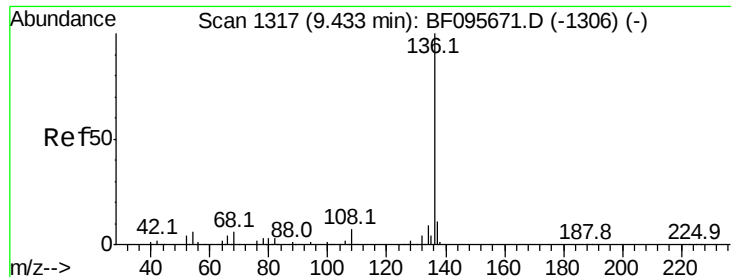




#21
Naphthalene-d8
Concen: 20.00 ng
RT: 9.35 min Scan# 1320
Delta R.T. -0.01 min
Lab File: BF095975.D
Acq: 17 Jun 2017 2:47

Instrument :
BNA_F
ClientSampleId :

Tot Ion:136	Resp:	278382
Ion Ratio	Lower	Upper
136	100	
137	10.9	8.5 12.7
54	6.8	4.9 7.3
68	6.0	4.1 6.1

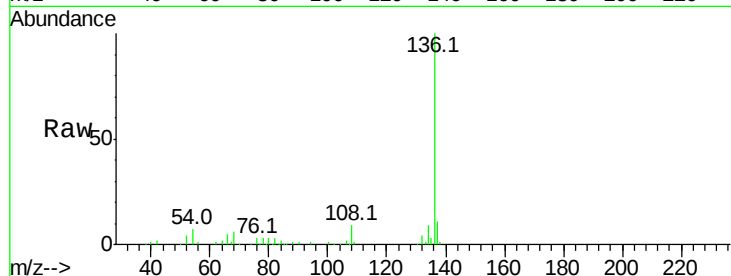


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

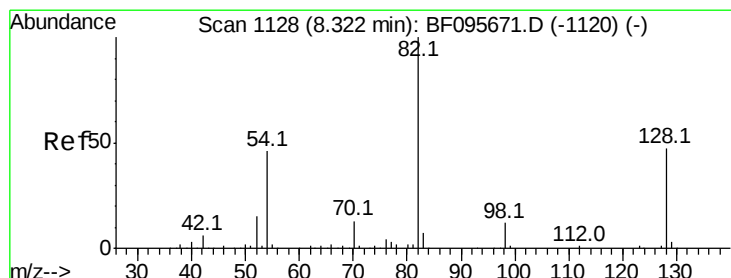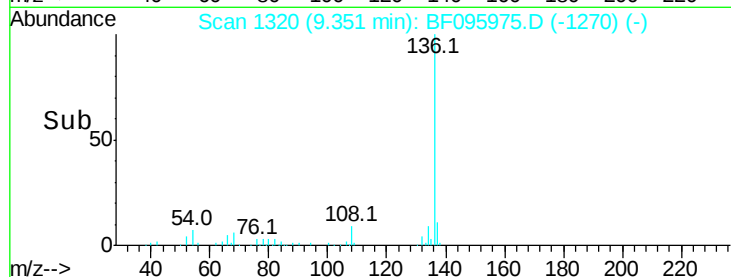
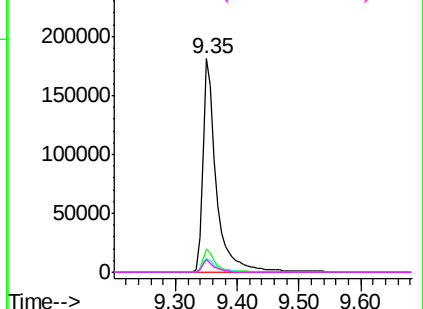



#23
Nitrobenzene-d5
Concen: 89.22 ng
RT: 8.24 min Scan# 1131
Delta R.T. -0.01 min
Lab File: BF095975.D
Acq: 17 Jun 2017 2:47

Tgt Ion: 82	Resp:	399917
Ion Ratio	Lower	Upper
82	100	
128	47.6	34.0 51.0
54	46.7	42.2 63.2

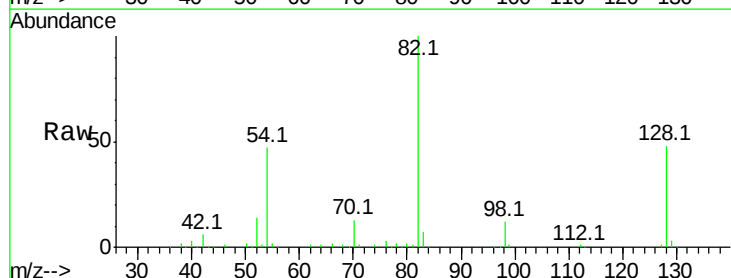

Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

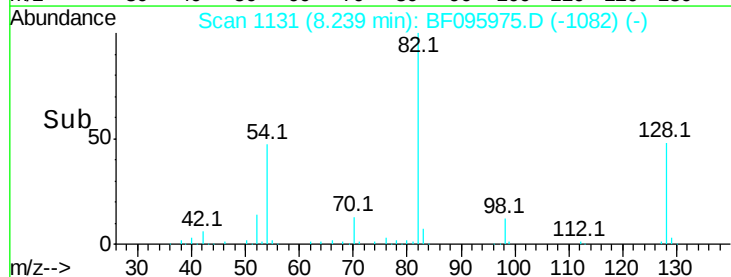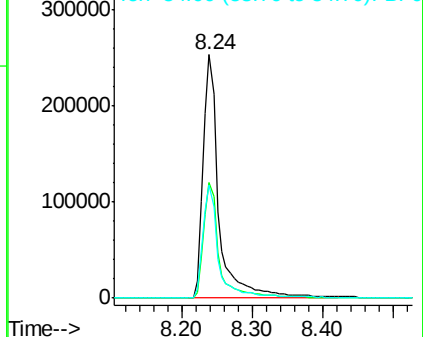

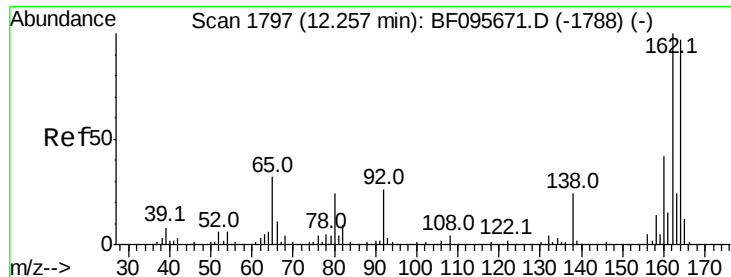

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 12.17 min Scan# 1799

Delta R.T. -0.01 min

Lab File: BF095975.D

Acq: 17 Jun 2017 2:47


Instrument :

BNA_F

ClientSampleId :

Tot Ion:164 Resp: 123244




Ion	Ratio	Lower	Upper
164	100		
162	102.5	82.6	123.8
160	43.3	36.2	54.2

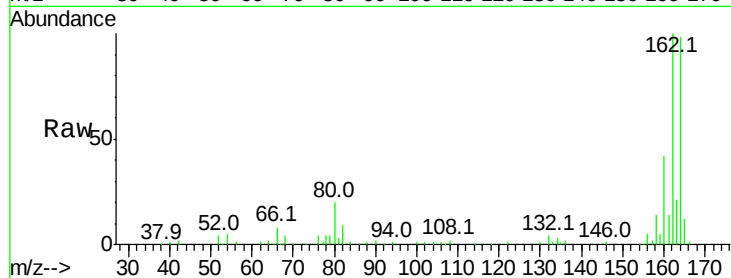

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

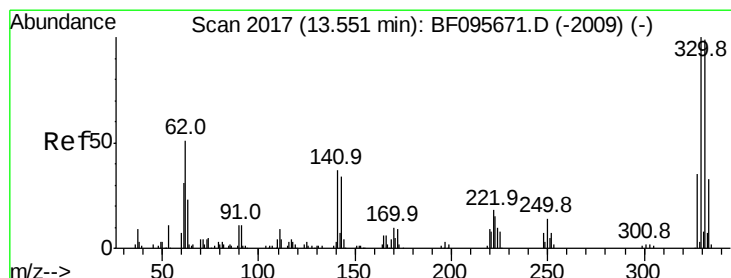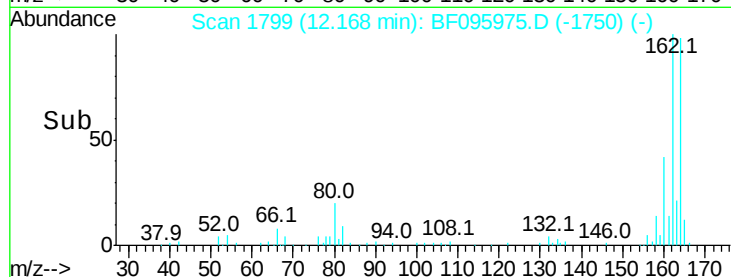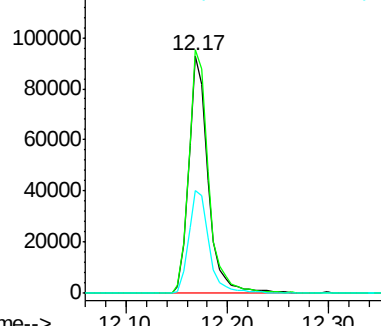

#41

2,4,6-Tribromophenol

Concen: 112.78 ng

RT: 13.47 min Scan# 2020


Delta R.T. -0.01 min

Lab File: BF095975.D

Acq: 17 Jun 2017 2:47

Tgt Ion:330 Resp: 122983



Ion	Ratio	Lower	Upper
330	100		
332	98.9	76.6	115.0
141	38.3	31.4	47.2

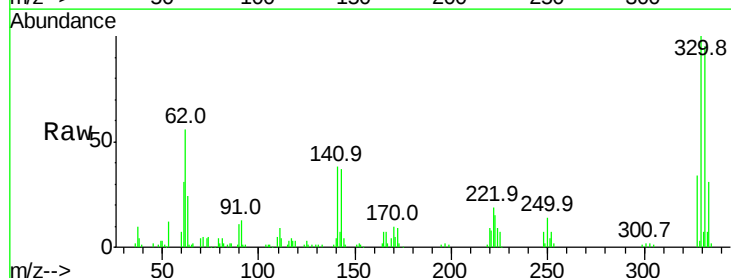


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



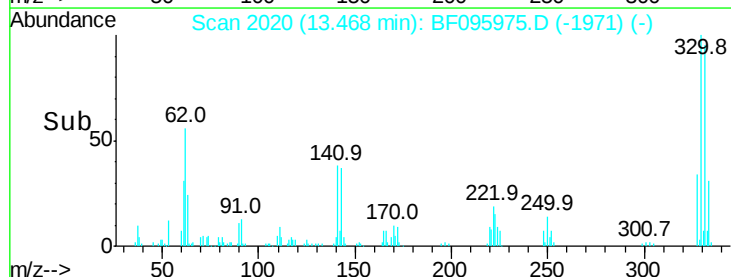
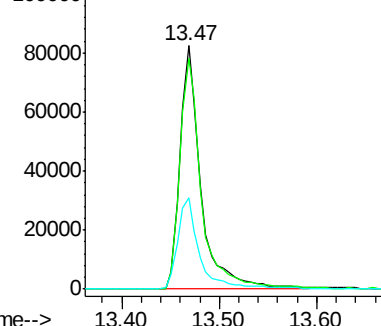


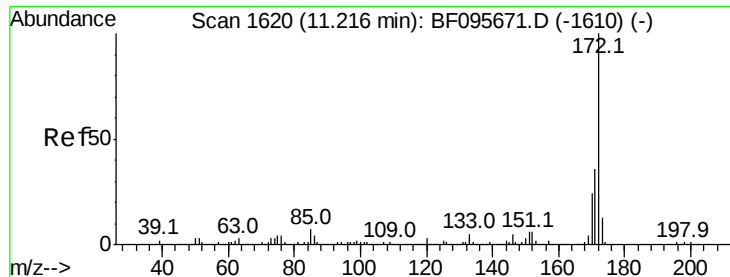

#44
2-Fluorobiphenyl
Concen: 89.73 ng
RT: 11.13 min Scan# 1623
Delta R.T. -0.01 min
Lab File: BF095975.D
Acq: 17 Jun 2017 2:47




Instrument :
BNA_F
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
172	100		
171	35.1	29.6	44.4
170	23.2	19.8	29.8

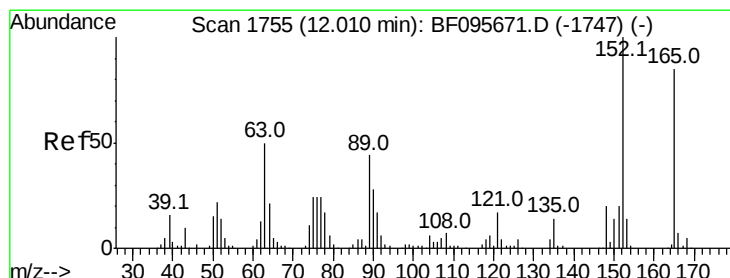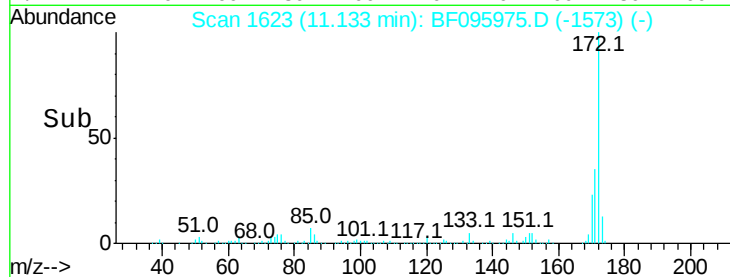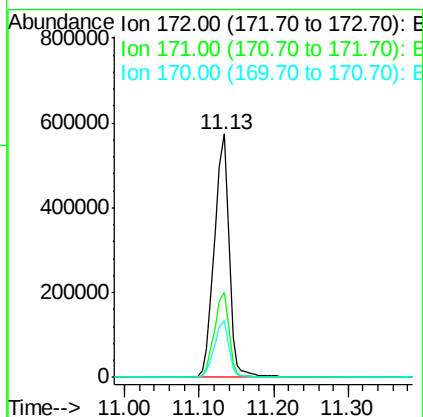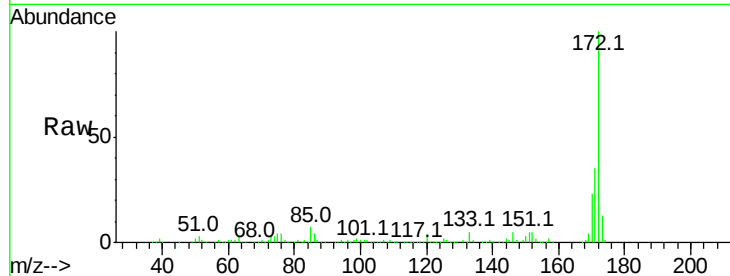

#50
2,6-Dinitrotoluene
Concen: 7.36 ng
RT: 12.17 min Scan# 1799
Delta R.T. 0.22 min
Lab File: BF095975.D
Acq: 17 Jun 2017 2:47

Tgt Ion	Ratio	Lower	Upper
165	100		
63	0.0	34.3	51.5#
89	0.0	37.1	55.7#


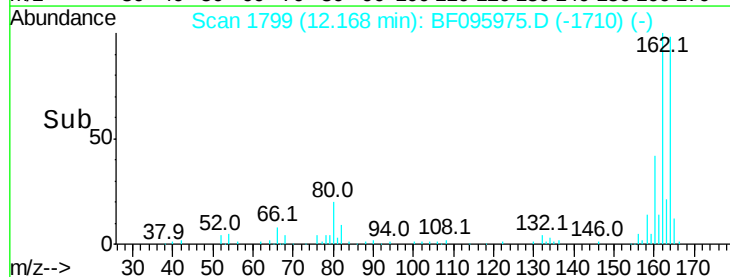
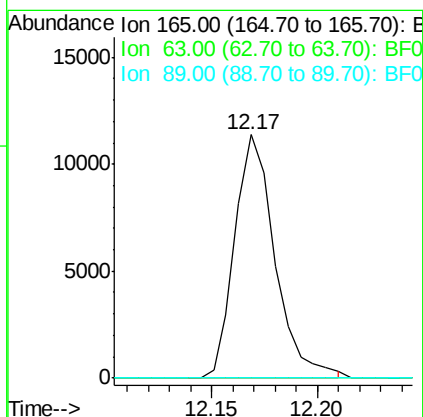
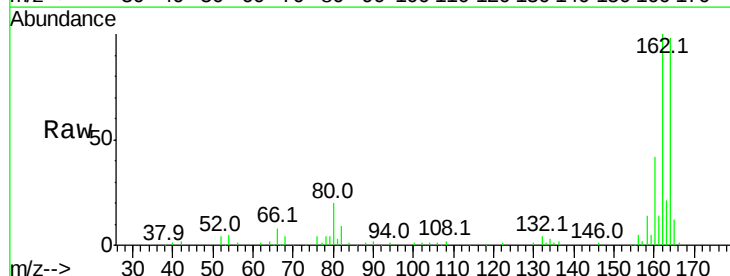


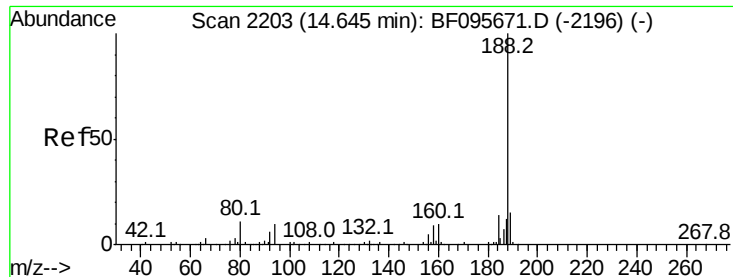

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 14.57 min Scan# 2207
Delta R.T. 0.00 min
Lab File: BF095975.D
Acq: 17 Jun 2017 2:47




Instrument :
BNA_F
ClientSampleId :


Tot Ion:188 Resp: 195117
Ion Ratio Lower Upper
188 100
94 9.4 9.4 14.2#
80 10.0 10.2 15.2#

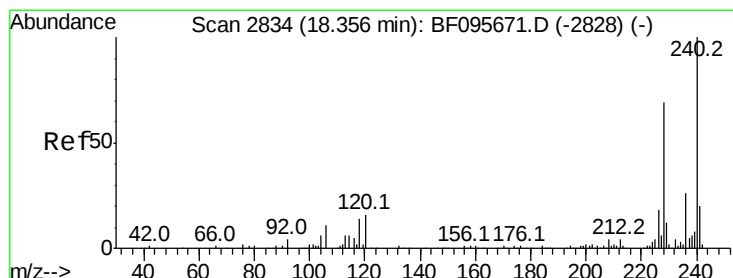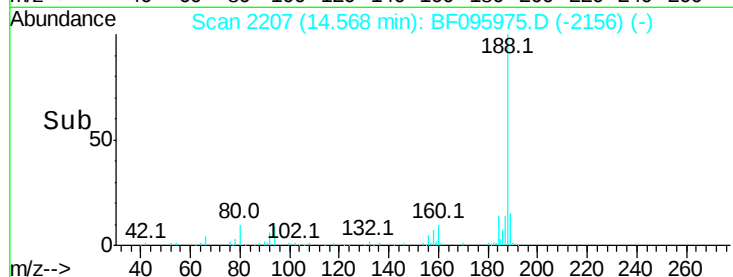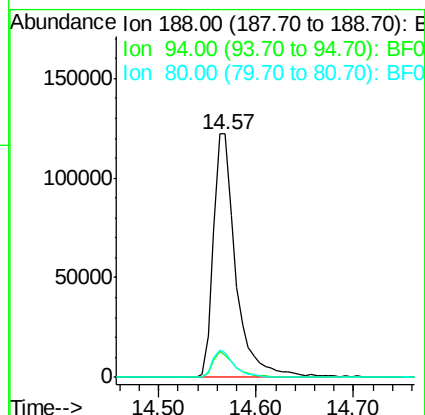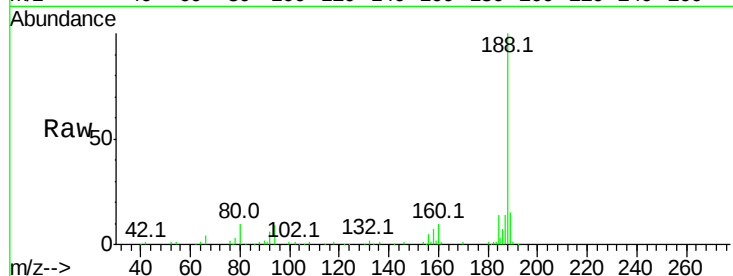

#75
Chrysene-d12
Concen: 20.00 ng
RT: 18.29 min Scan# 2840
Delta R.T. -0.01 min
Lab File: BF095975.D
Acq: 17 Jun 2017 2:47

Tgt Ion:240 Resp: 135699
Ion Ratio Lower Upper
240 100
120 13.8 5.8 8.8#
236 25.9 20.5 30.7

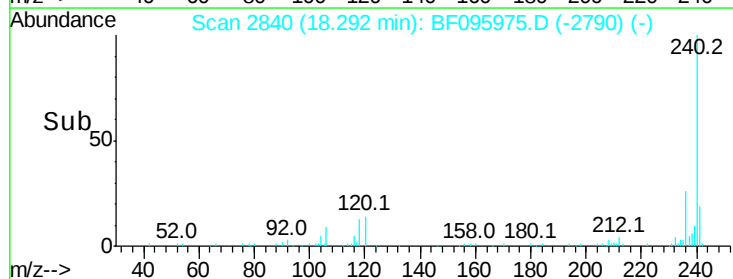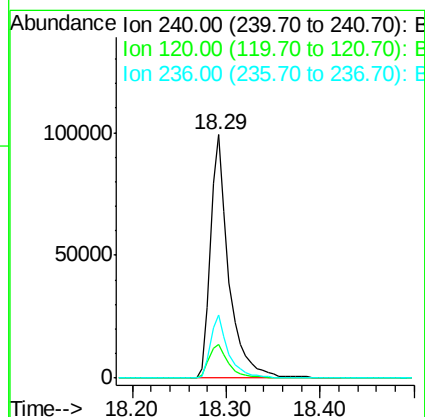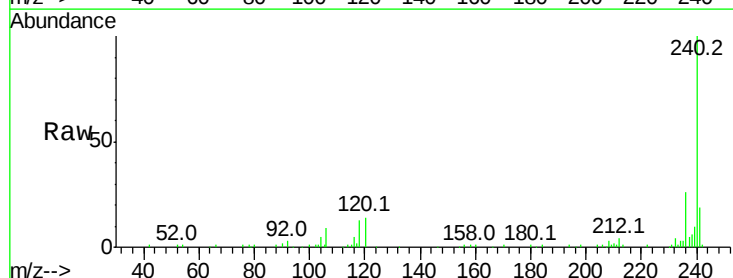


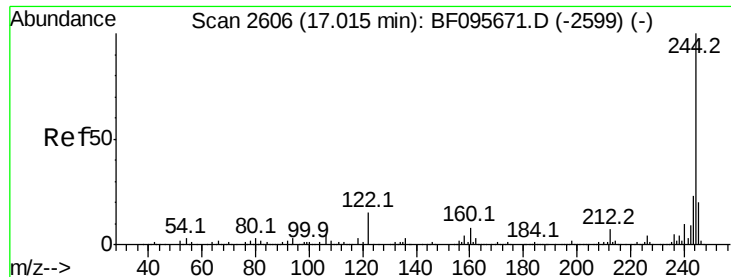


#78
 Terphenyl-d14
 Concen: 90.83 ng
 RT: 16.94 min Scan# 2611
 Delta R.T. -0.01 min
 Lab File: BF095975.D
 Acq: 17 Jun 2017 2:47

Instrument :
 BNA_F
 ClientSampleID :



Tot Ion:244 Resp: 496667
 Ion Ratio Lower Upper
 244 100
 212 7.0 6.0 9.0
 122 14.2 10.3 15.5

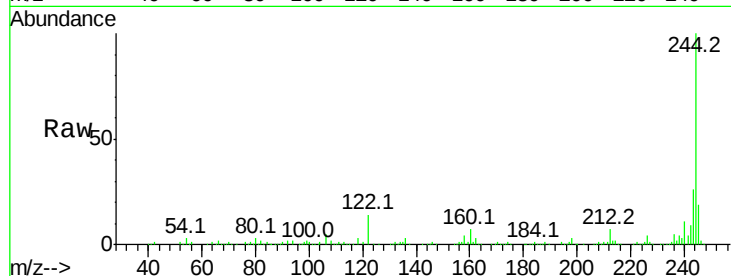

Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

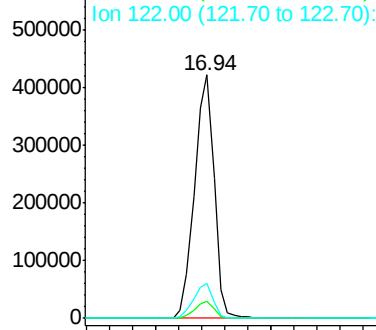


Time-->

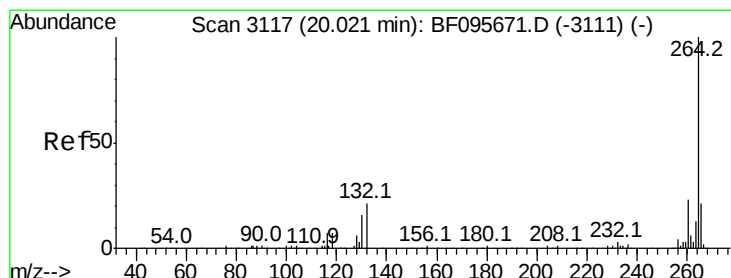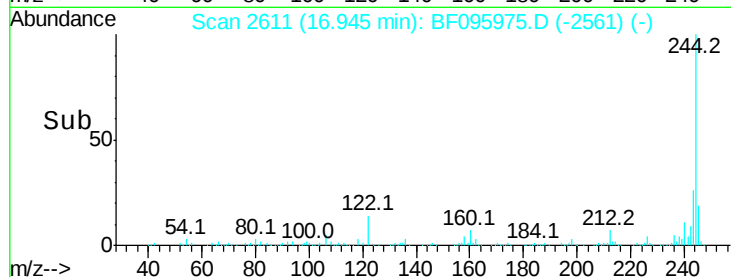


#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 19.96 min Scan# 3124
 Delta R.T. 0.00 min
 Lab File: BF095975.D
 Acq: 17 Jun 2017 2:47

Tgt Ion:264 Resp: 126563
 Ion Ratio Lower Upper
 264 100
 260 22.1 19.5 29.3
 265 21.5 17.2 25.8

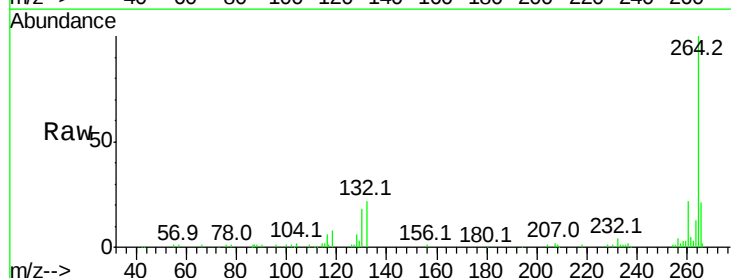

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

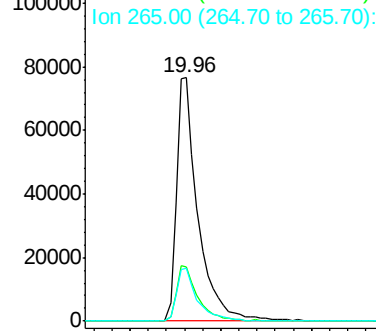

Time-->

