
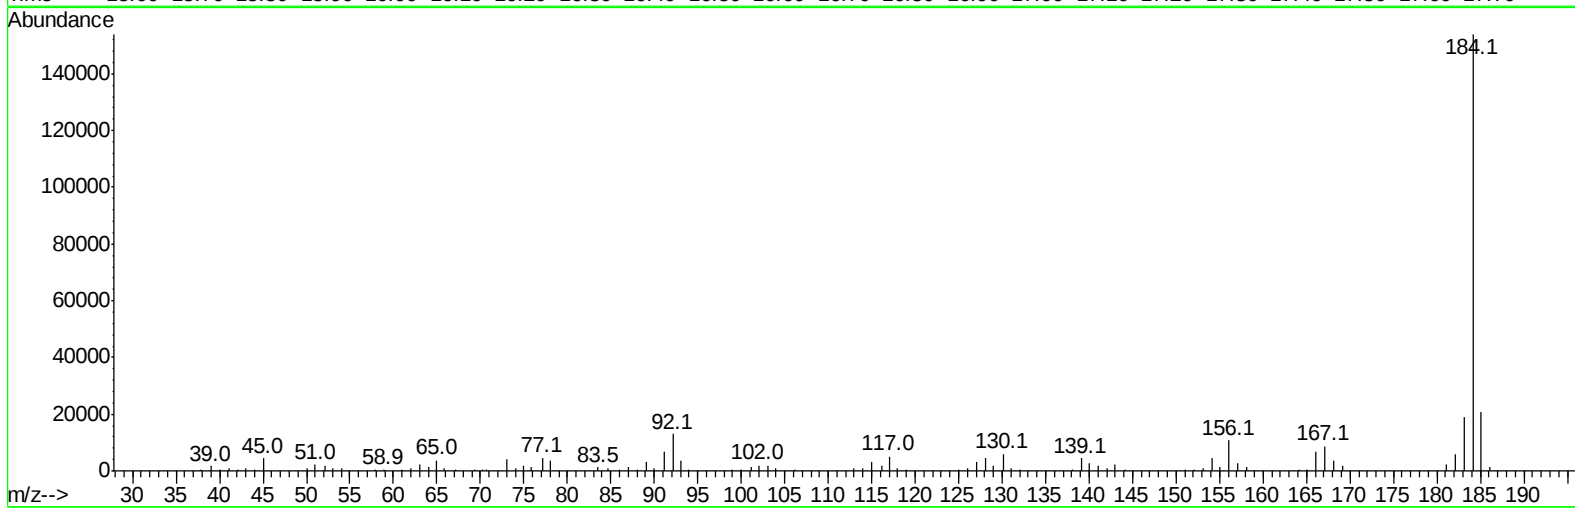


Data Path : Z:\HPCHEM1\BNA F\DATA\BF061617\
Data File : BF095950.D
Acq On : 16 Jun 2017 12:07
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 19 02:48:26 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 16 17:12:03 2017
Response via : Initial Calibration

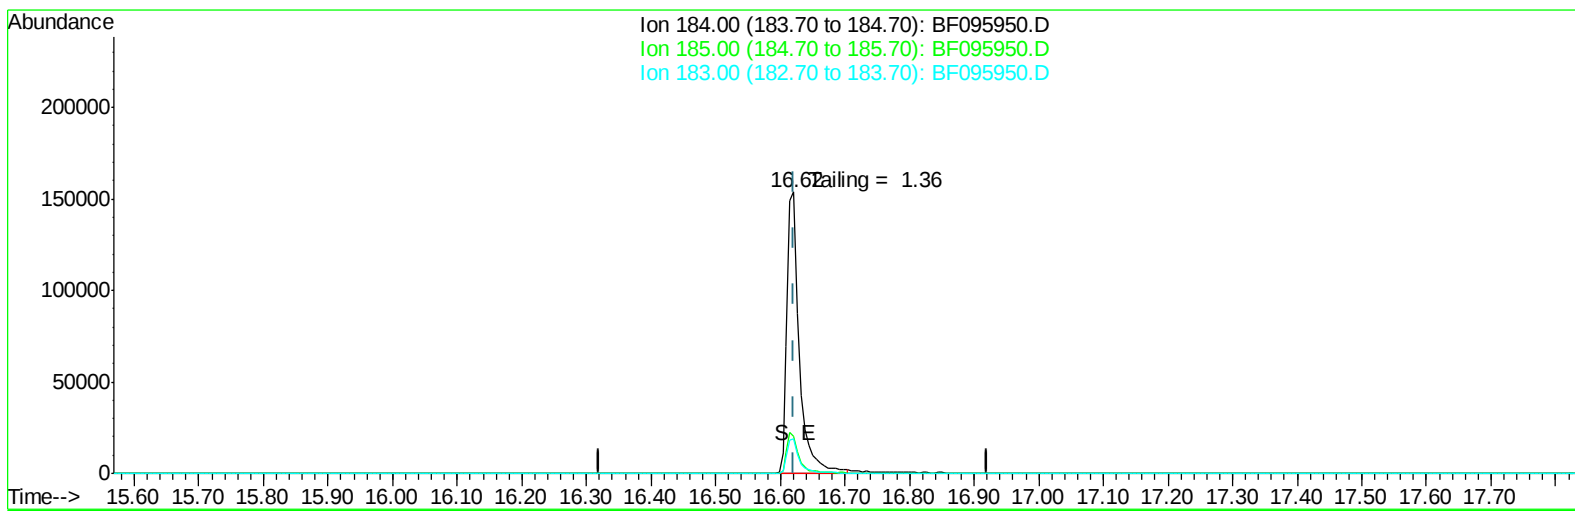

TIC: BF095950.D

(76) Benzidine



16.621min (+0.000) 0.00ng

response 216449

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	13.36#
183.00	12.20	12.46
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF061617\
Data File : BF095950.D
Acq On : 16 Jun 2017 12:07
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 19 02:48:26 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 16 17:12:03 2017
Response via : Initial Calibration

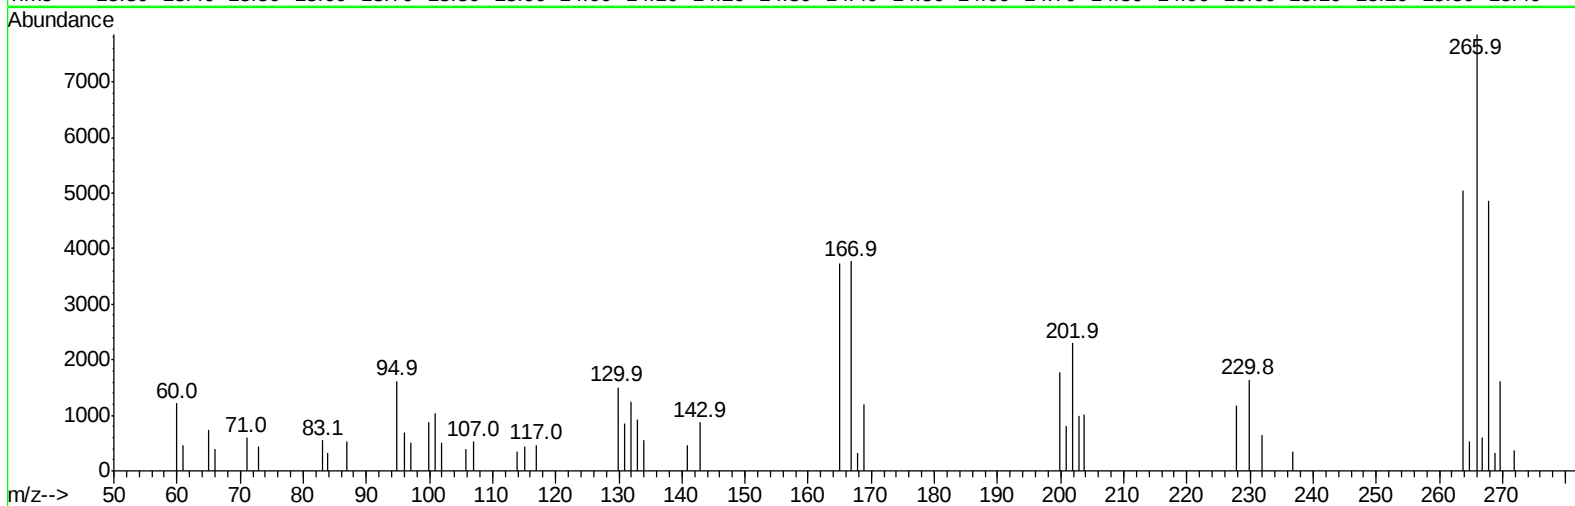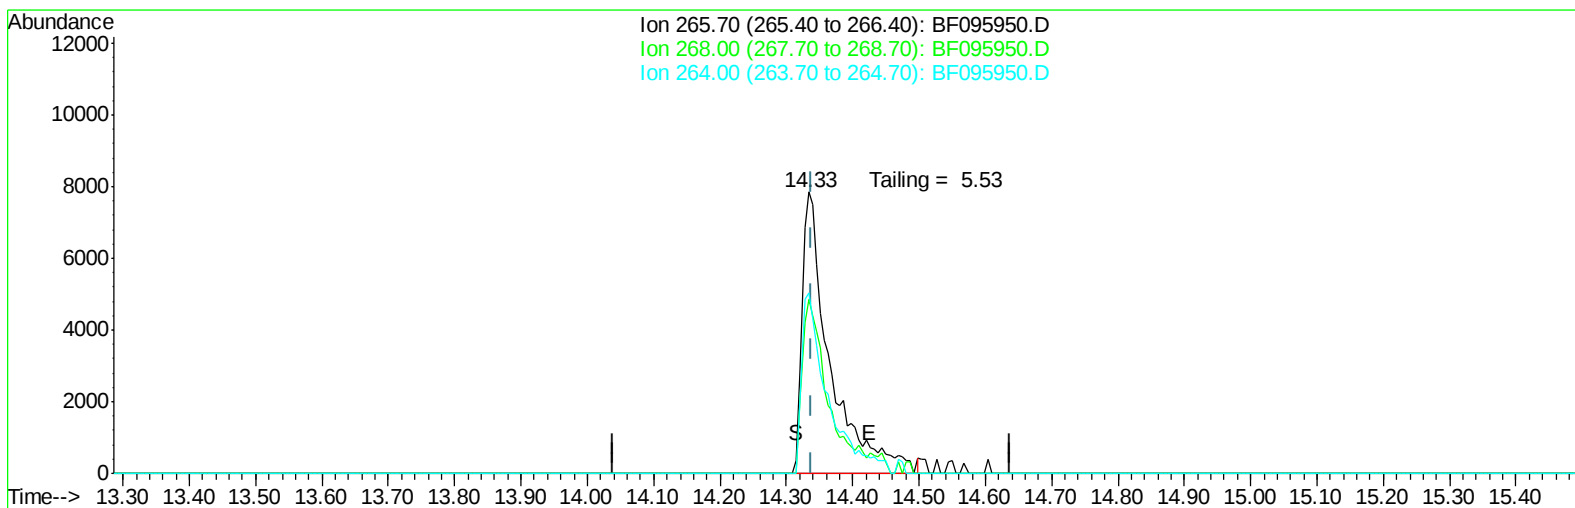

TIC: BF095950.D

(69) Pentachlorophenol (C)

14.333min (-0.006) 0.00ng

response 22509

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.97
264.00	64.60	64.13
0.00	0.00	0.00