
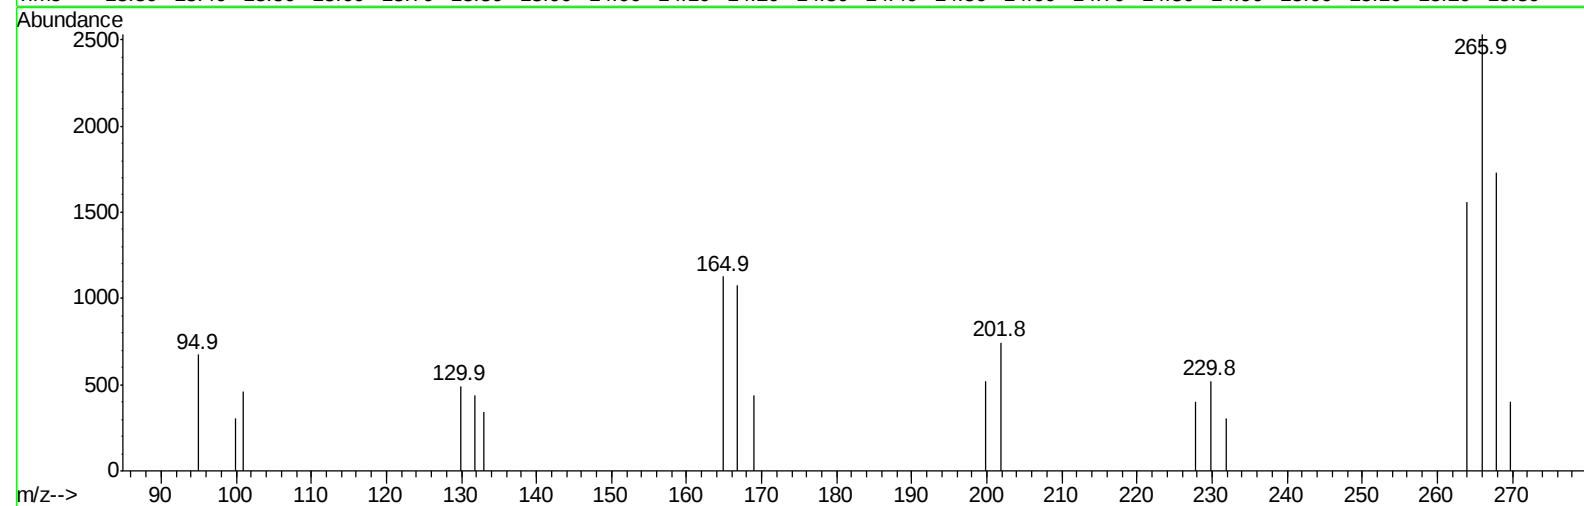


Data Path : Z:\HPCHEM1\BNA F\DATA\BF061617\
Data File : BF095973.D
Acq On : 17 Jun 2017 1:24
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 19 02:49:35 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 16 17:12:03 2017
Response via : Initial Calibration

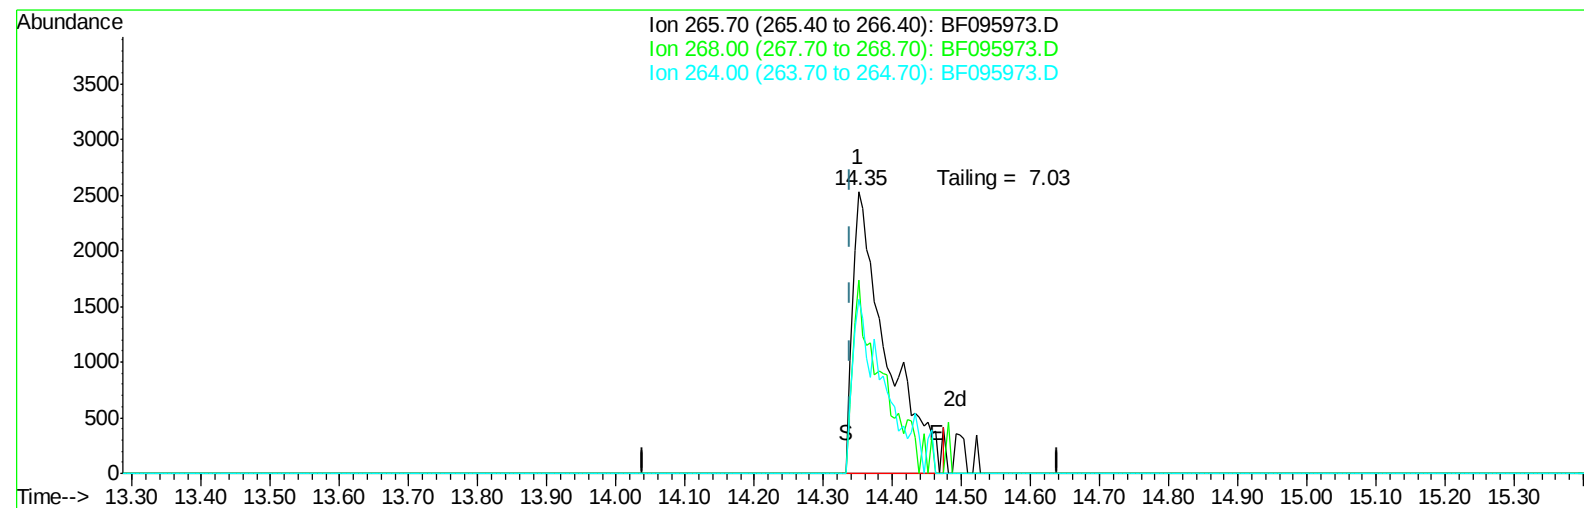

TIC: BF095973.D

(69) Pentachlorophenol (C)



14.351min (+0.012) 0.00ng

response 6544

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	68.43
264.00	64.60	61.71
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF061617\
Data File : BF095973.D
Acq On : 17 Jun 2017 1:24
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 19 02:49:35 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 16 17:12:03 2017
Response via : Initial Calibration

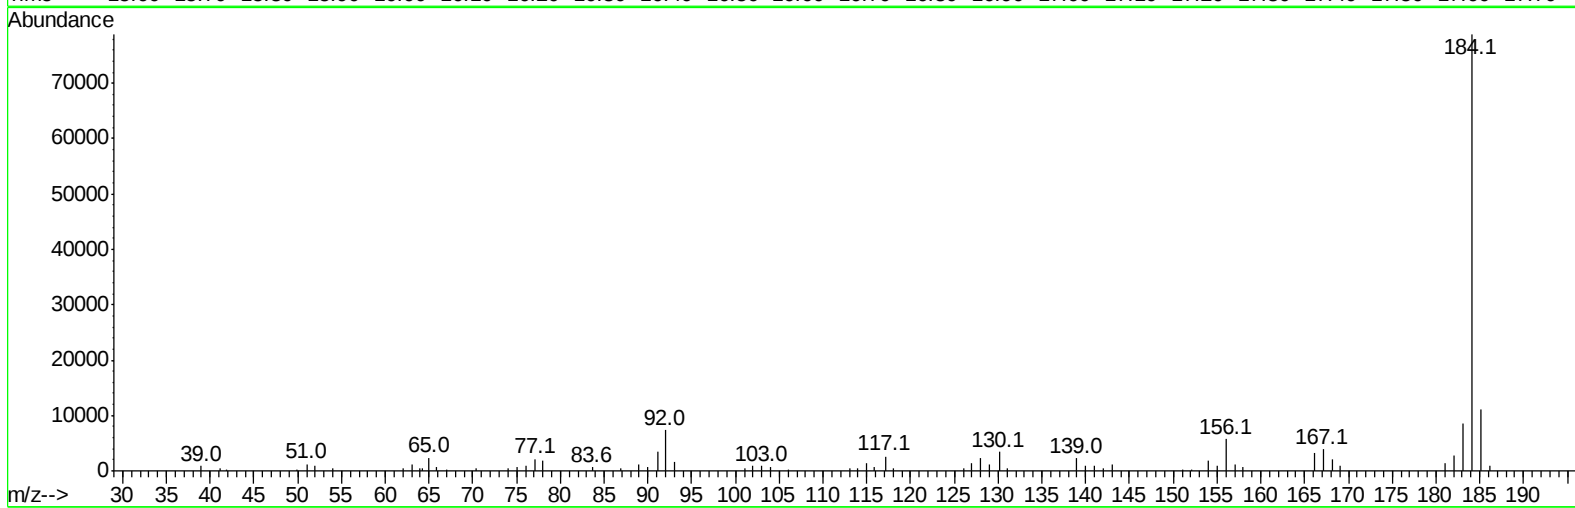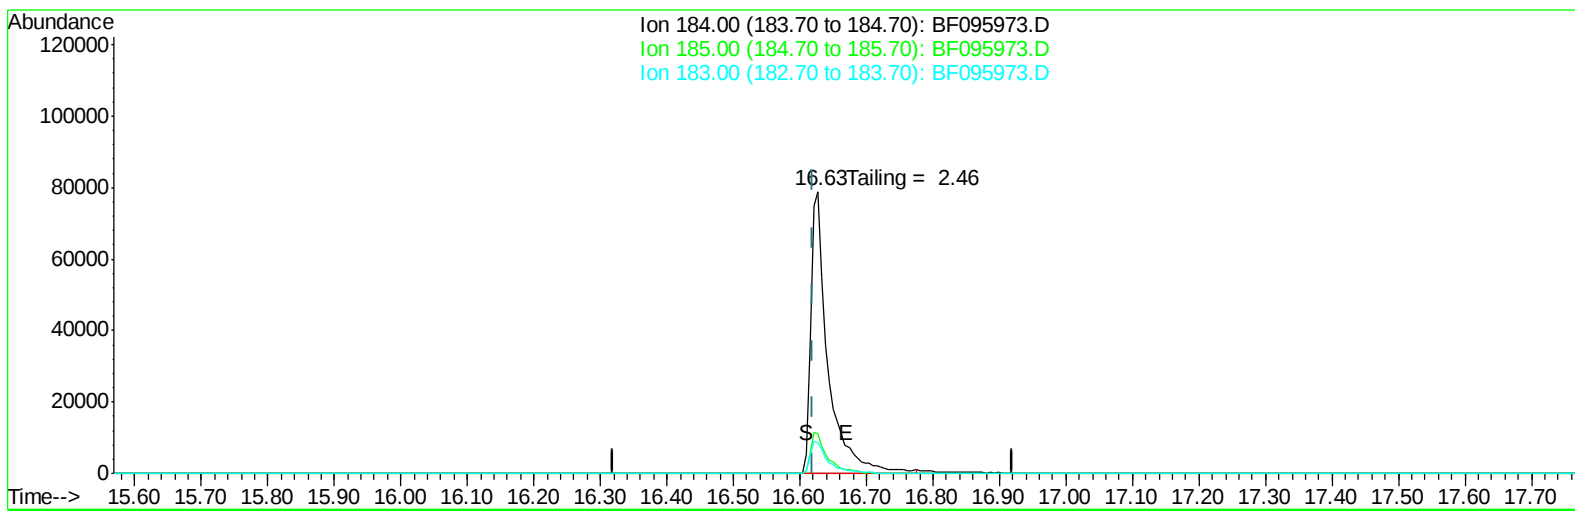

TIC: BF095973.D

(76) Benzidine

16.627min (+0.006) 0.00ng

response 142370

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.11#
183.00	12.20	10.85
0.00	0.00	0.00