

Data Path : Z:\HPCHEM1\BNA F\DATA\BF061617\
 Data File : BF095963.D
 Acq On : 16 Jun 2017 19:13
 Operator : SJ/MA
 Sample : I3676-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-09-6-7

Quant Time: Jun 17 00:04:55 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 16 17:12:03 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.32	152	62334	20.00	ng	0.00
21) Naphthalene-d8	9.35	136	253204	20.00	ng	0.00
38) Acenaphthene-d10	12.17	164	112425	20.00	ng	-0.01
63) Phenanthrene-d10	14.56	188	190382	20.00	ng	0.00
75) Chrysene-d12	18.29	240	126481	20.00	ng	0.00
86) Perylene-d12	19.96	264	123659	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.22	112	550657	140.77	ng	0.00
7) Phenol-d6	6.90	99	689731	147.28	ng	-0.01
23) Nitrobenzene-d5	8.24	82	385814	94.63	ng	-0.01
41) 2,4,6-Tribromophenol	13.47	330	133415	134.13	ng	-0.01
44) 2-Fluorobiphenyl	11.13	172	674541	83.49	ng	0.00
78) Terphenyl-d14	16.94	244	442205	86.77	ng	0.00
Target Compounds						Qvalue
49) Dimethylphthalate	11.83	163	130135	15.25	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF061617\
Data File : BF095963.D
Acq On : 16 Jun 2017 19:13
Operator : SJ/MA
Sample : I3676-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-09-6-7

Quant Time: Jun 17 00:04:55 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 16 17:12:03 2017
Response via : Initial Calibration

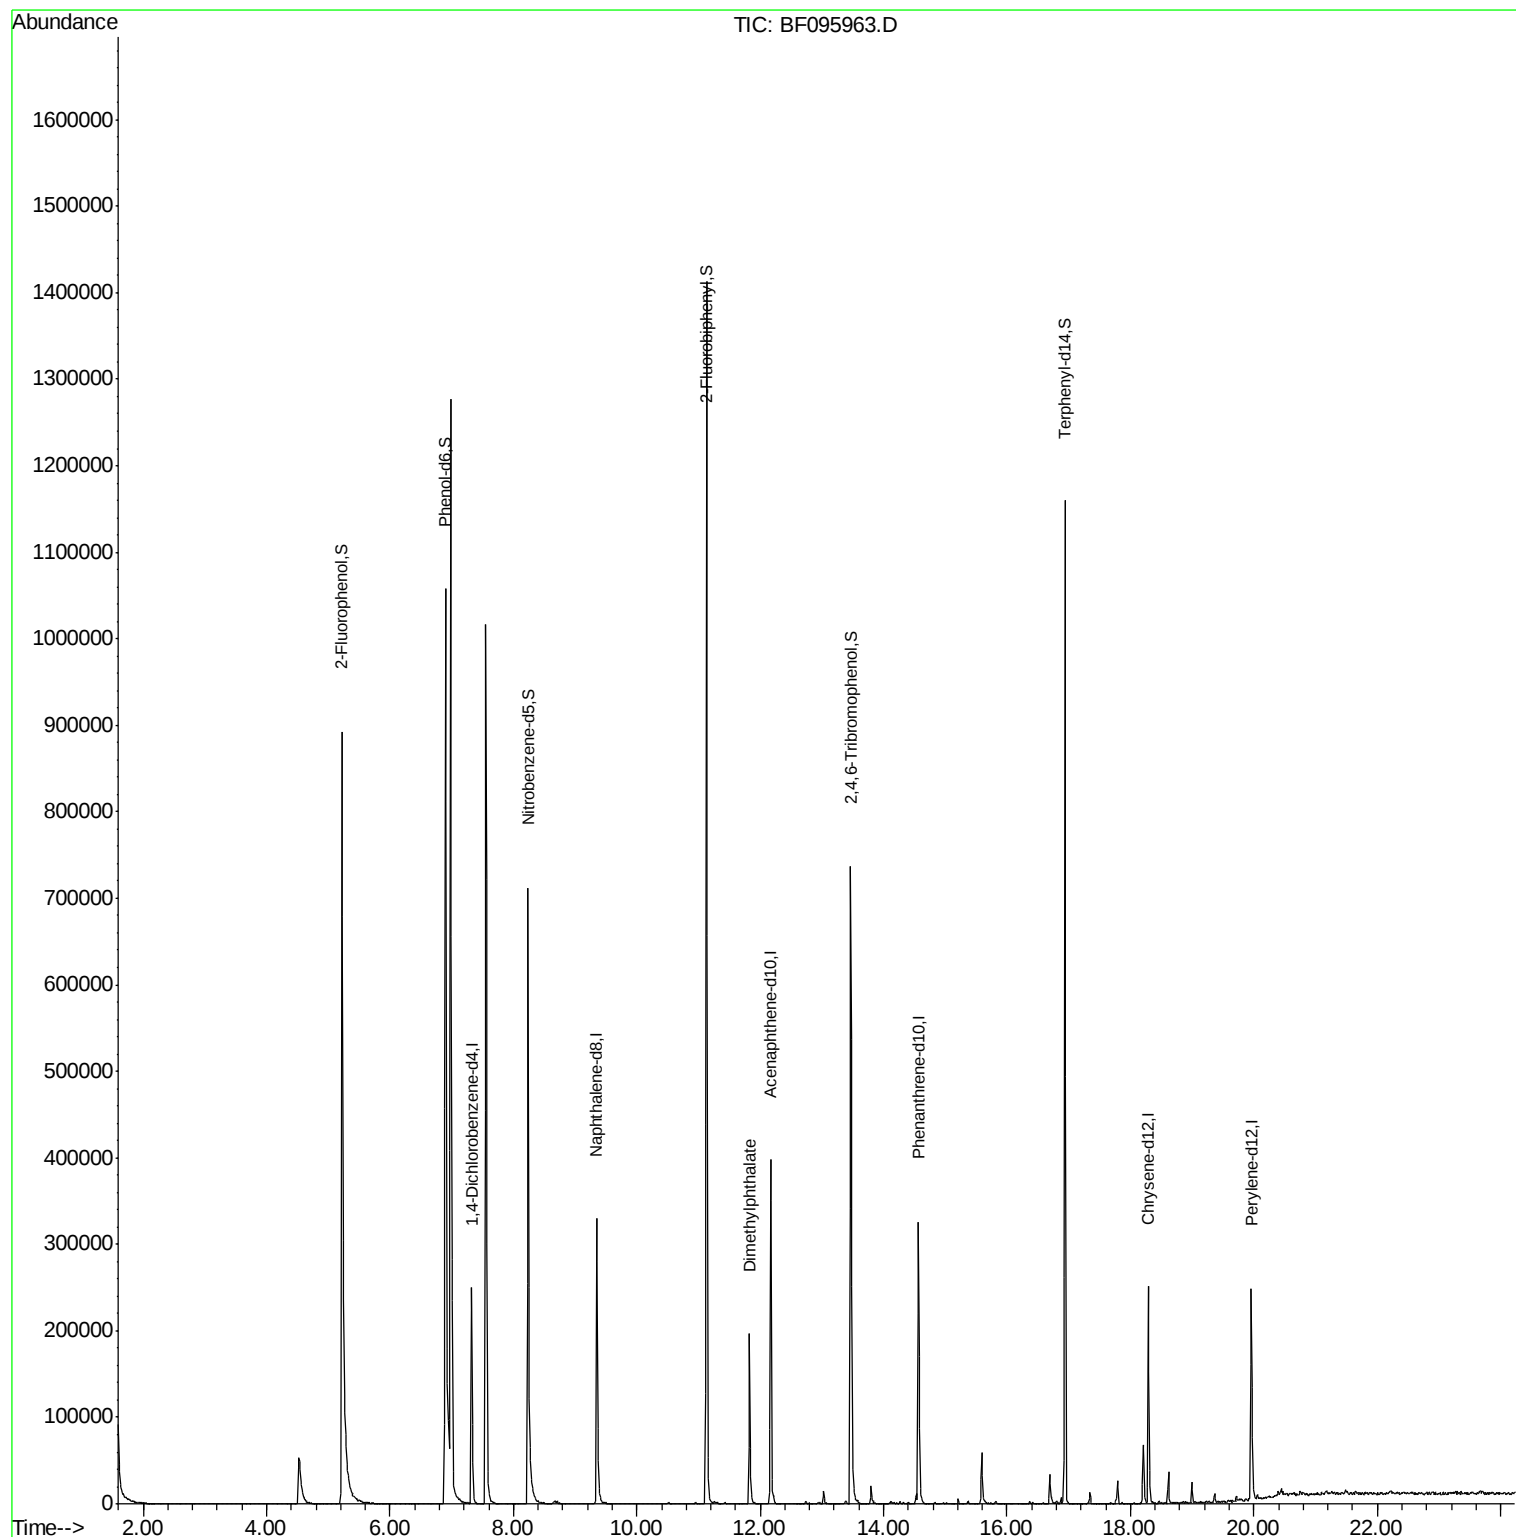

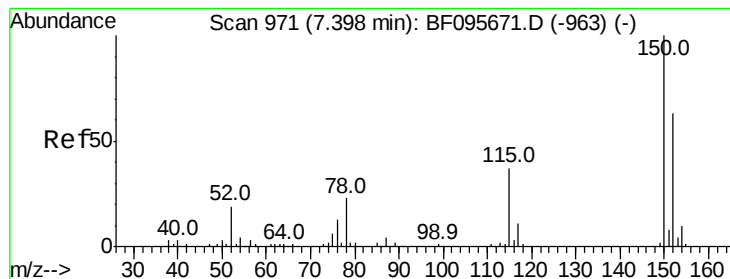


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.32 min Scan# 975
Delta R.T. 0.00 min
Lab File: BF095963.D
Acq: 16 Jun 2017 19:13

Instrument :
BNA_F
ClientSampleId :
SB-09-6-7

Tot Ion:152 Resp: 62334
Ion Ratio Lower Upper
152 100
150 160.0 126.2 189.2
115 58.6 52.2 78.2

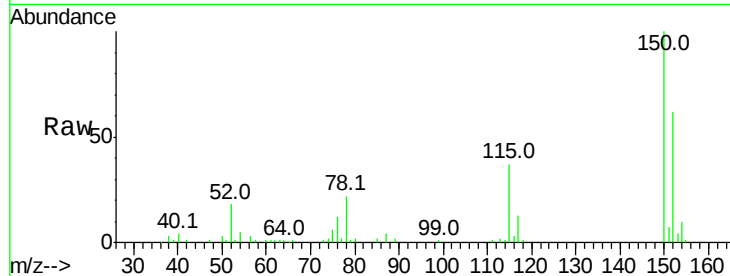


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

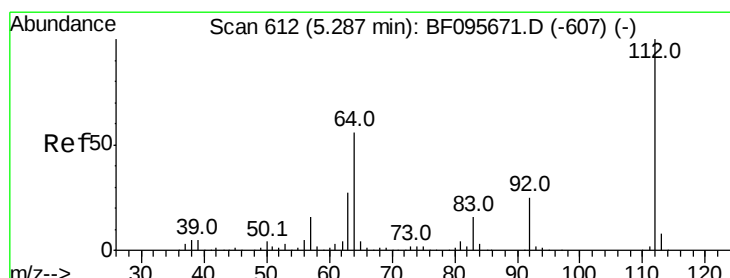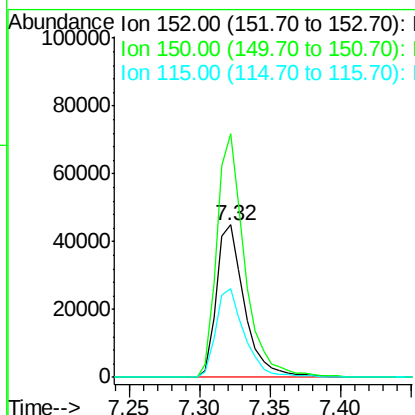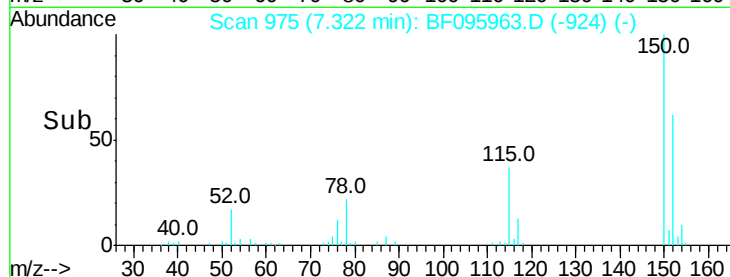



#5

2-Fluorophenol
Concen: 140.77 ng
RT: 5.22 min Scan# 618
Delta R.T. 0.01 min
Lab File: BF095963.D
Acq: 16 Jun 2017 19:13

Tgt Ion:112 Resp: 550657
Ion Ratio Lower Upper
112 100
64 53.9 46.0 69.0
63 27.5 23.4 35.0

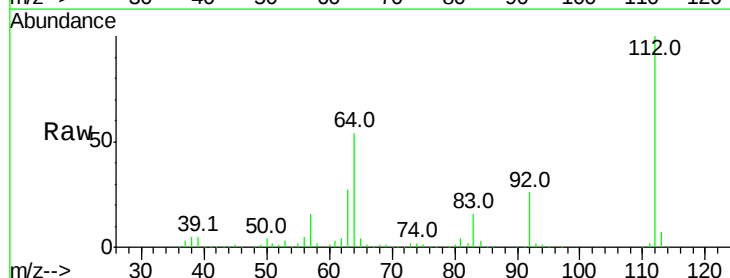

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

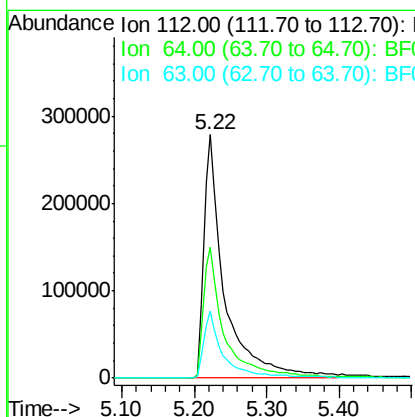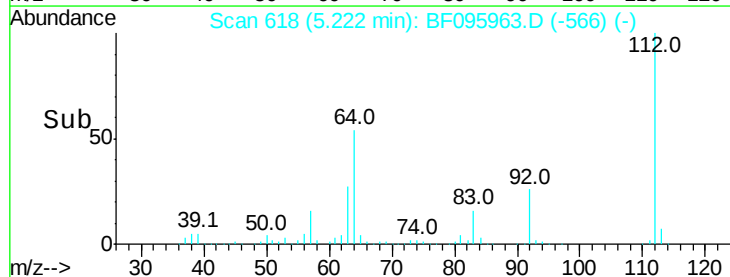



#7

Phenol-d6

Concen: 147.28 ng

RT: 6.90 min Scan# 903

Delta R.T. -0.01 min

Lab File: BF095963.D

Acq: 16 Jun 2017 19:13

Instrument :

BNA_F

ClientSampled :

SB-09-6-7


Tot Ion: 99 Resp: 689731

Ion Ratio Lower Upper

99 100

42 16.8 13.5 20.3




71 32.9 24.5 36.7

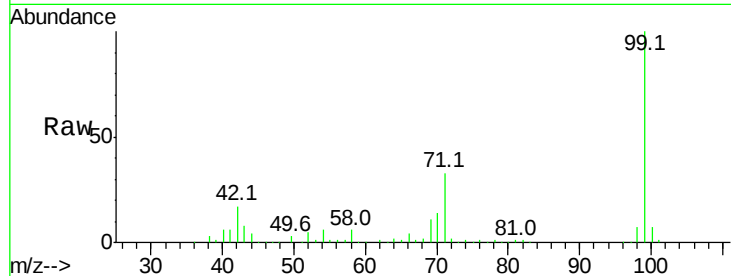

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

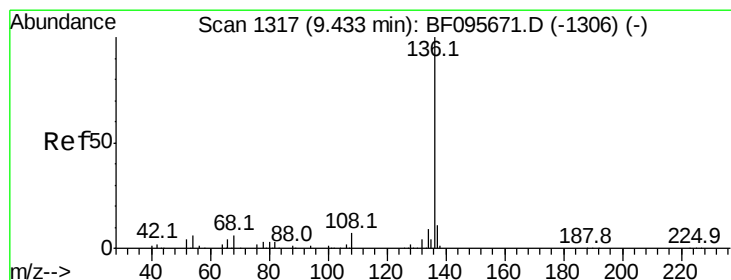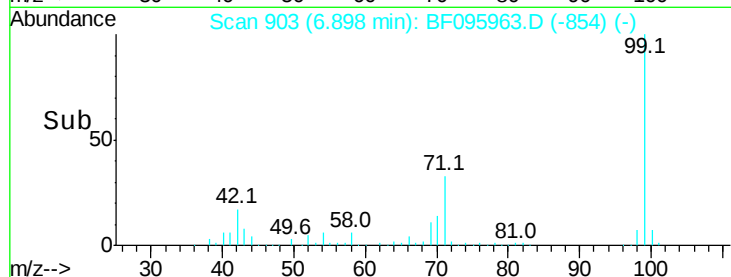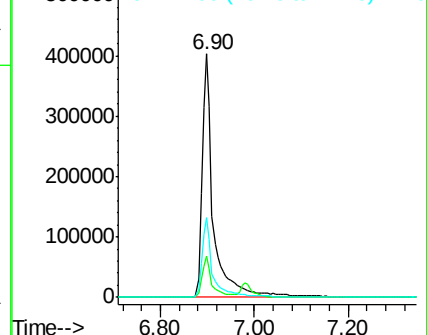

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 9.35 min Scan# 1320

Delta R.T. -0.01 min

Lab File: BF095963.D

Acq: 16 Jun 2017 19:13

Tgt Ion: 136 Resp: 253204


Ion Ratio Lower Upper

136 100

137 10.5 8.5 12.7

54 7.2 4.9 7.3

68 5.2 4.1 6.1


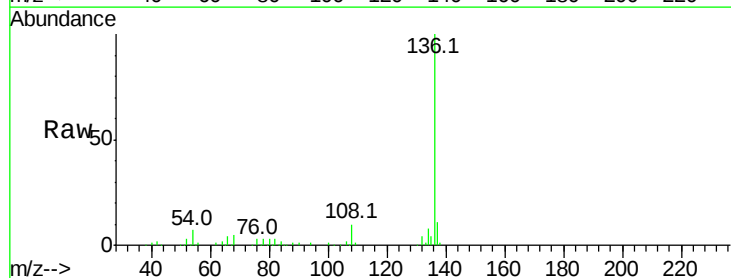



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



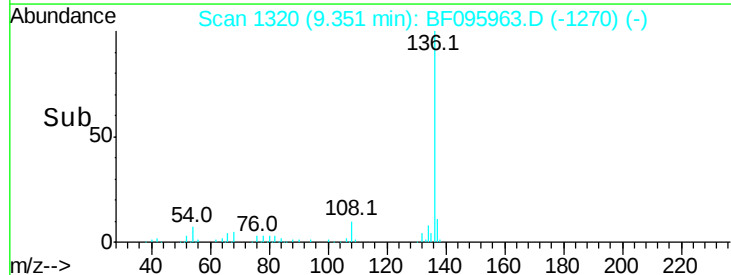
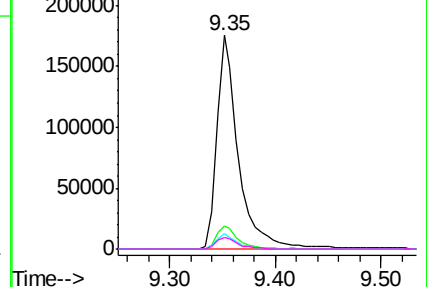


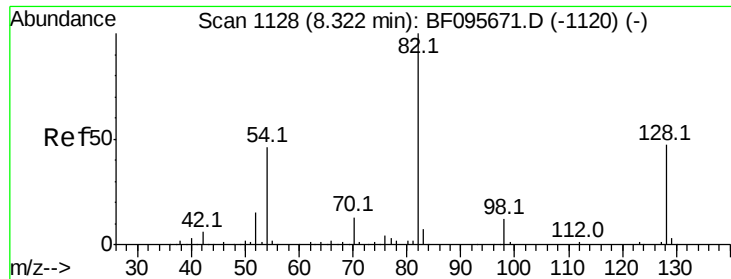

#23
 Nitrobenzene-d5
 Concen: 94.63 ng
 RT: 8.24 min Scan# 1131
 Delta R.T. -0.01 min
 Lab File: BF095963.D
 Acq: 16 Jun 2017 19:13




Instrument :
 BNA_F
 ClientSampleId :
 SB-09-6-7


Tot Ion: 82 Resp: 385814
 Ion Ratio Lower Upper
 82 100
 128 47.9 34.0 51.0
 54 48.3 42.2 63.2

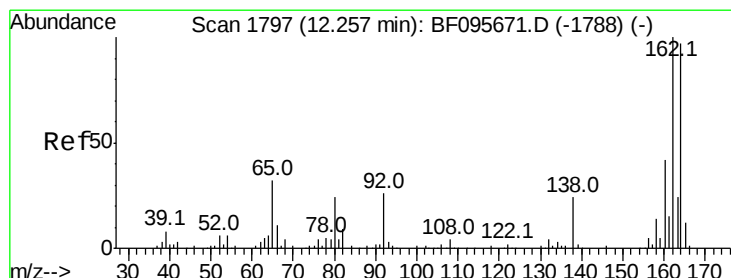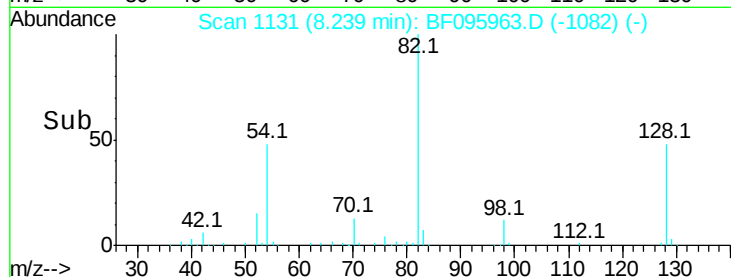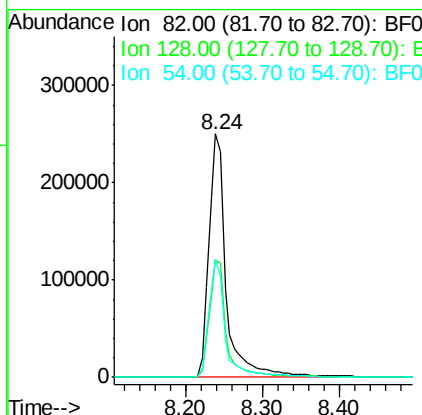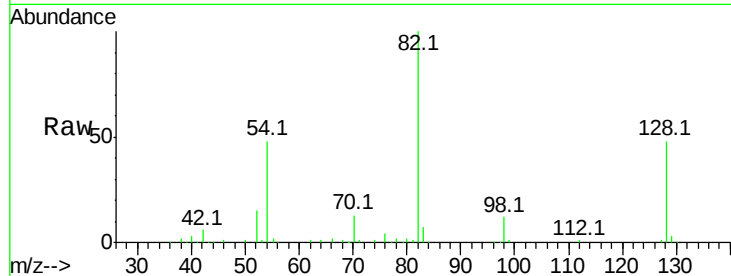

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 12.17 min Scan# 1799
 Delta R.T. -0.01 min
 Lab File: BF095963.D
 Acq: 16 Jun 2017 19:13

Tgt Ion:164 Resp: 112425
 Ion Ratio Lower Upper
 164 100
 162 107.1 82.6 123.8
 160 45.1 36.2 54.2

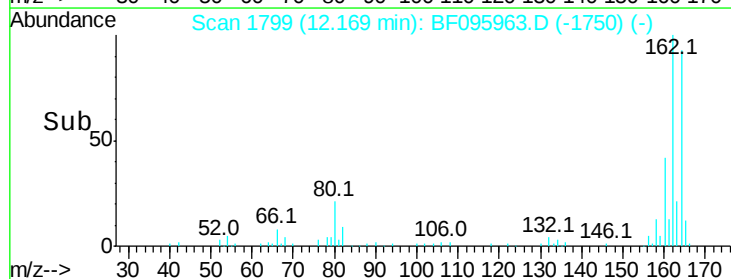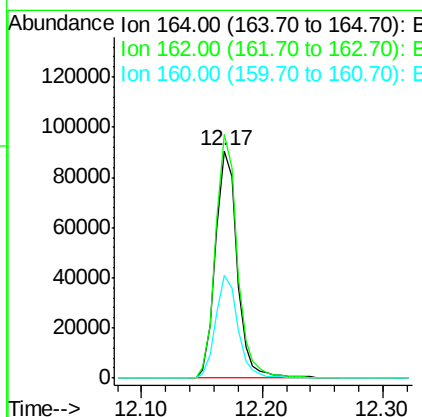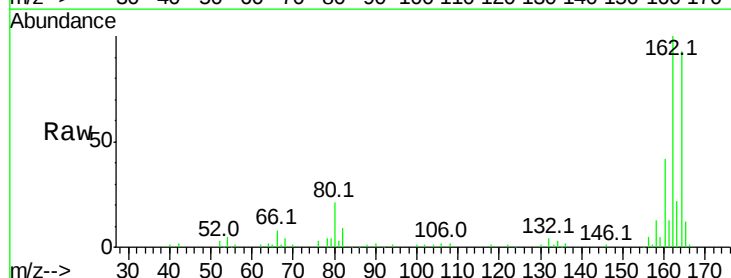


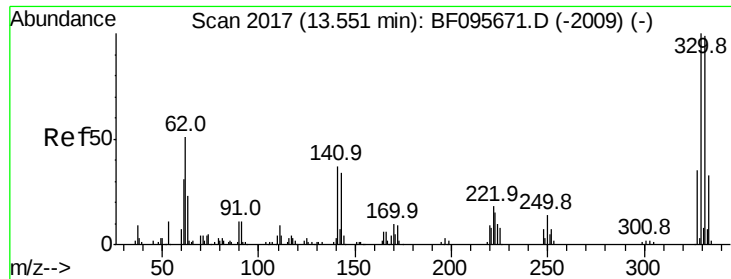




#41
 2,4,6-Tribromophenol
 Concen: 134.13 ng
 RT: 13.47 min Scan# 2020
 Delta R.T. -0.01 min
 Lab File: BF095963.D
 Acq: 16 Jun 2017 19:13

Instrument :
 BNA_F
 ClientSampleId :
 SB-09-6-7

Tot Ion:330 Resp: 133415
 Ion Ratio Lower Upper
 330 100
 332 97.8 76.6 115.0
 141 37.7 31.4 47.2

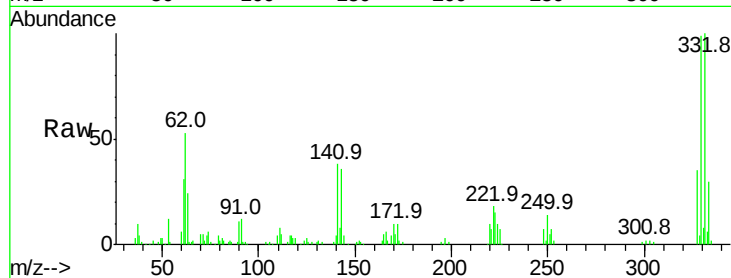


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

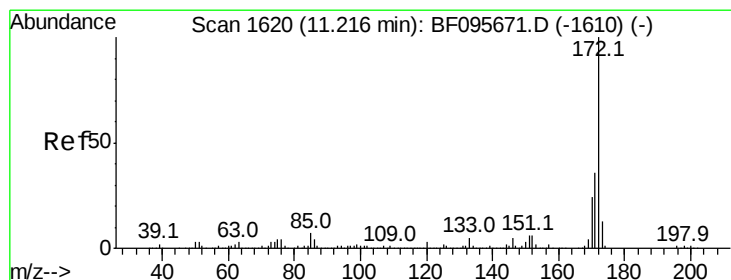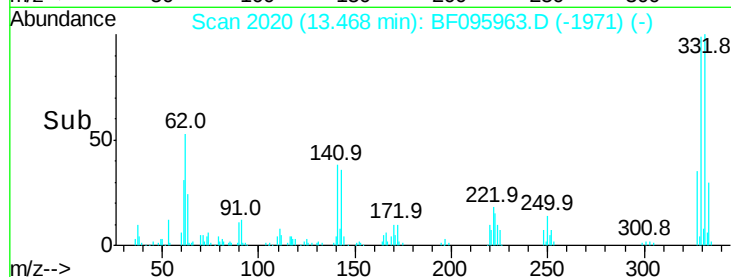
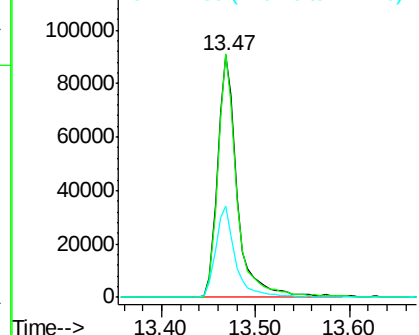



#44
 2-Fluorobiphenyl
 Concen: 83.49 ng
 RT: 11.13 min Scan# 1623
 Delta R.T. -0.01 min
 Lab File: BF095963.D
 Acq: 16 Jun 2017 19:13

Tgt Ion:172 Resp: 674541
 Ion Ratio Lower Upper
 172 100
 171 35.9 29.6 44.4
 170 23.4 19.8 29.8

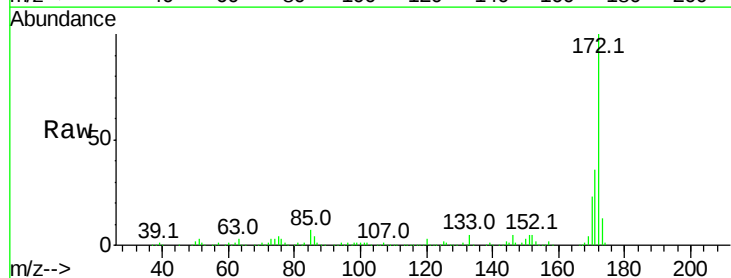

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

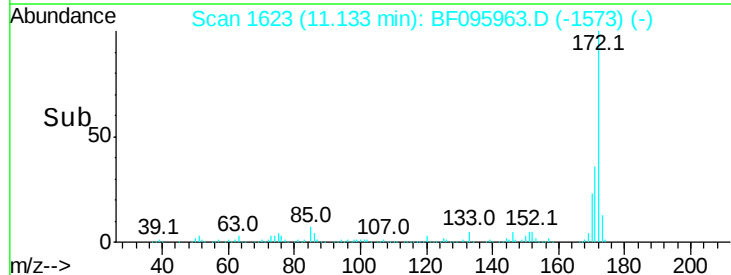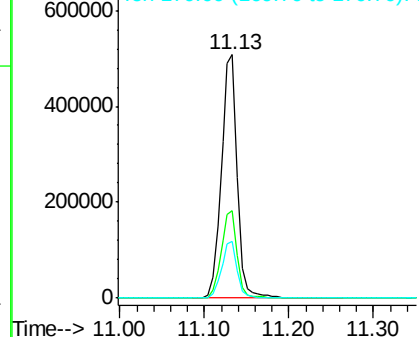

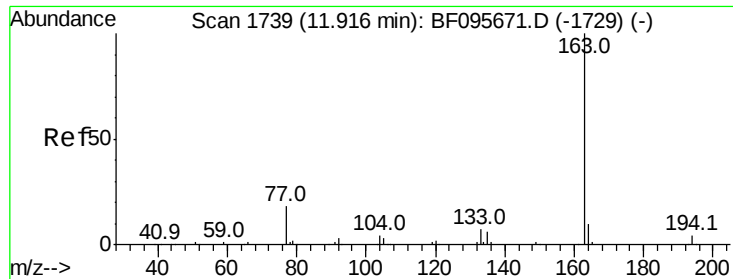

#49

Dimethylphthalate

Concen: 15.25 ng

RT: 11.83 min Scan# 1741

Delta R.T. -0.02 min

Lab File: BF095963.D

Acq: 16 Jun 2017 19:13

Instrument :

BNA_F

ClientSampleId :

SB-09-6-7


Tot Ion:163 Resp: 130135

Ion Ratio Lower Upper

163 100

194 3.0 2.6 4.0




164 10.3 8.4 12.6

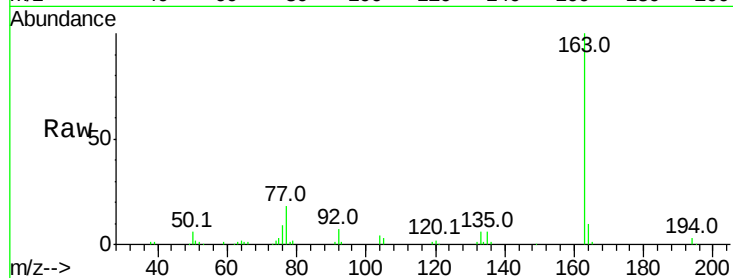

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

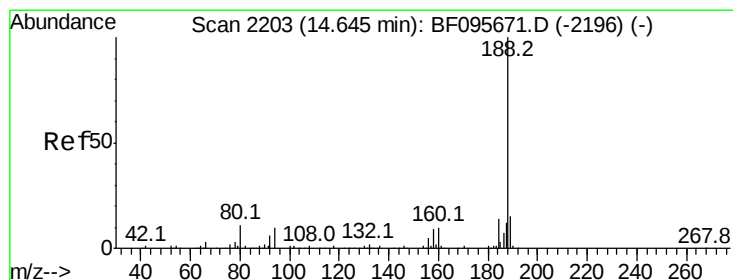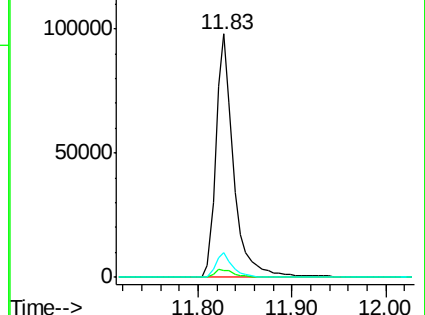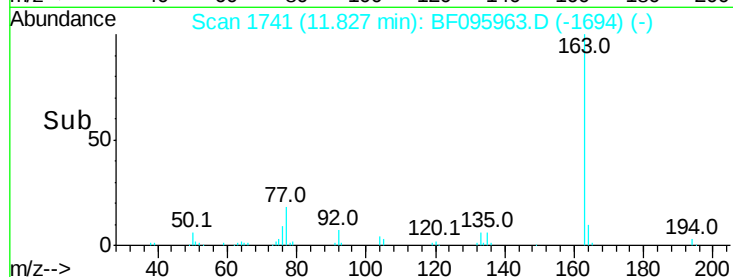

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 14.56 min Scan# 2206

Delta R.T. -0.01 min

Lab File: BF095963.D

Acq: 16 Jun 2017 19:13


Tgt Ion:188 Resp: 190382

Ion Ratio Lower Upper

188 100

94 10.4 9.4 14.2



80 11.9 10.2 15.2

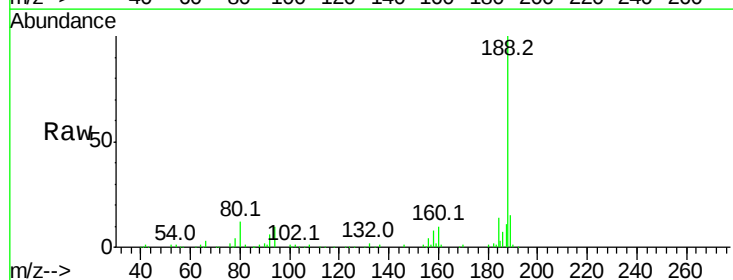


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

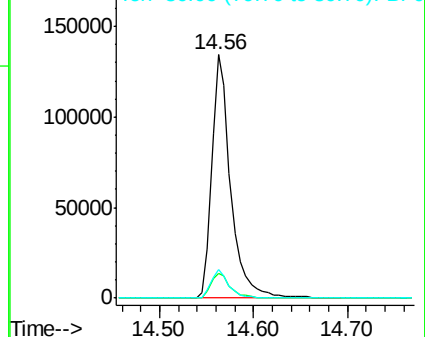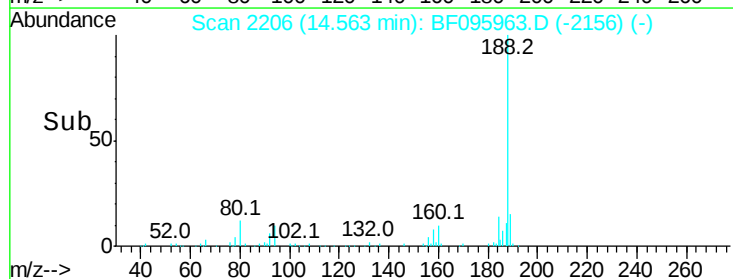


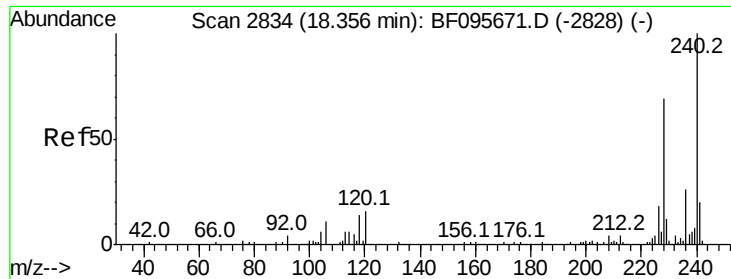




#75
 Chrysene-d12
 Concen: 20.00 ng
 RT: 18.29 min Scan# 2840
 Delta R.T. -0.01 min
 Lab File: BF095963.D
 Acq: 16 Jun 2017 19:13

Instrument :
 BNA_F
 ClientSampleId :
 SB-09-6-7

Tot Ion:240 Resp: 126481
 Ion Ratio Lower Upper
 240 100
 120 14.0 5.8 8.8#
 236 25.1 20.5 30.7

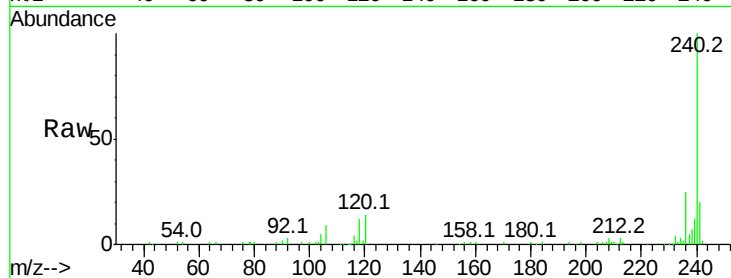


Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

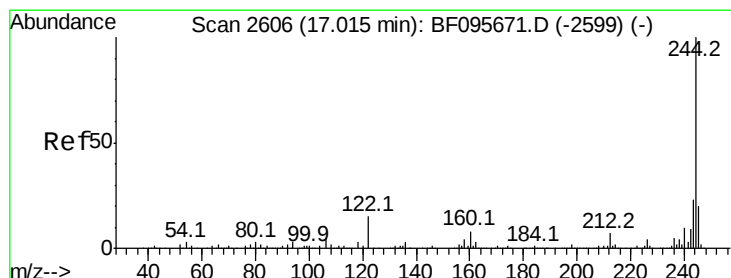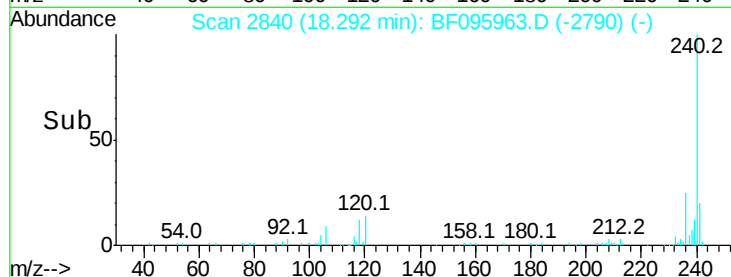
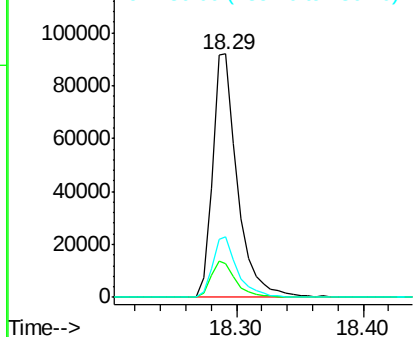



#78
 Terphenyl-d14
 Concen: 86.77 ng
 RT: 16.94 min Scan# 2611
 Delta R.T. -0.01 min
 Lab File: BF095963.D
 Acq: 16 Jun 2017 19:13

Tgt Ion:244 Resp: 442205
 Ion Ratio Lower Upper
 244 100
 212 6.8 6.0 9.0
 122 13.4 10.3 15.5

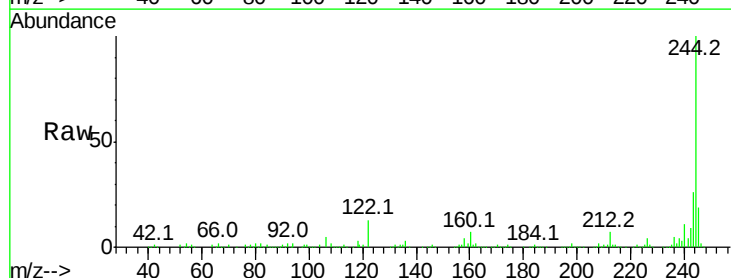

Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

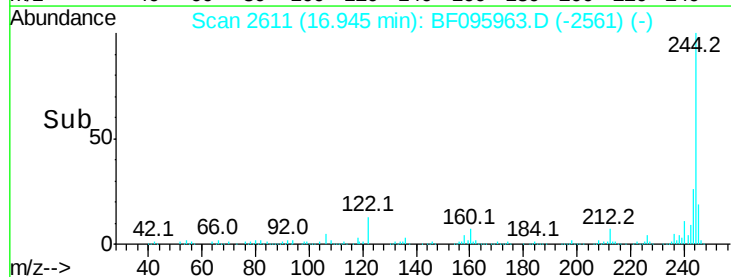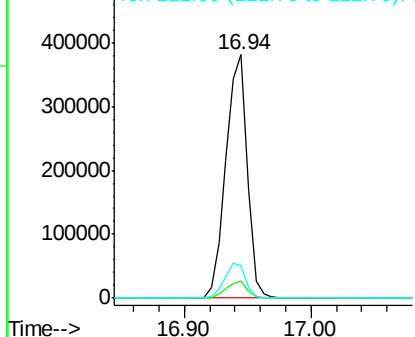

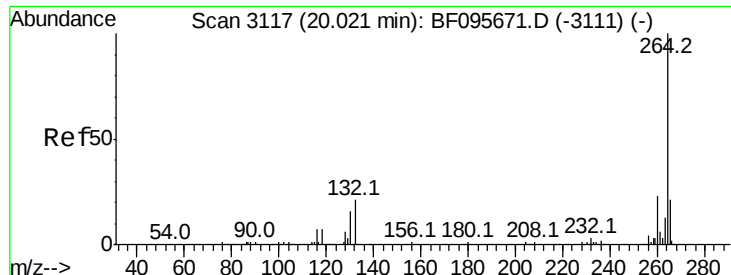

#86
 Pervlene-d12
 Concen: 20.00 ng
 RT: 19.96 min Scan# 3123
 Delta R.T. -0.01 min
 Lab File: BF095963.D
 Acq: 16 Jun 2017 19:13

Instrument :
 BNA_F
 ClientSampleId :
 SB-09-6-7

Tot Ion:	264	Resp:	123659
Ion	Ratio	Lower	Upper
264	100		
260	23.5	19.5	29.3
265	21.6	17.2	25.8

