

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061617\
 Data File : BF095961.D
 Acq On : 16 Jun 2017 18:09
 Operator : SJ/MA
 Sample : PB99832BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB99832BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.534	497	501	519	rBV	60572	170933	8.34%	1.171%
2	5.228	615	619	647	rBV	835228	1647052	80.40%	11.283%
3	6.898	899	903	913	rBV	1029644	1504053	73.42%	10.303%
4	6.981	913	917	937	rVB	1239449	1930796	94.25%	13.226%
5	7.322	971	975	989	rVB	248521	333635	16.29%	2.285%
6	7.557	1010	1015	1034	rBV	1036413	1357639	66.27%	9.300%
7	8.239	1126	1131	1162	rBV	694237	1018957	49.74%	6.980%
8	9.351	1316	1320	1337	rBV	331405	460272	22.47%	3.153%
9	11.133	1616	1623	1638	rBV	1598699	2048553	100.00%	14.033%
10	12.169	1795	1799	1813	rBV2	371106	503447	24.58%	3.449%
11	13.468	2015	2020	2037	rBV	698960	999466	48.79%	6.847%
12	14.562	2202	2206	2223	rBV2	315241	453940	22.16%	3.110%
13	16.945	2605	2611	2626	rBB	1337959	1517775	74.09%	10.397%
14	18.292	2836	2840	2850	rBV	239266	319658	15.60%	2.190%
15	19.956	3119	3123	3137	rBV2	230788	331783	16.20%	2.273%


Sum of corrected areas: 14597959

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061617\
Data File : BF095961.D
Acq On : 16 Jun 2017 18:09
Operator : SJ/MA
Sample : PB99832BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB99832BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

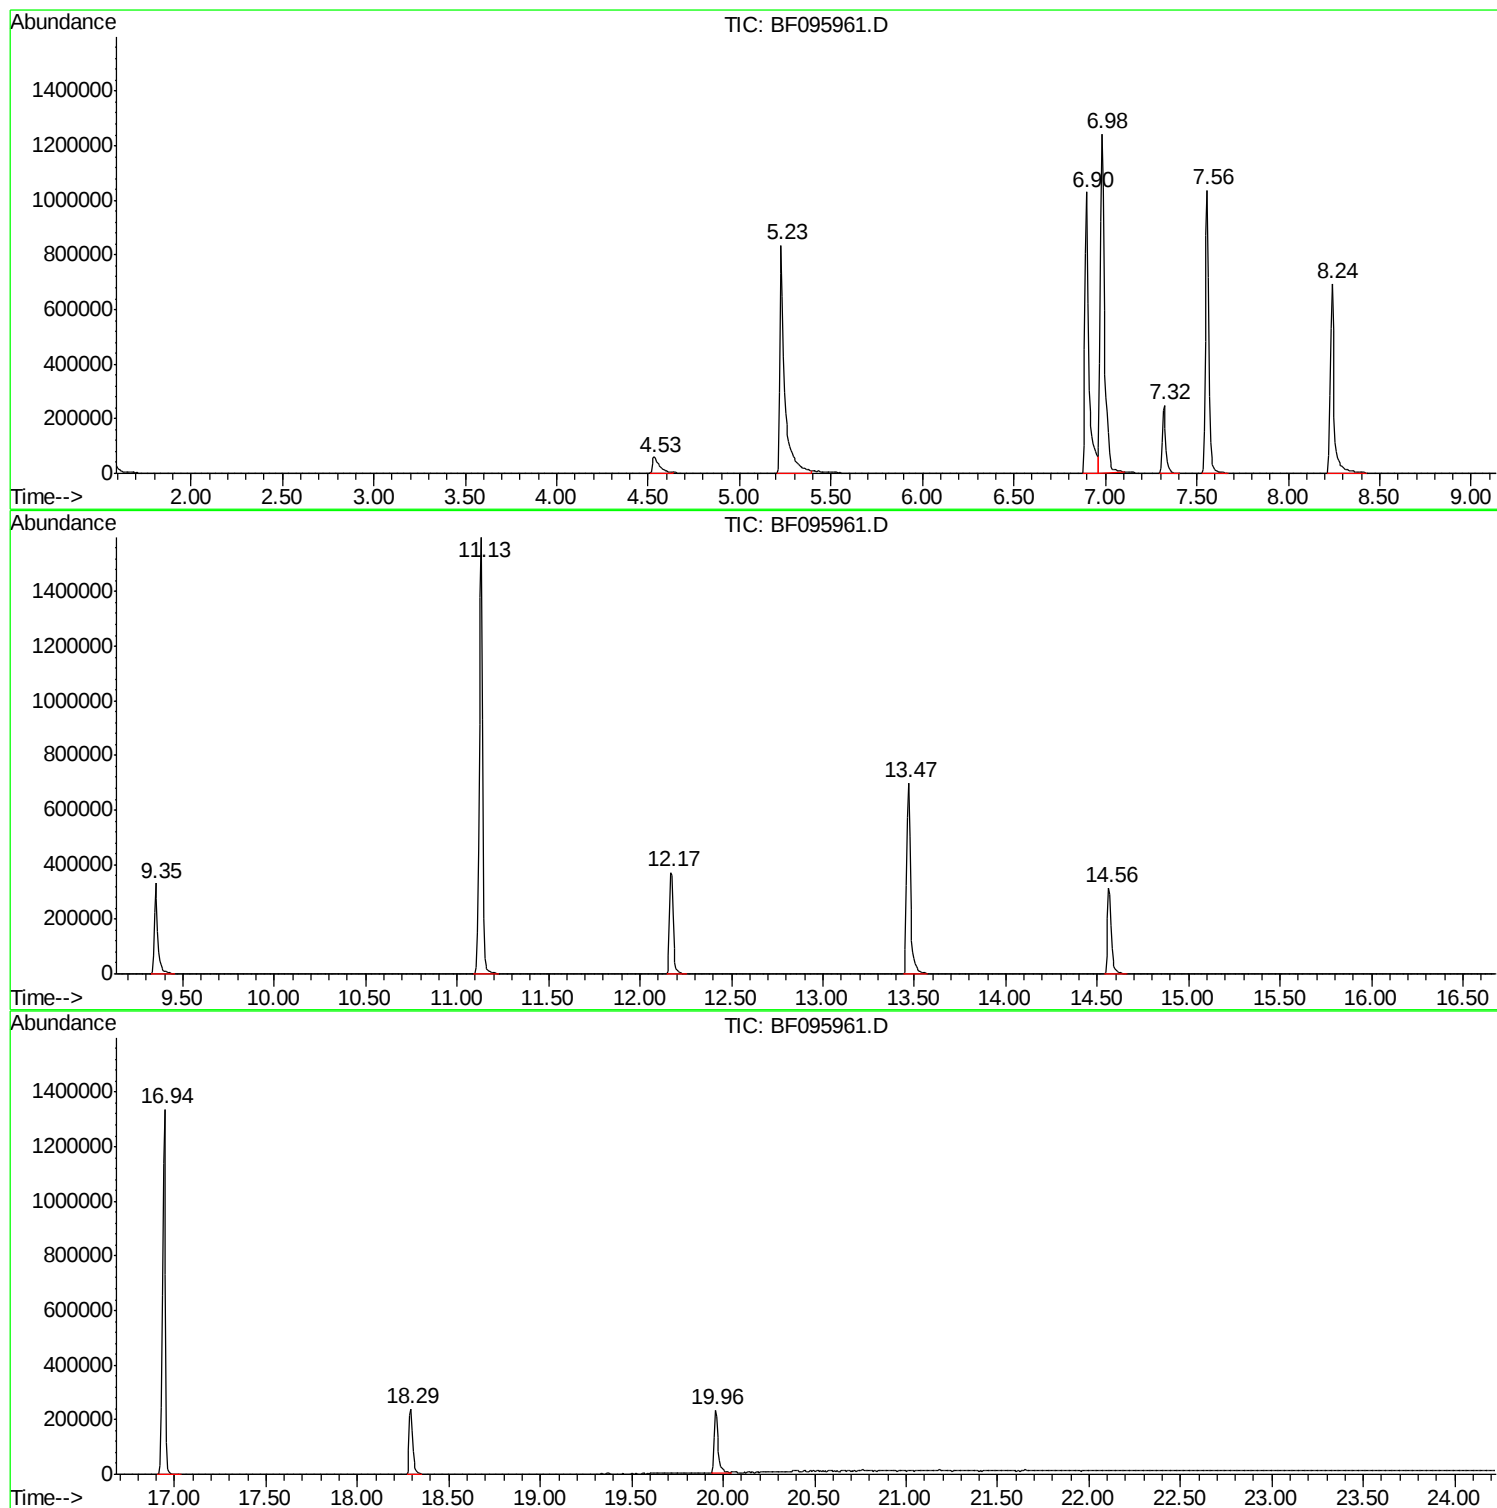

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061617\
Data File : BF095961.D
Acq On : 16 Jun 2017 18:09
Operator : SJ/MA
Sample : PB99832BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :
PB99832BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.53	10.25 ng	170933	1,4-Dichlorobenzene-d4	7.32

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2			1,8-Nonanediol, 8-methyl-	174	C10H22O2	054725-73-4	25
3			5-Hexen-2-one	98	C6H10O	000109-49-9	9
4			Butane	58	C4H10	000106-97-8	9
5			3-Hexanol	102	C6H14O	000623-37-0	9

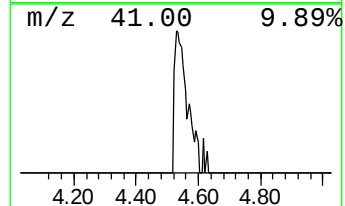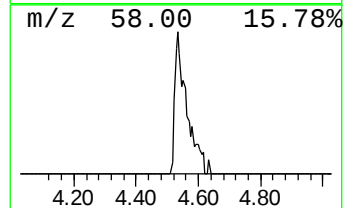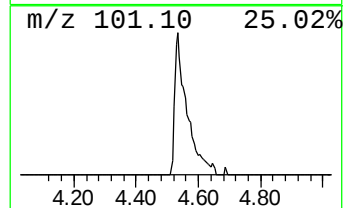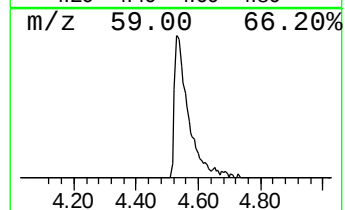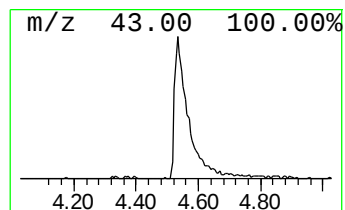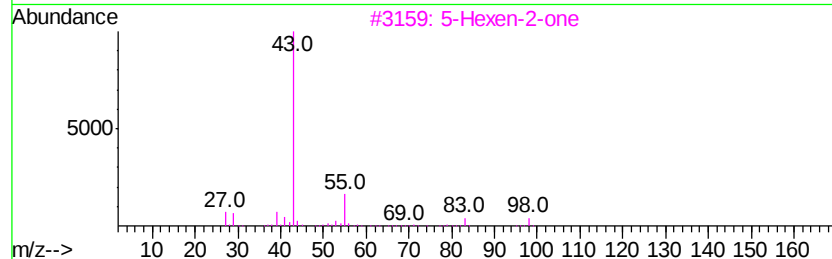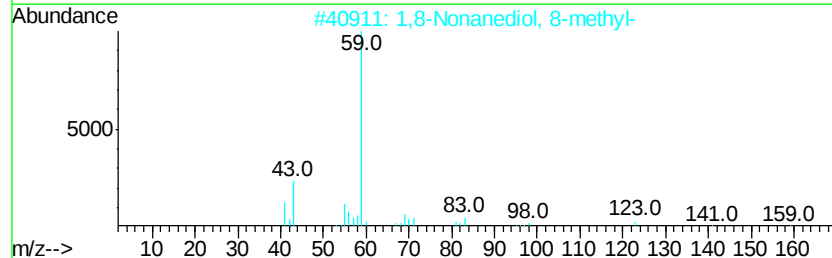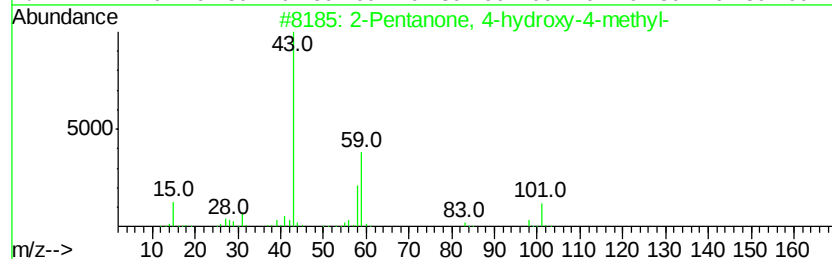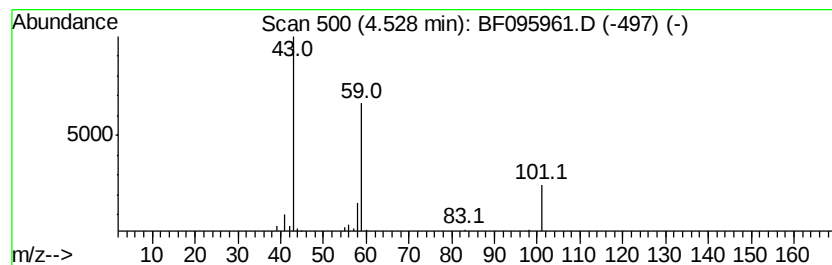

Data Path : Z:\HPCHEM1\BNA F\DATA\BF061617\
Data File : BF095961.D
Acq On : 16 Jun 2017 18:09
Operator : SJ/MA
Sample : PB99832BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB99832BL









Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.98 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.98	115.74 ng	1930800	1,4-Dichlorobenzene-d4	7.32

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	27
2	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
3	5-Aminoindole	132	C8H8N2	005192-03-0	12
4	Amphetaminil	250	C17H18N2	017590-01-1	10
5	Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10

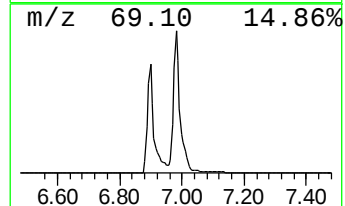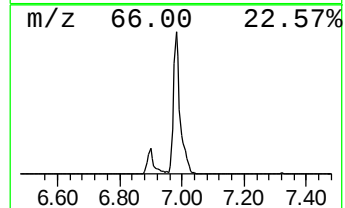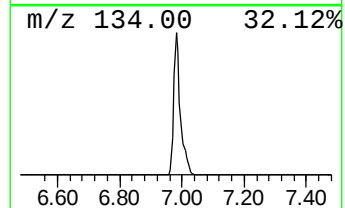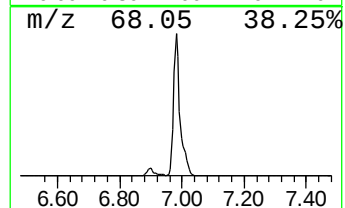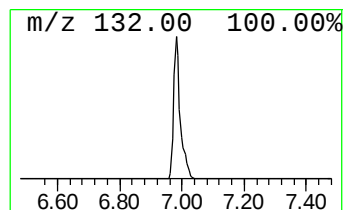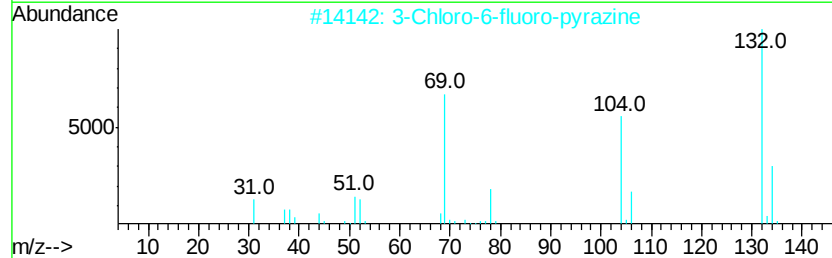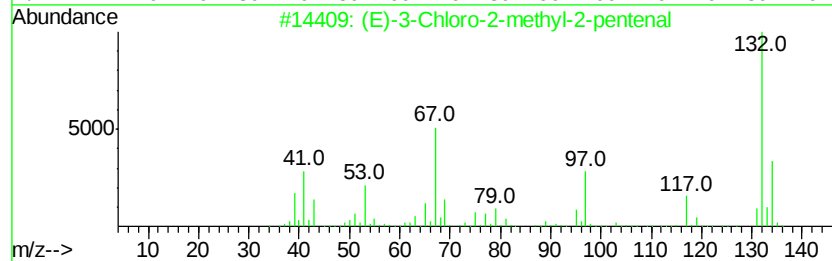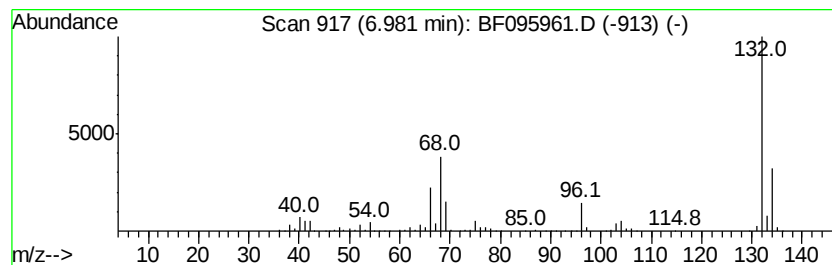

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061617\
Data File : BF095961.D
Acq On : 16 Jun 2017 18:09
Operator : SJ/MA
Sample : PB99832BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB99832BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.53	10.3	ng	170933	1	7.32	333635	20.0
unknown6.98	6.98	115.7	ng	1930800	1	7.32	333635	20.0