


Data Path : Z:\HPCHEM1\BNA F\Data\BF061617\
 Data File : BF095950.D
 Acq On : 16 Jun 2017 12:07
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 16 17:12:03 2017

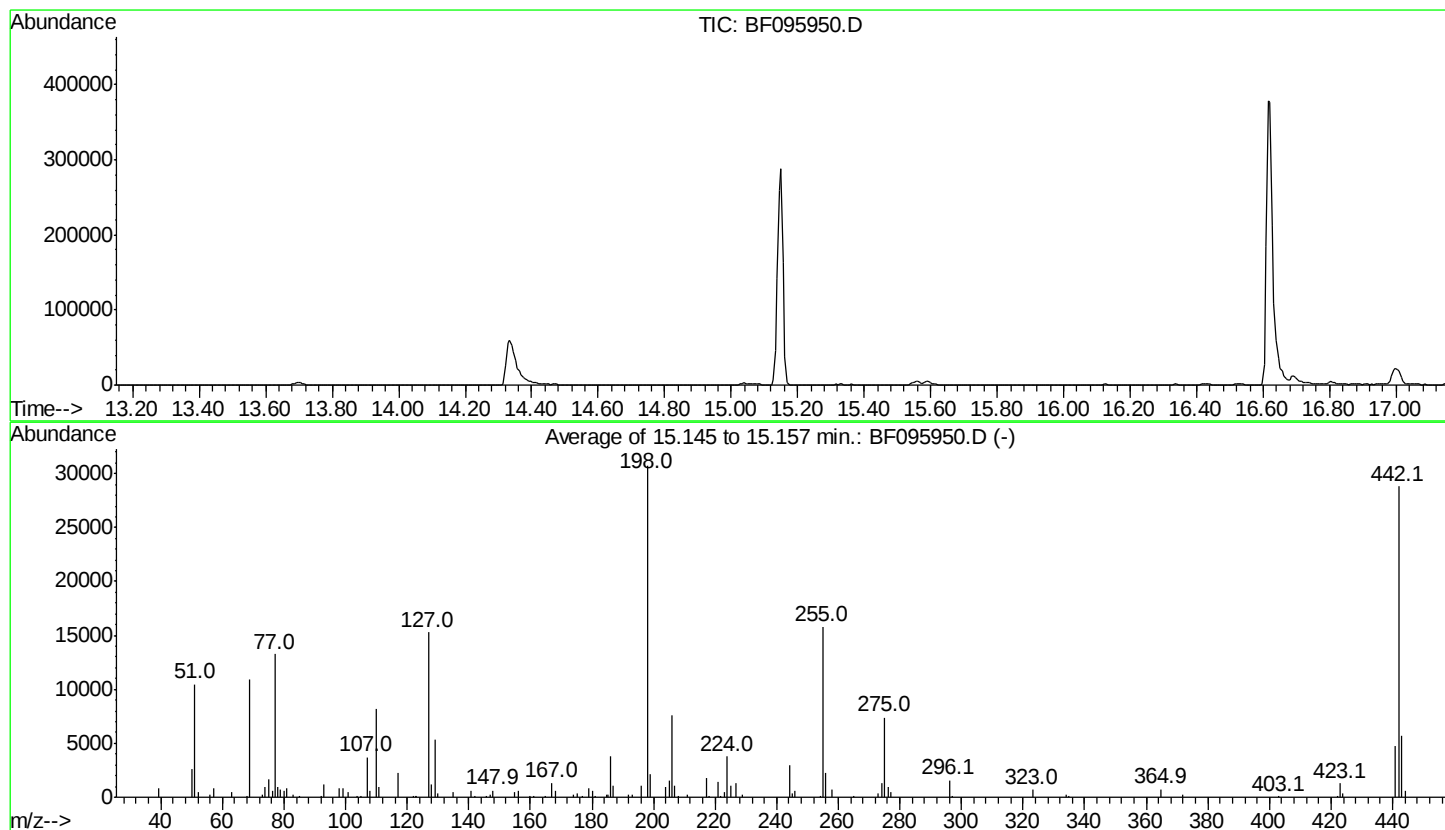

AutoFind: Scans 2305, 2306, 2307; Background Corrected with Scan 2299

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.2	10501	PASS
68	69	0.00	2	0.9	100	PASS
69	198	0.00	100	35.4	10871	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.7	15288	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	30741	PASS
199	198	5	9	7.0	2145	PASS
275	198	10	60	24.1	7404	PASS
365	198	1	100	2.4	727	PASS
441	442	0.01	24	16.6	4774	PASS
442	198	50	100	93.7	28805	PASS
443	442	15	24	19.9	5739	PASS