


Data Path : Z:\HPCHEM1\BNA_F\Data\BF061617\
 Data File : BF095973.D
 Acq On : 17 Jun 2017 1:24
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 16 17:12:03 2017

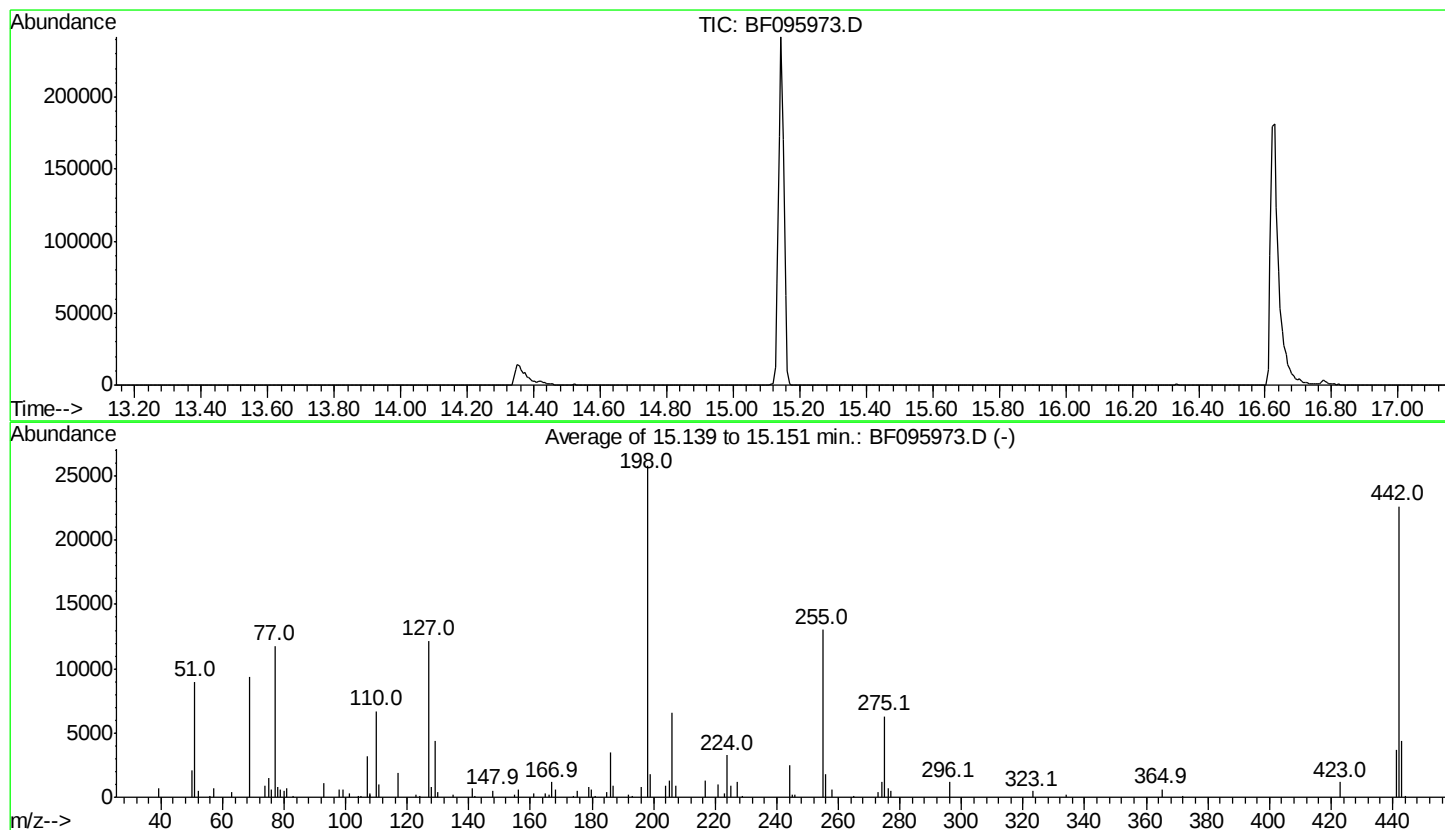

AutoFind: Scans 2304, 2305, 2306; Background Corrected with Scan 2298

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.9	8998	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.3	9377	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.1	12160	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	25805	PASS
199	198	5	9	7.0	1811	PASS
275	198	10	60	24.5	6327	PASS
365	198	1	100	2.4	619	PASS
441	442	0.01	24	16.1	3649	PASS
442	198	50	100	87.8	22654	PASS
443	442	15	24	19.5	4412	PASS