
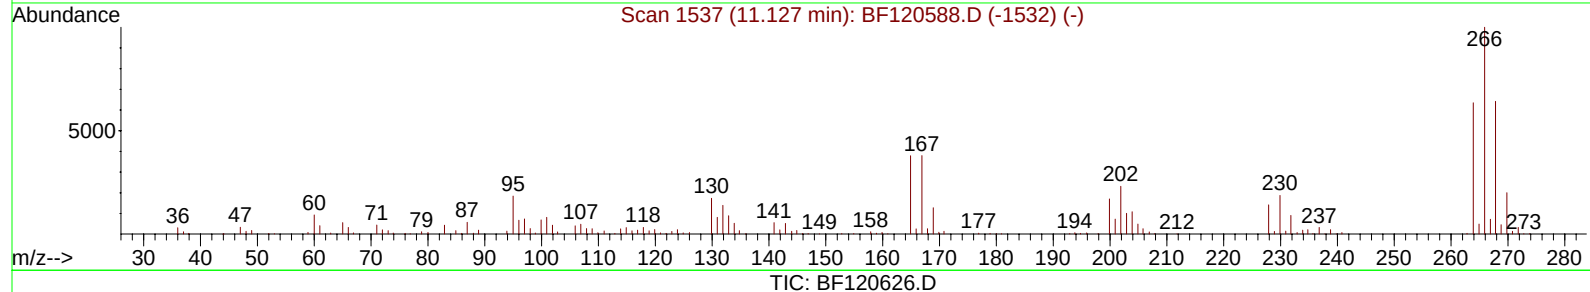
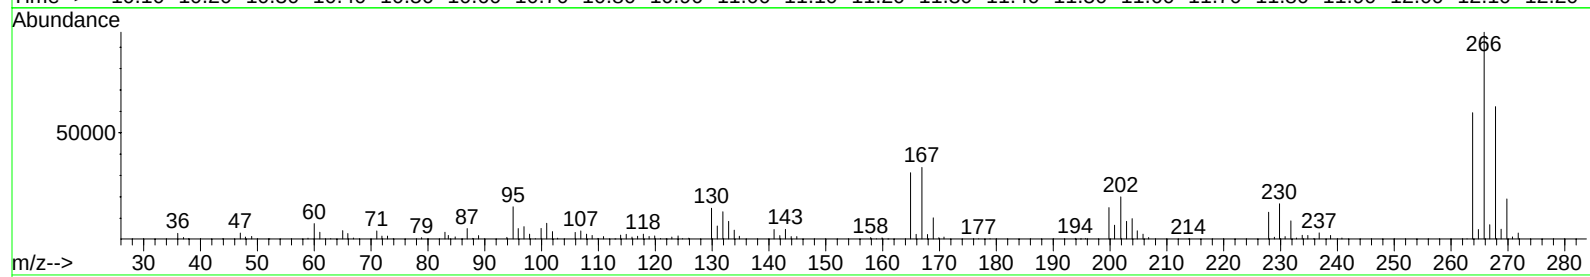


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061620\
 Data File : BF120626.D
 Acq On : 16 Jun 2020 7:53
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 16 17:42:33 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 11 11:28:22 2020
 Response via : Initial Calibration

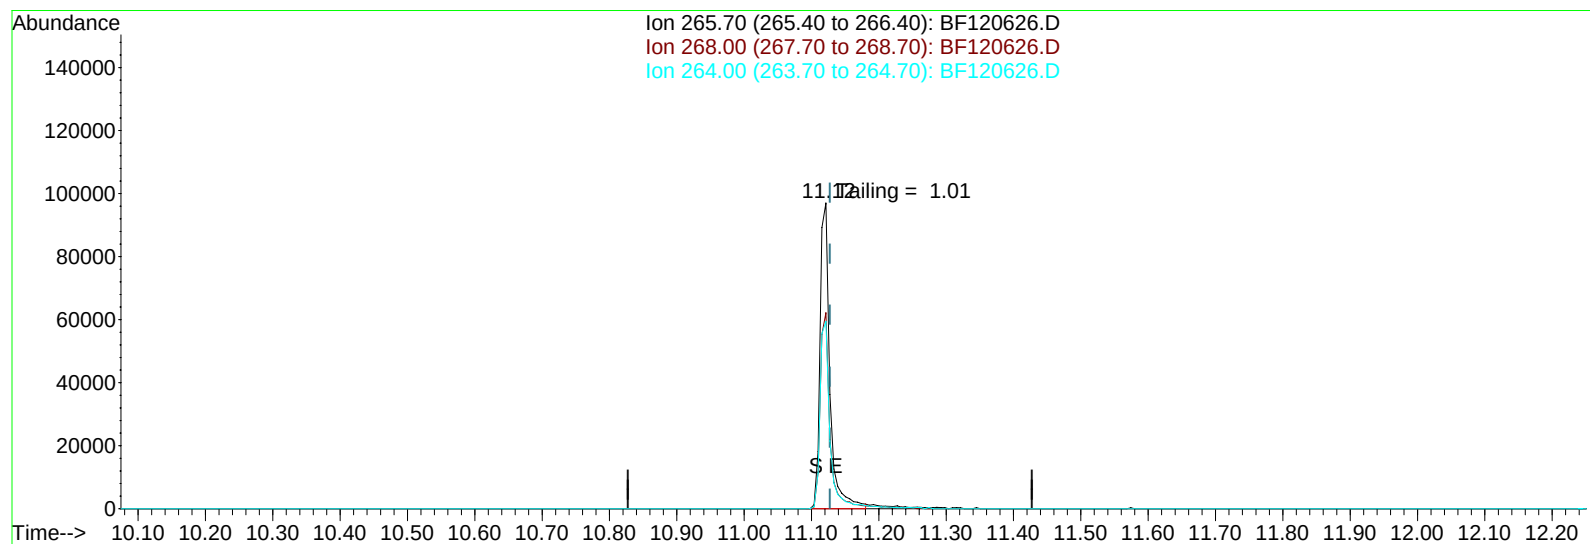

(70) Pentachlorophenol (C)




11.121min (-0.006) 25774.40ng

response 102463

Ion	Exp%	Act%
265.70	100	100
268.00	64.20	64.12
264.00	63.50	61.22
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061620\
 Data File : BF120626.D
 Acq On : 16 Jun 2020 7:53
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 16 17:42:33 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 11 11:28:22 2020
 Response via : Initial Calibration

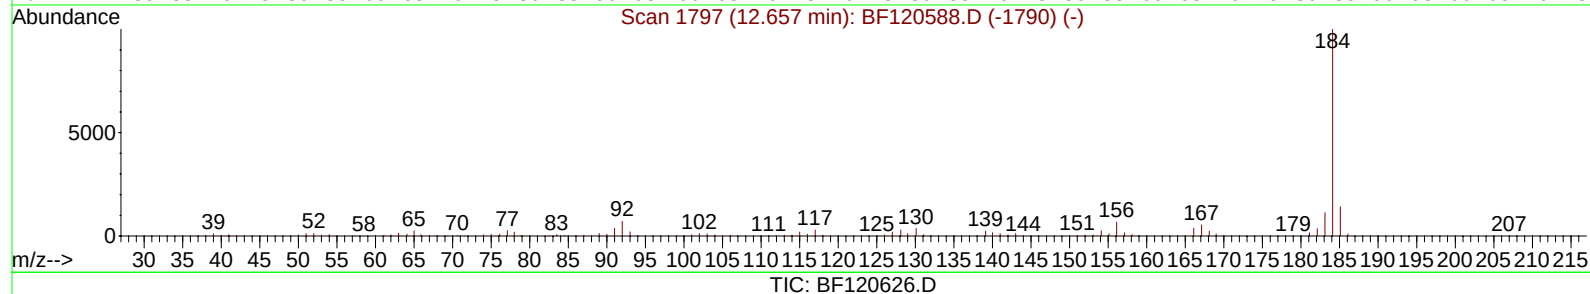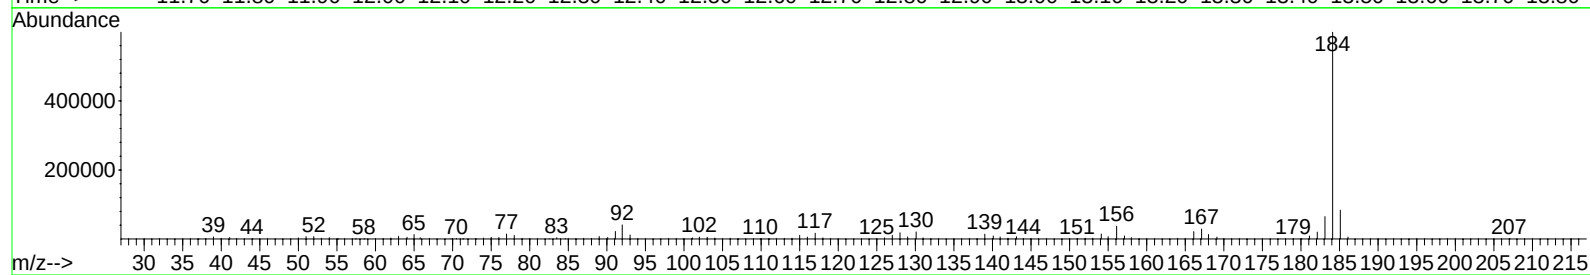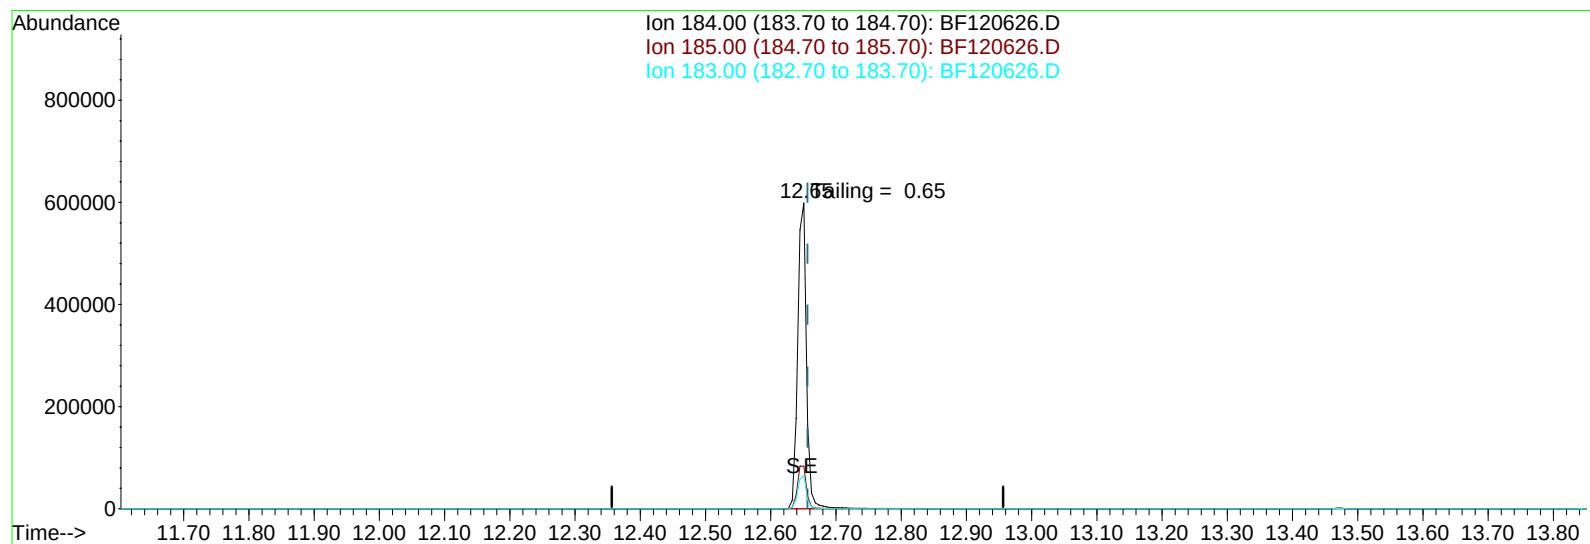

(77) Benzidine

12.651min (-0.006) 30625.18ng

response 559291

Ion	Exp%	Act%
184.00	100	100
185.00	14.20	13.94
183.00	11.30	10.87
0.00	0.00	0.00