
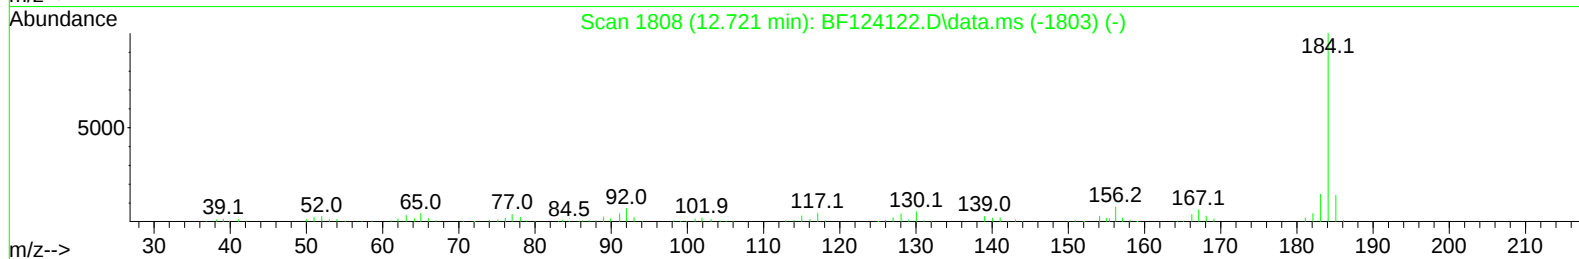
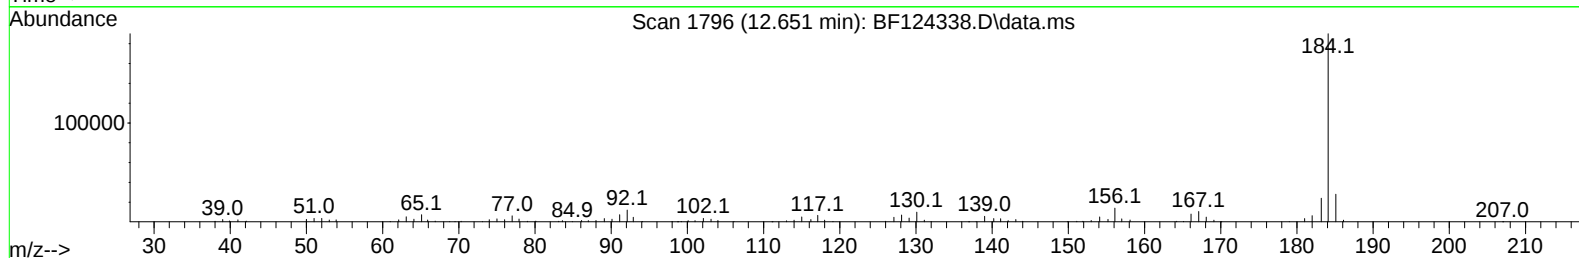


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061621\
Data File : BF124338.D
Acq On : 16 Jun 2021 9:55
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 16 11:05:22 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 15 20:09:26 2021
Response via : Initial Calibration

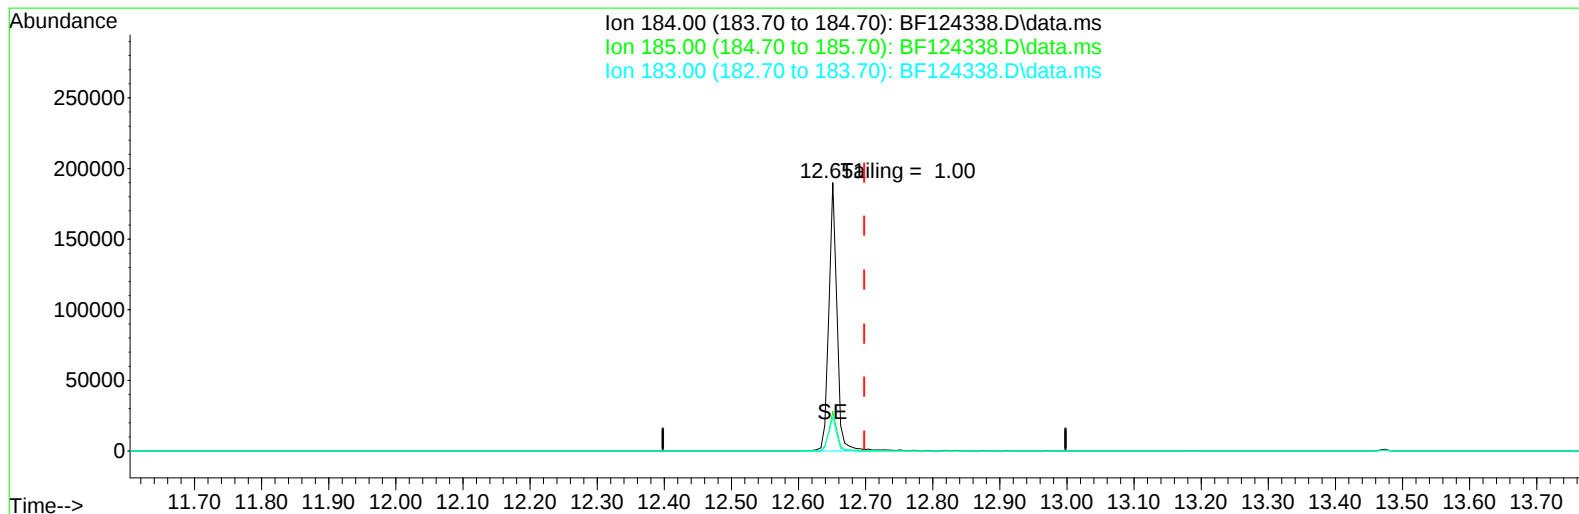

TIC: BF124338.D\data.ms

(77) Benzidine




12.651min (-0.047) 0.00 ng

response 160899

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.77
183.00	9.80	12.69#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061621\
Data File : BF124338.D
Acq On : 16 Jun 2021 9:55
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 16 11:05:22 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 15 20:09:26 2021
Response via : Initial Calibration

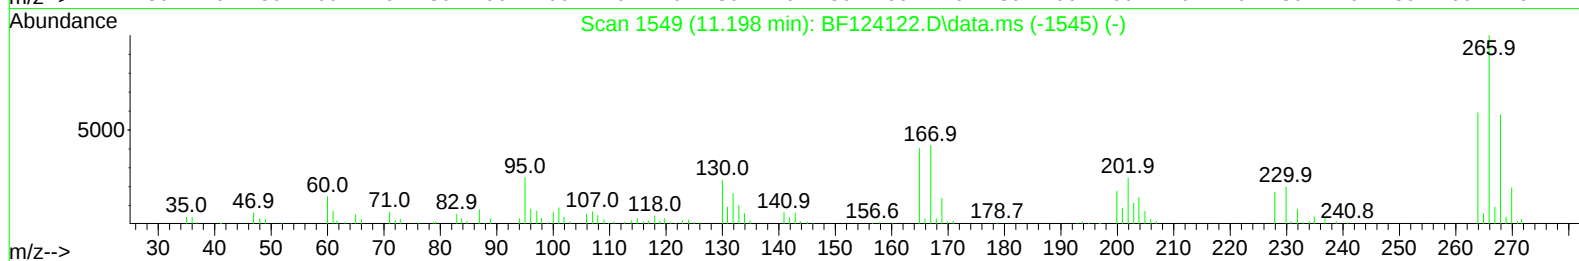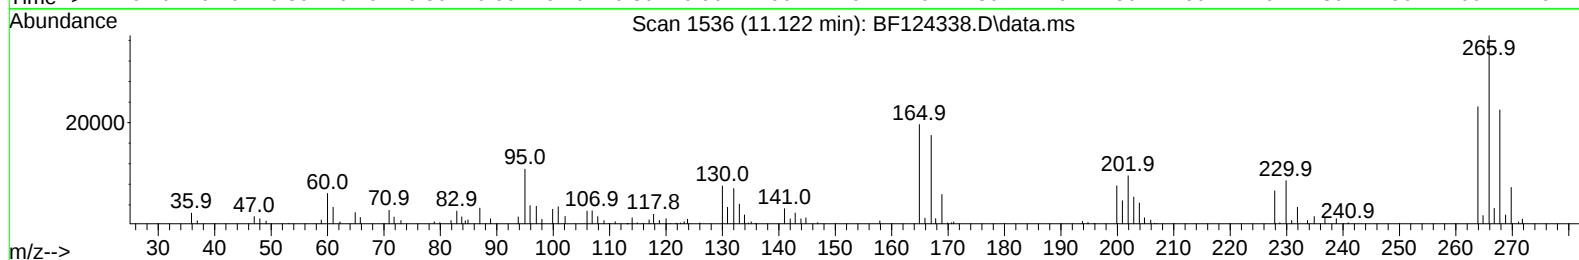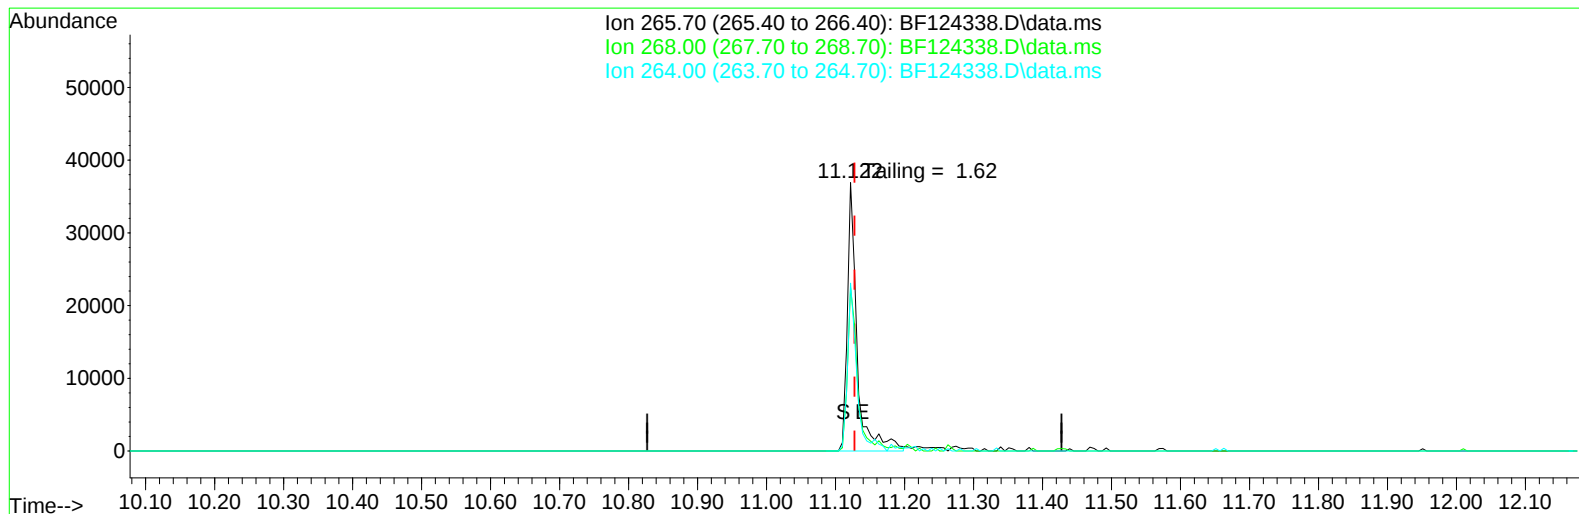

TIC: BF124338.D\data.ms

(70) Pentachlorophenol (C)

11.122min (-0.006) 33184.95 ng

response 35216

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	60.86
264.00	65.70	62.53
0.00	0.00	0.00