
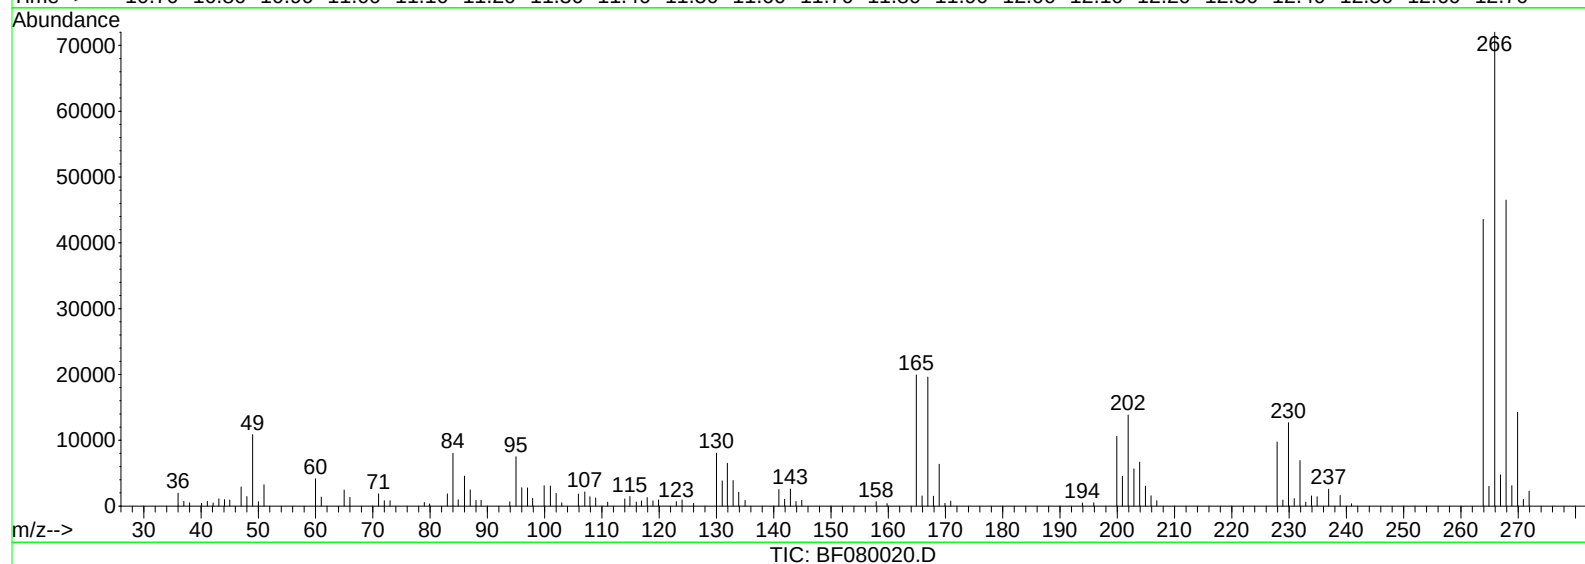


Data Path : Z:\HPCHEM1\BNA F\Data\BF061715\
Data File : BF080020.D
Acq On : 17 Jun 2015 11:31
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 17 17:14:24 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 17 16:41:53 2015
Response via : Initial Calibration

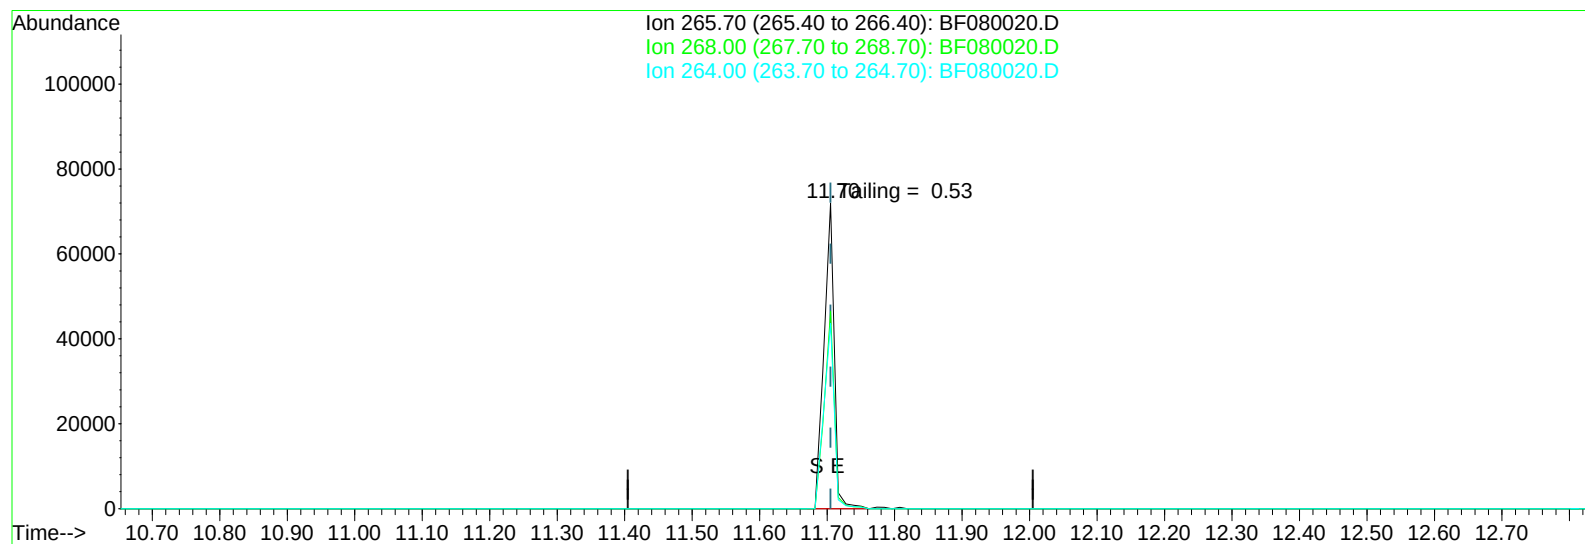

(69) Pentachlorophenol (C)



11.705min (+0.000) 51995.65ng

response 76253

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	64.56
264.00	62.70	60.50
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF061715\
 Data File : BF080020.D
 Acq On : 17 Jun 2015 11:31
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 17 17:14:24 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF061715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 17 16:41:53 2015
 Response via : Initial Calibration

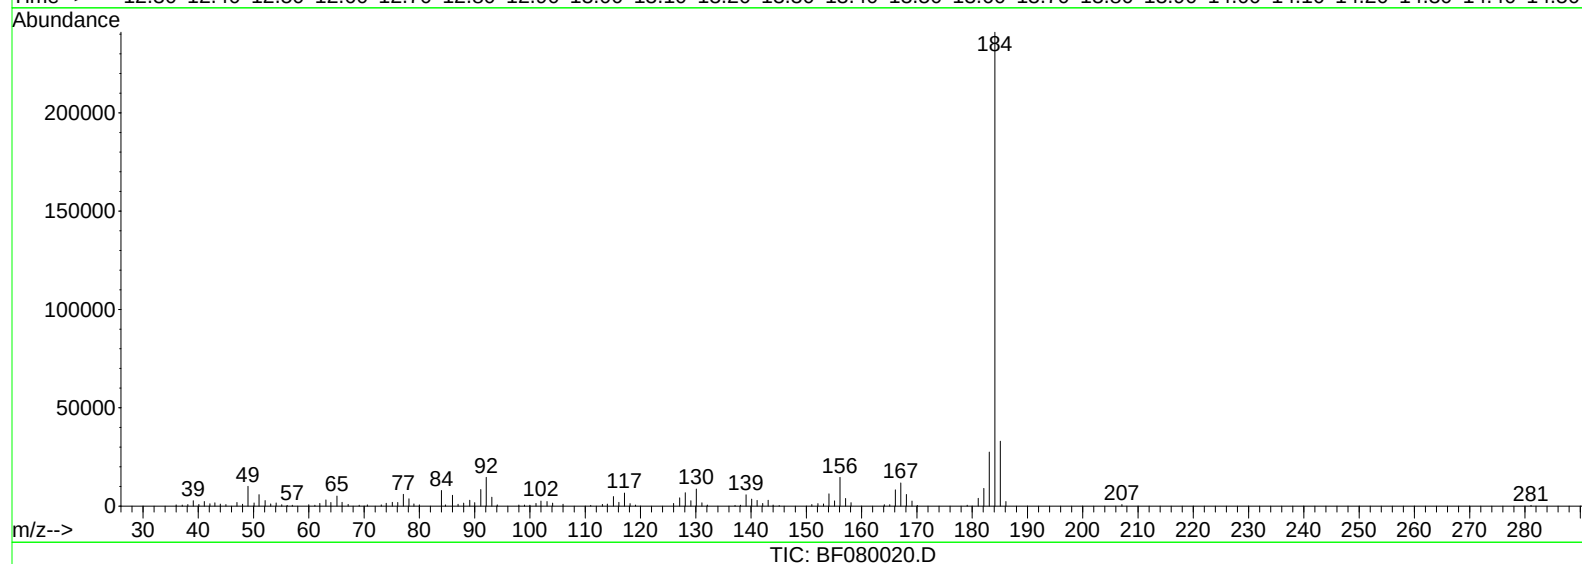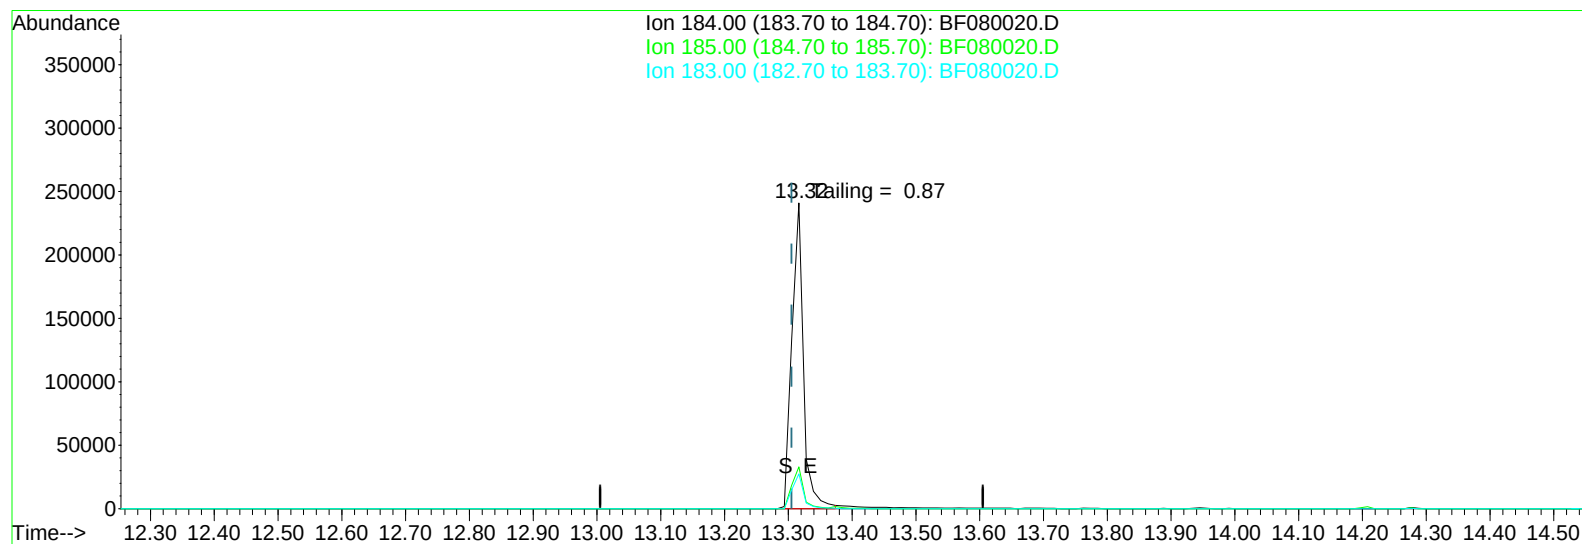

(76) Benzidine

13.317min (+0.012) 0.00ng

response 313762

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	13.69
183.00	9.50	11.40#
0.00	0.00	0.00