


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061715\
Data File : BF080020.D
Acq On : 17 Jun 2015 11:31
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jun 17 16:41:53 2015

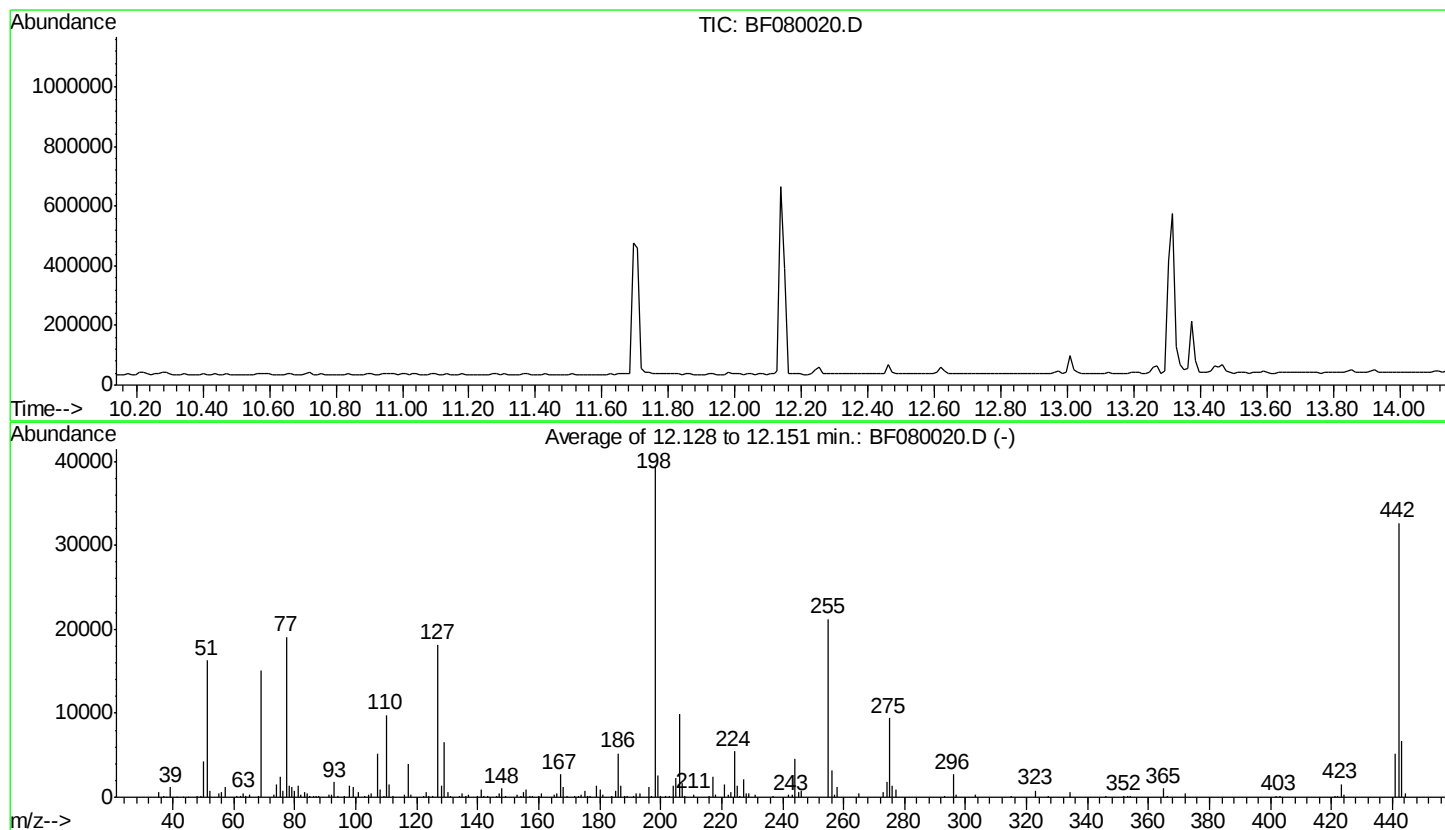

AutoFind: Scans 791, 792, 793; Background Corrected with Scan 788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.2	16276	PASS
68	69	0.00	2	1.4	214	PASS
69	198	0.00	100	38.3	15102	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.0	18142	PASS
197	198	0.00	2	0.3	133	PASS
198	198	100	100	100.0	39472	PASS
199	198	5	9	6.7	2656	PASS
275	198	10	60	23.8	9391	PASS
365	198	1	100	2.6	1025	PASS
441	442	0.01	24	15.9	5188	PASS
442	198	50	100	82.7	32658	PASS
443	442	15	24	20.5	6692	PASS