


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061715\
 Data File : BF080032.D
 Acq On : 17 Jun 2015 19:34
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 17 16:41:53 2015

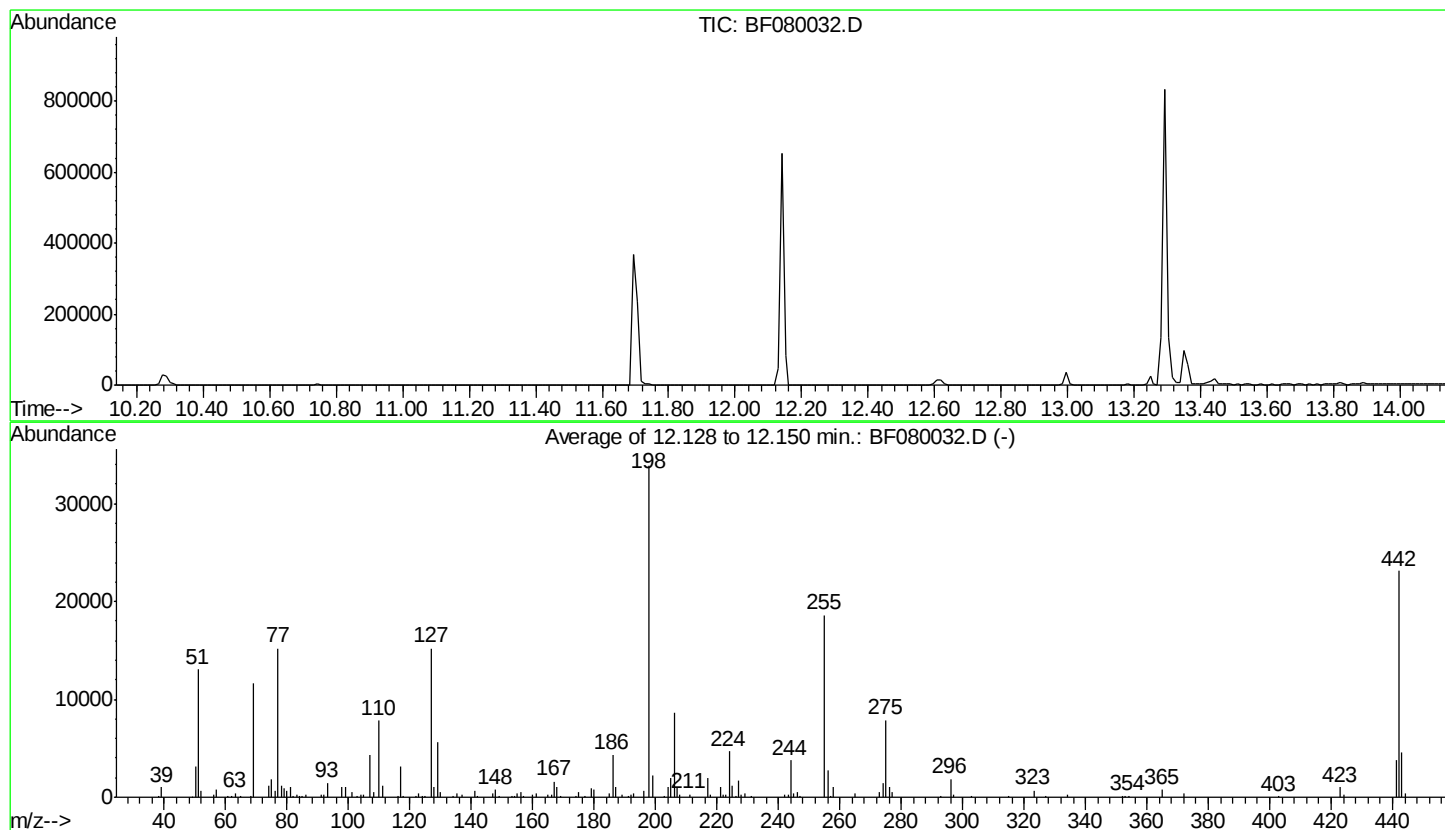

AutoFind: Scans 791, 792, 793; Background Corrected with Scan 788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.5	13037	PASS
68	69	0.00	2	1.5	169	PASS
69	198	0.00	100	34.3	11622	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.0	15241	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	33896	PASS
199	198	5	9	6.5	2194	PASS
275	198	10	60	23.3	7909	PASS
365	198	1	100	2.3	778	PASS
441	442	0.01	24	16.6	3836	PASS
442	198	50	100	68.3	23141	PASS
443	442	15	24	19.6	4533	PASS