
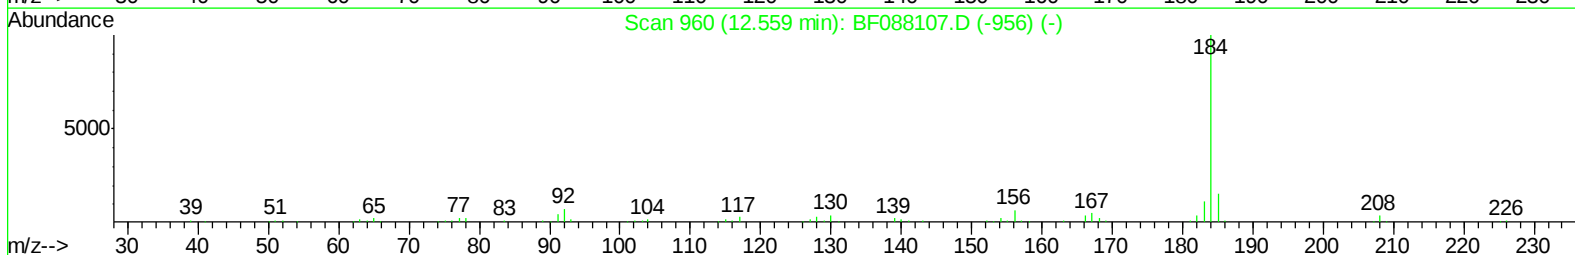
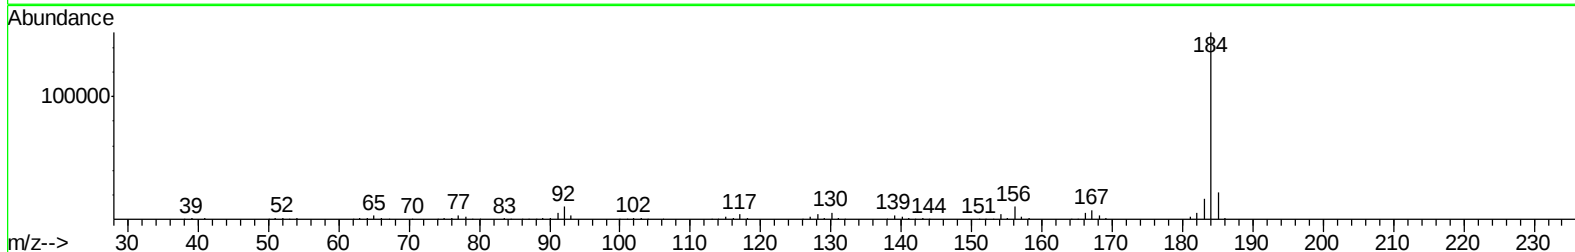


Data Path : Z:\HPCHEM1\BNA_F\Data\BF061716\
 Data File : BF088108.D
 Acq On : 17 Jun 2016 23:15
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 20 07:20:29 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 17 16:09:13 2016
 Response via : Initial Calibration

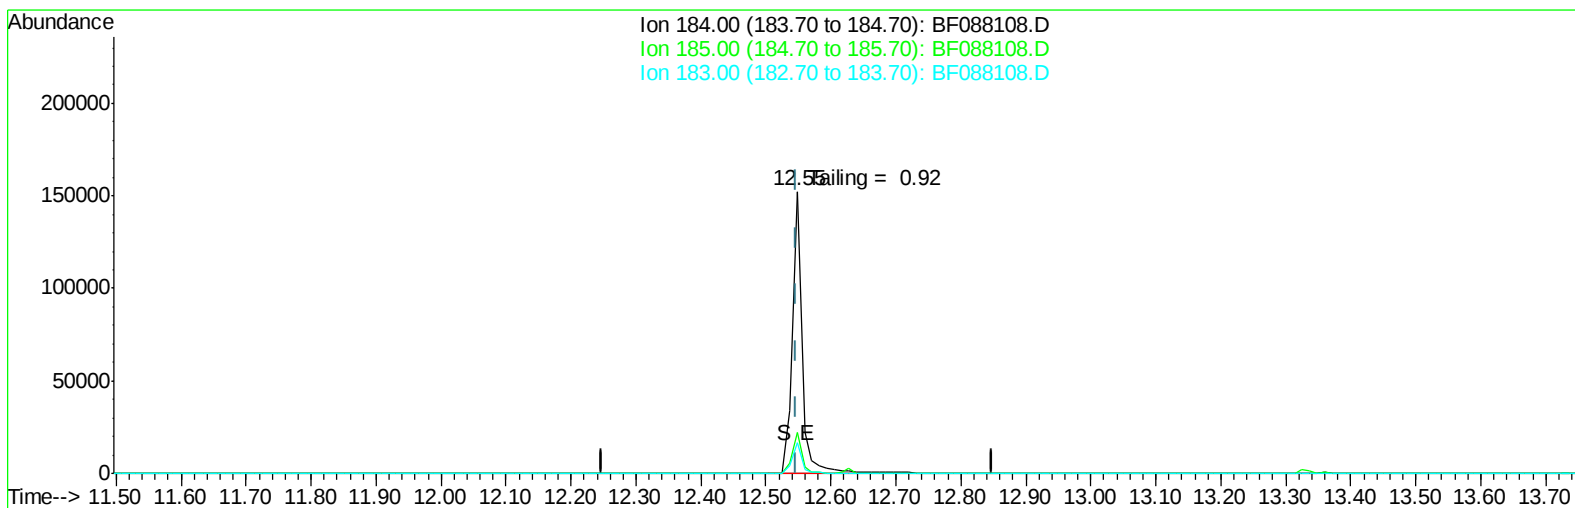

TIC: BF088108.D

(76) Benzidine




12.548min (-0.000) 18455.68ng

response 158927

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	14.63
183.00	11.60	11.12
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF061716\
Data File : BF088108.D
Acq On : 17 Jun 2016 23:15
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 20 07:20:29 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 17 16:09:13 2016
Response via : Initial Calibration

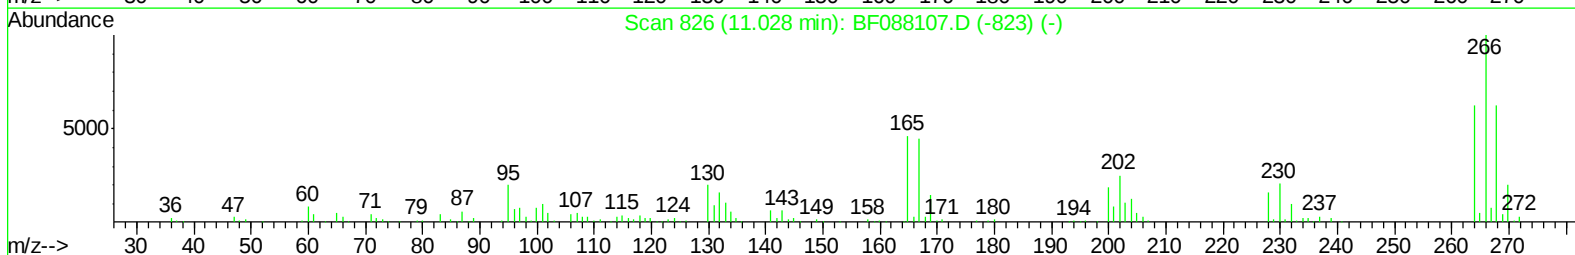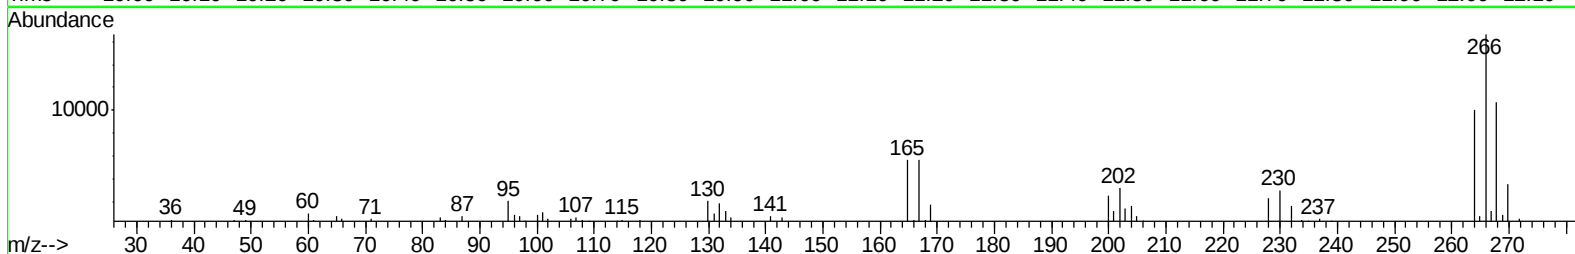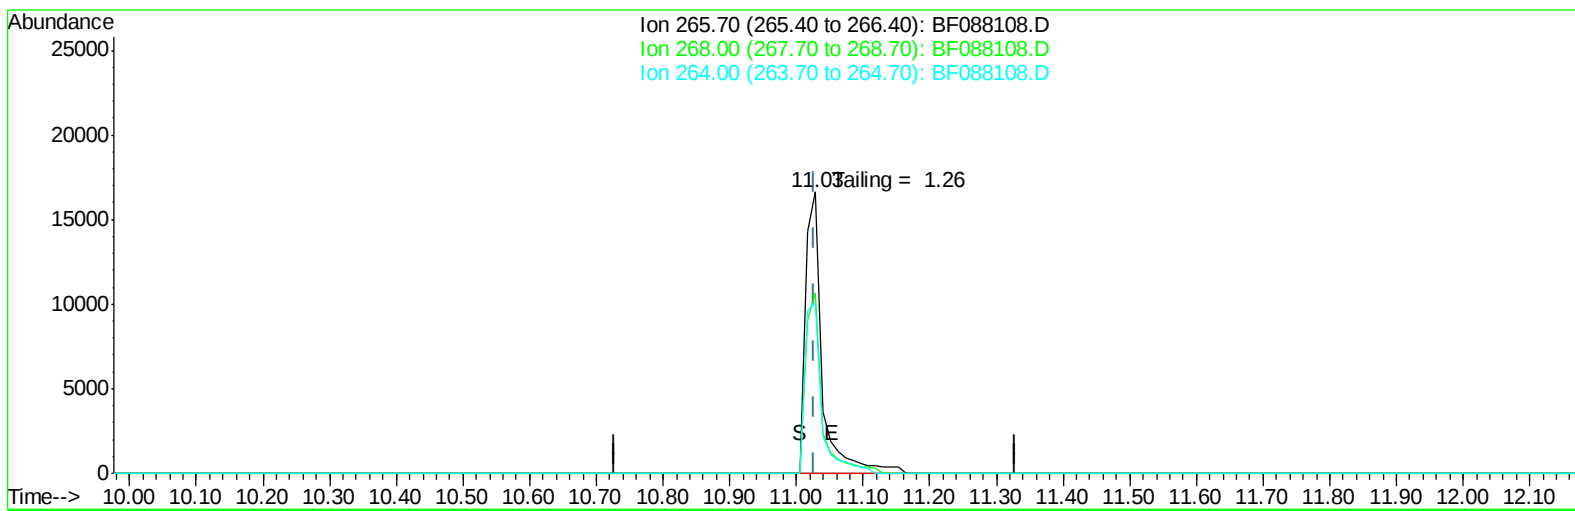

TIC: BF088108.D

(69) Pentachlorophenol (C)

11.028min (-0.000) 0.00ng

response 28932

Ion	Exp%	Act%
265.70	100	100
268.00	66.00	64.33
264.00	62.00	60.61
0.00	0.00	0.00